

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013885.D
 Acq On : 03 Dec 2019 11:47
 Operator : SY/MD
 Sample : K6007-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	82	rVB	278723	270407	12.21%	1.579%
2	1.569	143	149	160	rVB	280788	324032	14.64%	1.892%
3	2.126	314	322	334	rVB	550383	779443	35.21%	4.550%
4	2.737	509	512	515	rBV4	1398	821	0.04%	0.005%
5	2.753	515	517	519	rVB3	799	315	0.01%	0.002%
6	2.830	538	541	544	rBV3	1042	892	0.04%	0.005%
7	2.872	552	554	555	rBV3	793	282	0.01%	0.002%
8	2.923	569	570	571	rVB	961	185	0.01%	0.001%
9	2.933	571	573	575	rBV2	835	505	0.02%	0.003%
10	3.065	611	614	617	rBV3	1147	736	0.03%	0.004%
11	3.081	617	619	623	rVV3	1353	917	0.04%	0.005%
12	3.219	659	662	665	rBV4	1074	866	0.04%	0.005%
13	3.248	669	671	673	rBV3	1134	476	0.02%	0.003%
14	3.293	680	685	687	rBV5	1159	1005	0.05%	0.006%
15	3.315	690	692	695	rBV4	1521	950	0.04%	0.006%
16	3.351	700	703	707	rBV4	1529	945	0.04%	0.006%
17	3.495	744	748	752	rVB7	890	878	0.04%	0.005%
18	3.528	752	758	759	rBV3	1423	1313	0.06%	0.008%
19	3.553	764	766	770	rVB4	1715	906	0.04%	0.005%
20	3.692	806	809	812	rBV5	1184	754	0.03%	0.004%
21	3.737	822	823	824	rBV	539	144	0.01%	0.001%
22	3.769	828	833	837	rVV7	1685	1590	0.07%	0.009%
23	3.785	837	838	842	rVB4	1933	984	0.04%	0.006%
24	3.811	842	846	847	rBV3	772	458	0.02%	0.003%
25	3.868	860	864	867	rBV4	1583	1261	0.06%	0.007%
26	3.920	869	880	908	rBV2	166981	456153	20.60%	2.663%
27	4.235	976	978	980	rBV3	1169	677	0.03%	0.004%
28	4.396	1013	1028	1055	rVB	355788	875736	39.55%	5.112%
29	4.637	1099	1103	1104	rBV4	1274	889	0.04%	0.005%
30	4.717	1125	1128	1134	rVB7	1597	1904	0.09%	0.011%
31	4.785	1146	1149	1150	rBV3	929	467	0.02%	0.003%
32	4.843	1165	1167	1170	rBV3	931	510	0.02%	0.003%
33	4.891	1178	1182	1184	rBV3	1479	1034	0.05%	0.006%
34	4.936	1194	1196	1197	rVB2	891	312	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013885.D
 Acq On : 03 Dec 2019 11:47
 Operator : SY/MD
 Sample : K6007-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.949	1199	1200	1201	rBV	835	254	0.01%	0.001%
36	5.090	1225	1244	1270	rBV2	872302	2214006	100.00%	12.924%
37	5.582	1395	1397	1401	rBV3	1717	1400	0.06%	0.008%
38	5.659	1407	1421	1449	rBV	753153	1489616	67.28%	8.696%
39	6.113	1549	1562	1591	rVB	529560	1048967	47.38%	6.123%
40	6.868	1796	1797	1800	rVB3	1677	617	0.03%	0.004%
41	6.888	1800	1803	1805	rBV3	1498	1123	0.05%	0.007%
42	6.949	1820	1822	1826	rBV5	1386	622	0.03%	0.004%
43	7.026	1834	1846	1868	rBV	266725	473275	21.38%	2.763%
44	7.302	1930	1932	1934	rBV2	1510	676	0.03%	0.004%
45	7.354	1936	1948	1966	rVV	1060461	1806126	81.58%	10.543%
46	7.659	2032	2043	2059	rBV	192230	323258	14.60%	1.887%
47	7.933	2125	2128	2130	rBV4	1927	1680	0.08%	0.010%
48	8.129	2178	2189	2221	rBV2	492301	1041487	47.04%	6.080%
49	8.585	2330	2331	2332	rBV	1147	441	0.02%	0.003%
50	8.891	2413	2426	2446	rBV	1149253	1859575	83.99%	10.855%
51	9.392	2578	2582	2586	rBV4	2001	1714	0.08%	0.010%
52	9.434	2593	2595	2596	rBV2	1377	746	0.03%	0.004%
53	9.730	2685	2687	2689	rBV3	1281	529	0.02%	0.003%
54	10.071	2790	2793	2797	rVB4	1458	963	0.04%	0.006%
55	10.254	2838	2850	2870	rBV	668801	1058911	47.83%	6.181%
56	10.559	2944	2945	2946	rBV	714	217	0.01%	0.001%
57	10.723	2994	2996	2999	rBV3	1331	960	0.04%	0.006%
58	10.762	3004	3008	3009	rBV4	1121	718	0.03%	0.004%
59	10.855	3035	3037	3038	rBV2	1560	703	0.03%	0.004%
60	10.916	3054	3056	3059	rBV3	685	458	0.02%	0.003%
61	11.006	3080	3084	3085	rBV3	1363	861	0.04%	0.005%
62	11.116	3114	3118	3120	rBV4	1419	921	0.04%	0.005%
63	11.141	3123	3126	3131	rVV5	1526	1540	0.07%	0.009%
64	11.190	3138	3141	3143	rBV3	1658	1190	0.05%	0.007%
65	11.209	3145	3147	3149	rBV3	2067	1405	0.06%	0.008%
66	11.289	3160	3172	3189	rBV	967624	1498196	67.67%	8.746%
67	11.575	3259	3261	3264	rBV3	1402	897	0.04%	0.005%
68	11.592	3264	3266	3270	rVB4	1790	1182	0.05%	0.007%
69	11.666	3277	3289	3309	rBV	967859	1555857	70.27%	9.082%
70	12.029	3400	3402	3403	rBV2	1583	678	0.03%	0.004%
71	12.061	3409	3412	3415	rBV3	1793	1432	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013885.D
Acq On : 03 Dec 2019 11:47
Operator : SY/MD
Sample : K6007-23
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

72	12.109	3425	3427	3429	rBV3	1047	595	0.03%	0.003%
73	12.357	3502	3504	3507	rBV3	1160	507	0.02%	0.003%
74	12.392	3514	3515	3516	rBV	859	275	0.01%	0.002%
75	12.582	3570	3574	3577	rBV5	1384	856	0.04%	0.005%
76	12.637	3589	3591	3592	rBV2	1049	420	0.02%	0.002%
77	12.662	3596	3599	3603	rBV3	1352	1099	0.05%	0.006%
78	12.685	3603	3606	3607	rBV3	2369	1100	0.05%	0.006%
79	12.887	3667	3669	3671	rBV3	1581	654	0.03%	0.004%
80	13.167	3753	3756	3759	rBV5	2507	1688	0.08%	0.010%
81	14.530	4178	4180	4184	rBV4	1723	1397	0.06%	0.008%


Sum of corrected areas: 17130539

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013885.D
Acq On : 03 Dec 2019 11:47
Operator : SY/MD
Sample : K6007-23
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

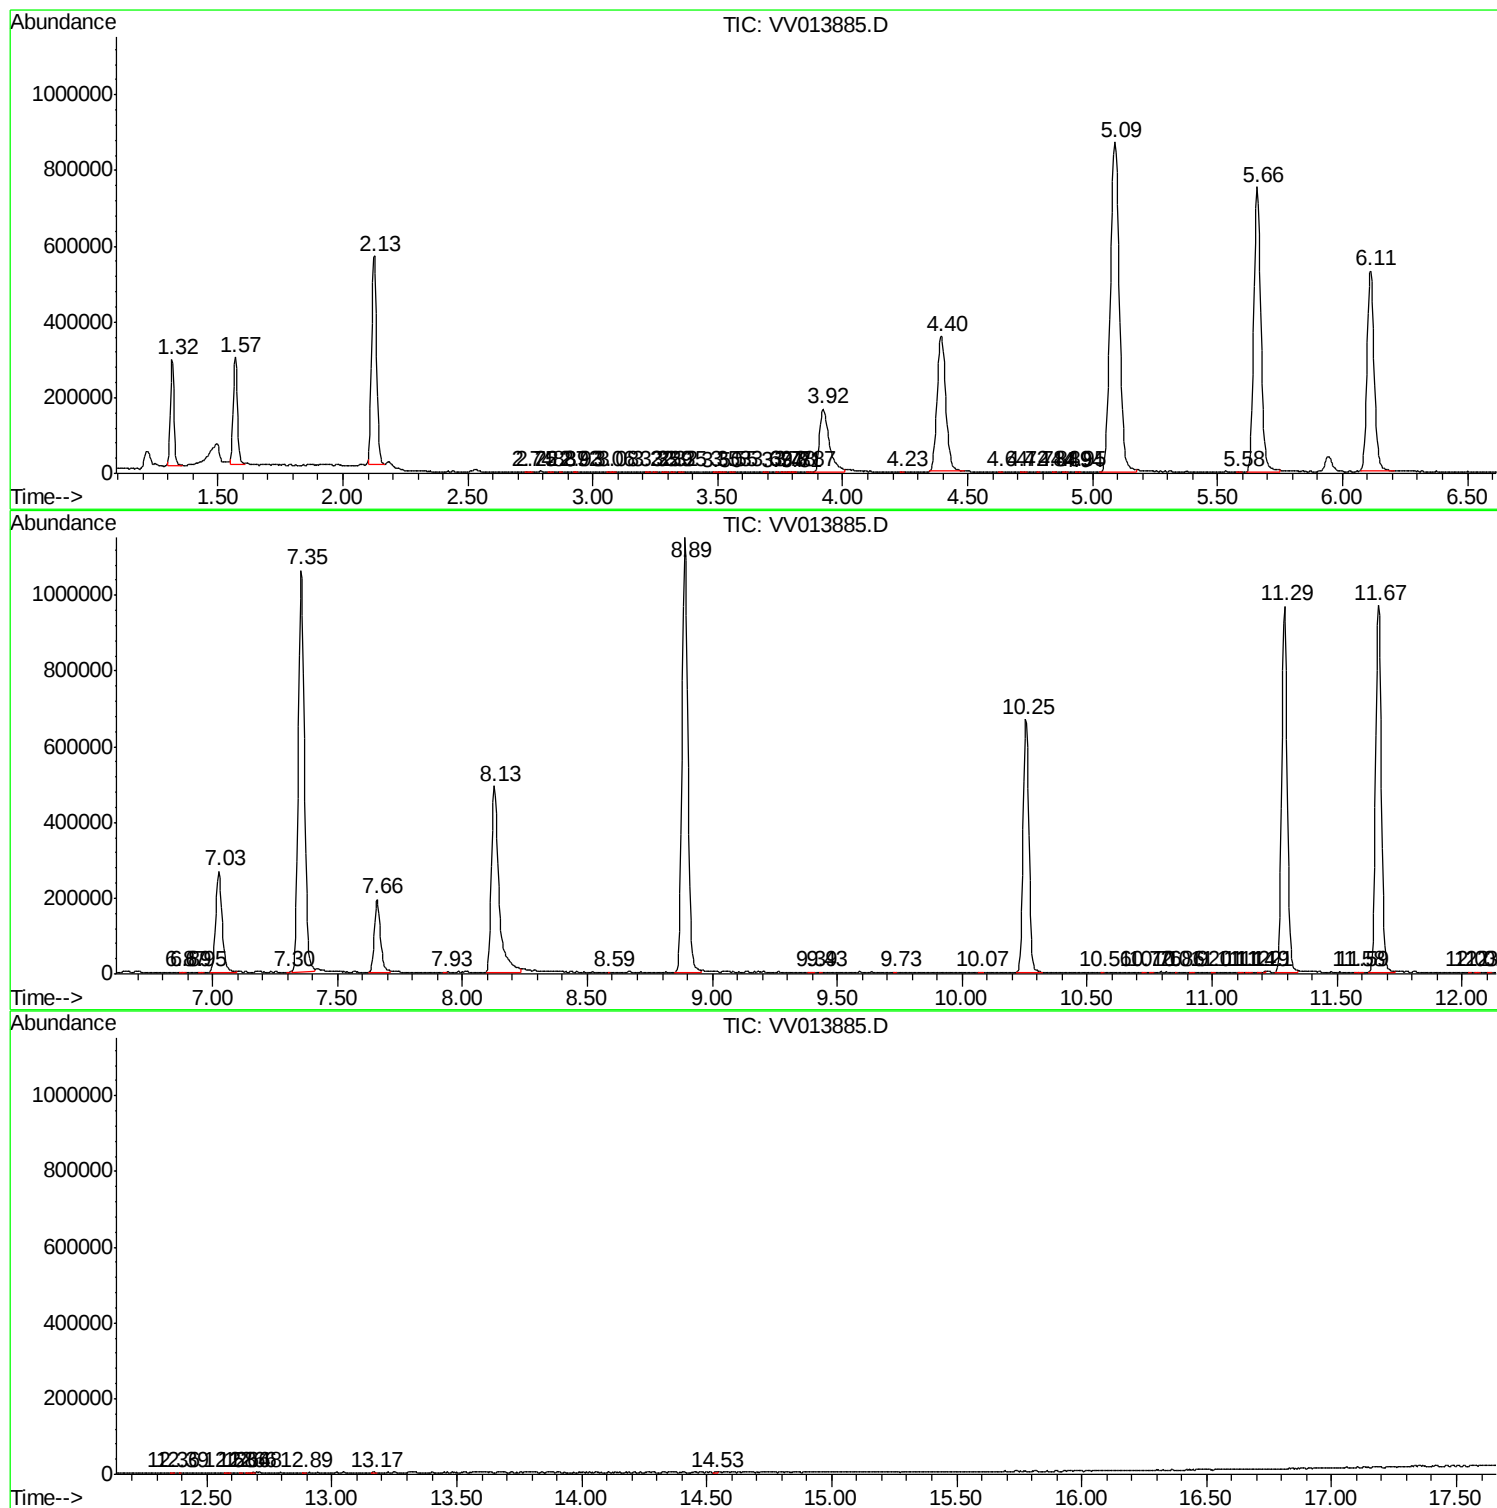

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013885.D
Acq On : 03 Dec 2019 11:47
Operator : SY/MD
Sample : K6007-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120319\
Data File : VV013885.D
Acq On : 03 Dec 2019 11:47
Operator : SY/MD
Sample : K6007-23
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc