

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013887.D
 Acq On : 03 Dec 2019 12:36
 Operator : SY/MD
 Sample : K6089-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.216	32	39	46	rBV2	42719	71189	3.13%	0.409%
2	1.315	64	70	79	rVB	302223	286004	12.58%	1.643%
3	1.566	142	148	163	rVB	297480	345940	15.22%	1.988%
4	2.122	313	321	334	rVB	604386	837998	36.87%	4.815%
5	2.527	438	447	458	rVB3	8805	16688	0.73%	0.096%
6	2.595	466	468	470	rBV2	913	494	0.02%	0.003%
7	2.714	503	505	509	rVB4	1551	818	0.04%	0.005%
8	2.749	514	516	518	rBV3	1373	753	0.03%	0.004%
9	2.849	543	547	548	rBV2	712	468	0.02%	0.003%
10	2.923	567	570	572	rBV3	1120	696	0.03%	0.004%
11	2.984	588	589	594	rVB4	1554	823	0.04%	0.005%
12	3.013	595	598	603	rVB6	1491	1341	0.06%	0.008%
13	3.061	611	613	615	rBV3	859	538	0.02%	0.003%
14	3.135	633	636	641	rVB5	940	925	0.04%	0.005%
15	3.161	641	644	646	rBV2	939	513	0.02%	0.003%
16	3.206	655	658	659	rBV3	794	519	0.02%	0.003%
17	3.360	703	706	710	rBV5	962	758	0.03%	0.004%
18	3.386	710	714	717	rBV6	1187	1191	0.05%	0.007%
19	3.479	739	743	747	rVB6	1541	1247	0.05%	0.007%
20	3.511	747	753	754	rBV5	1771	1488	0.07%	0.009%
21	3.534	758	760	764	rBV4	1142	746	0.03%	0.004%
22	3.585	774	776	778	rBV3	1597	825	0.04%	0.005%
23	3.630	785	790	793	rBV7	1772	1131	0.05%	0.006%
24	3.650	793	796	800	rBV2	834	771	0.03%	0.004%
25	3.711	811	815	818	rBV4	1229	992	0.04%	0.006%
26	3.756	825	829	832	rBV3	1167	905	0.04%	0.005%
27	3.807	843	845	846	rVB2	1600	481	0.02%	0.003%
28	3.855	858	860	863	rVB4	1102	536	0.02%	0.003%
29	3.920	868	880	924	rBV	170416	491031	21.60%	2.821%
30	4.193	962	965	968	rVB5	1990	1179	0.05%	0.007%
31	4.248	977	982	984	rBV6	1775	1842	0.08%	0.011%
32	4.270	987	989	995	rVB6	1407	1106	0.05%	0.006%
33	4.309	997	1001	1005	rBV5	1563	1520	0.07%	0.009%
34	4.392	1009	1027	1048	rBV	385558	926417	40.76%	5.323%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013887.D
 Acq On : 03 Dec 2019 12:36
 Operator : SY/MD
 Sample : K6089-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.730	1130	1132	1135	rVB3	1532	730	0.03%	0.004%
36	4.749	1135	1138	1139	rBV2	1085	605	0.03%	0.003%
37	4.868	1173	1175	1178	rVB3	1987	924	0.04%	0.005%
38	4.907	1183	1187	1188	rBV4	1451	1173	0.05%	0.007%
39	4.968	1203	1206	1208	rBV3	1018	598	0.03%	0.003%
40	4.994	1209	1214	1219	rVB7	1692	1761	0.08%	0.010%
41	5.087	1223	1243	1268	rBV2	911094	2272839	100.00%	13.059%
42	5.511	1373	1375	1382	rVV7	1667	1938	0.09%	0.011%
43	5.656	1407	1420	1437	rBV	733002	1431814	63.00%	8.227%
44	6.109	1548	1561	1586	rBV	506981	1012632	44.55%	5.818%
45	6.373	1641	1643	1645	rVV3	1089	675	0.03%	0.004%
46	6.473	1669	1674	1675	rBV3	1100	838	0.04%	0.005%
47	6.505	1681	1684	1686	rBV3	1558	1024	0.05%	0.006%
48	6.656	1719	1731	1734	rBV3	4122	6424	0.28%	0.037%
49	6.878	1795	1800	1802	rBV5	1555	1320	0.06%	0.008%
50	6.891	1802	1804	1808	rVB3	1191	798	0.04%	0.005%
51	6.939	1814	1819	1822	rVB6	891	711	0.03%	0.004%
52	6.958	1822	1825	1826	rBV	1073	532	0.02%	0.003%
53	6.968	1826	1828	1830	rBV3	1192	563	0.02%	0.003%
54	7.023	1834	1845	1867	rBV	264712	471756	20.76%	2.711%
55	7.167	1888	1890	1893	rBV3	1513	1043	0.05%	0.006%
56	7.225	1905	1908	1912	rBV5	1639	1417	0.06%	0.008%
57	7.244	1912	1914	1915	rBV2	1187	472	0.02%	0.003%
58	7.293	1927	1929	1934	rVB4	1168	674	0.03%	0.004%
59	7.354	1935	1948	1967	rBV	1011457	1744573	76.76%	10.024%
60	7.659	2032	2043	2059	rBV	185331	313140	13.78%	1.799%
61	7.868	2105	2108	2109	rBV3	1368	744	0.03%	0.004%
62	7.945	2129	2132	2133	rBV3	1274	800	0.04%	0.005%
63	8.129	2178	2189	2224	rBV2	472857	1003407	44.15%	5.765%
64	8.537	2314	2316	2320	rBV4	1229	604	0.03%	0.003%
65	8.566	2323	2325	2328	rBV3	2266	1303	0.06%	0.007%
66	8.723	2371	2374	2377	rBV4	2382	1266	0.06%	0.007%
67	8.807	2396	2400	2402	rBV4	1569	1062	0.05%	0.006%
68	8.891	2413	2426	2447	rBV	1069139	1714217	75.42%	9.849%
69	9.106	2491	2493	2496	rBV3	1735	863	0.04%	0.005%
70	9.177	2512	2515	2517	rBV4	1449	1312	0.06%	0.008%
71	9.248	2533	2537	2543	rVB7	1615	1494	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013887.D
 Acq On : 03 Dec 2019 12:36
 Operator : SY/MD
 Sample : K6089-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	9.357	2569	2571	2573	rBV3	1224	805	0.04%	0.005%
73	9.386	2577	2580	2583	rVV4	1579	1277	0.06%	0.007%
74	9.411	2586	2588	2592	rBV4	1319	902	0.04%	0.005%
75	9.473	2604	2607	2608	rBV2	835	494	0.02%	0.003%
76	9.540	2626	2628	2632	rBV5	1005	586	0.03%	0.003%
77	9.563	2632	2635	2636	rBV3	1198	547	0.02%	0.003%
78	9.614	2647	2651	2655	rBV4	1676	1497	0.07%	0.009%
79	9.749	2689	2693	2694	rBV2	1214	802	0.04%	0.005%
80	9.974	2760	2763	2765	rBV3	1922	1045	0.05%	0.006%
81	10.029	2779	2780	2785	rVB4	1402	733	0.03%	0.004%
82	10.080	2791	2796	2800	rVB6	1189	1122	0.05%	0.006%
83	10.109	2800	2805	2807	rBV5	1449	1318	0.06%	0.008%
84	10.190	2828	2830	2833	rVB2	1308	767	0.03%	0.004%
85	10.209	2833	2836	2838	rBV4	1131	800	0.04%	0.005%
86	10.254	2838	2850	2869	rBV	702701	1128802	49.66%	6.486%
87	10.617	2960	2963	2964	rBV2	2250	1384	0.06%	0.008%
88	10.659	2974	2976	2979	rBV3	1134	560	0.02%	0.003%
89	10.710	2989	2992	2994	rBV3	2186	1512	0.07%	0.009%
90	10.800	3016	3020	3021	rBV4	1365	739	0.03%	0.004%
91	10.958	3064	3069	3072	rBV6	2378	2795	0.12%	0.016%
92	11.022	3086	3089	3090	rBV3	1364	736	0.03%	0.004%
93	11.061	3099	3101	3102	rBV2	1420	782	0.03%	0.004%
94	11.164	3131	3133	3134	rBV2	1436	673	0.03%	0.004%
95	11.289	3160	3172	3194	rBV	999351	1559768	68.63%	8.962%
96	11.585	3262	3264	3266	rVB2	1434	512	0.02%	0.003%
97	11.665	3277	3289	3309	rBV	1080592	1691636	74.43%	9.720%
98	12.138	3432	3436	3438	rBV5	2455	2005	0.09%	0.012%
99	12.222	3458	3462	3464	rBV3	1821	1354	0.06%	0.008%
100	12.849	3654	3657	3658	rBV2	1171	683	0.03%	0.004%


Sum of corrected areas: 17404555

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013887.D
Acq On : 03 Dec 2019 12:36
Operator : SY/MD
Sample : K6089-22
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

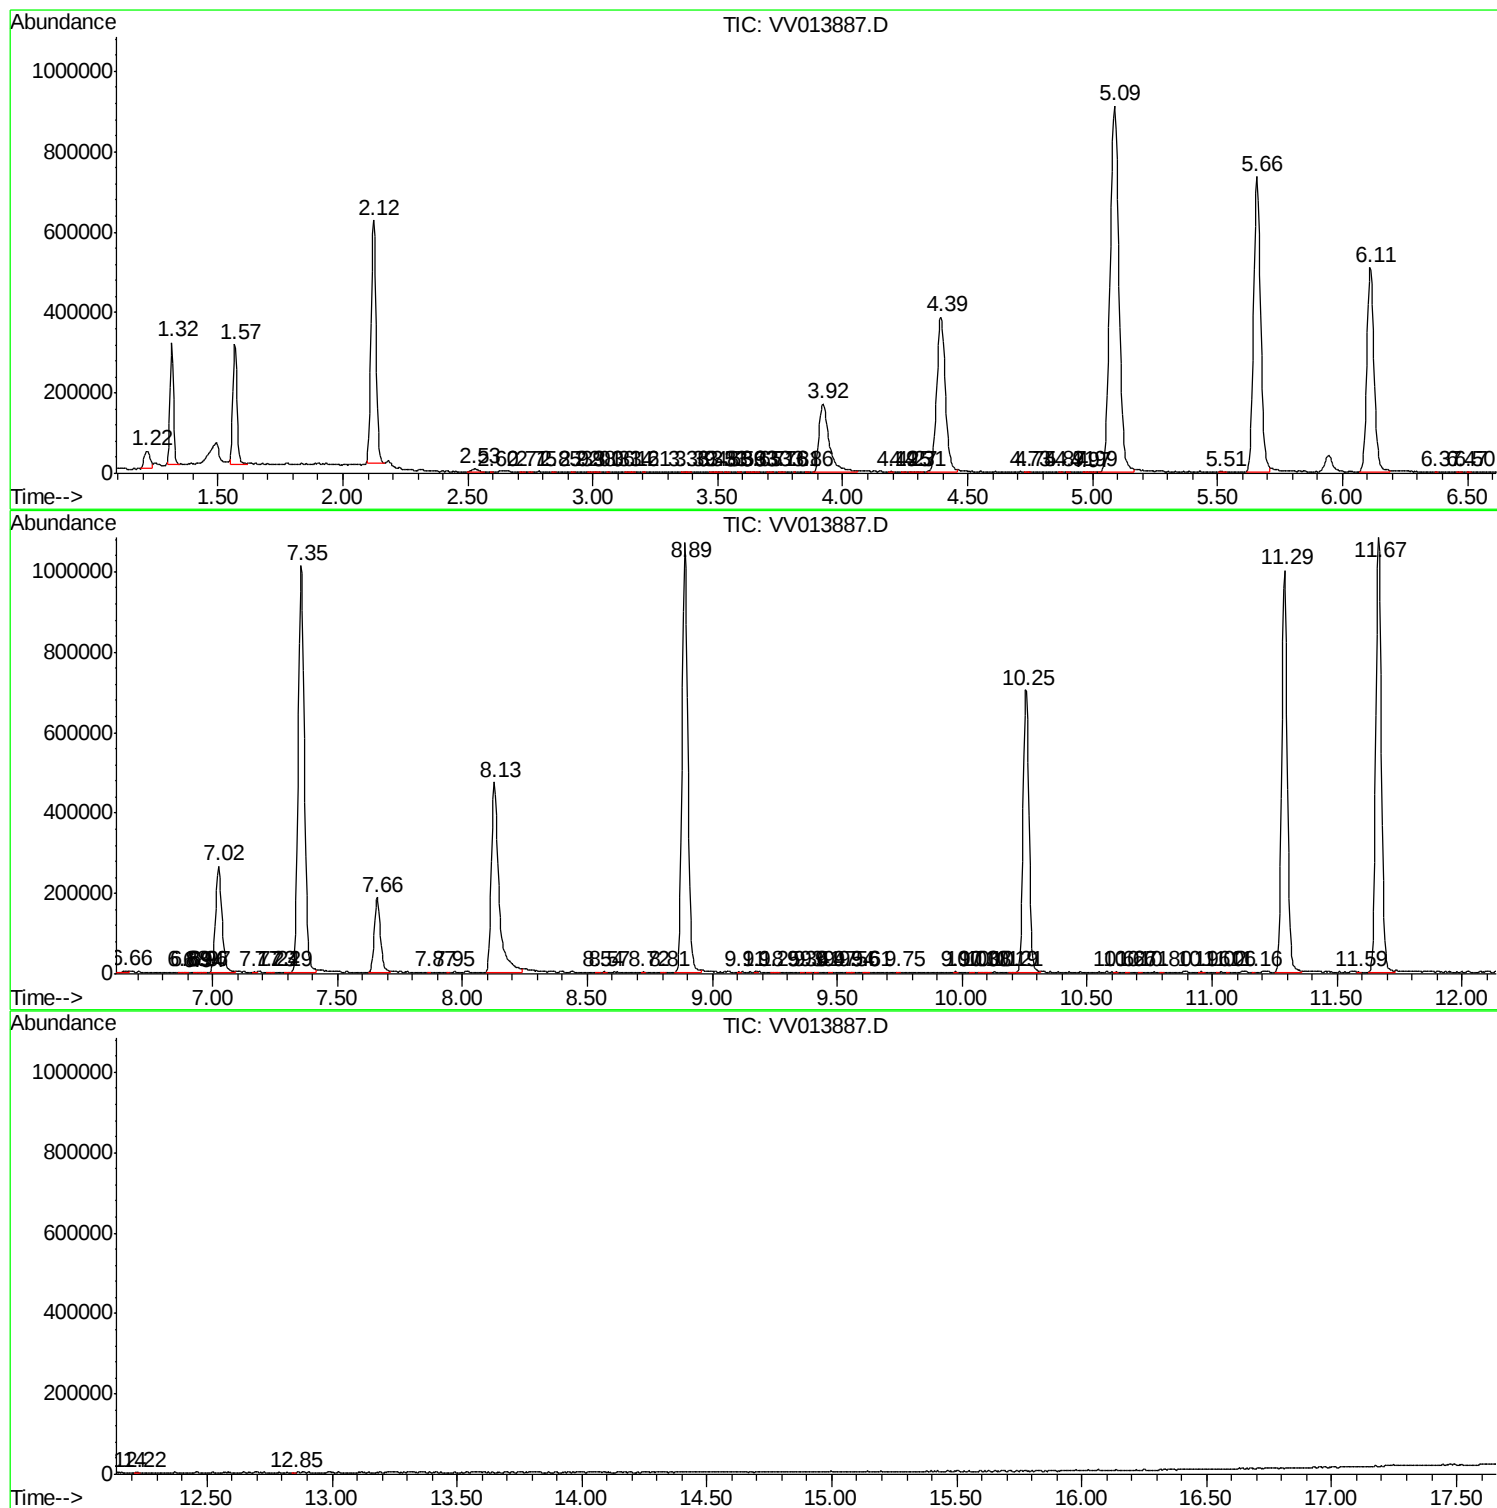

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013887.D
Acq On : 03 Dec 2019 12:36
Operator : SY/MD
Sample : K6089-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120319\
Data File : VV013887.D
Acq On : 03 Dec 2019 12:36
Operator : SY/MD
Sample : K6089-22
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc