

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013891.D
 Acq On : 03 Dec 2019 14:15
 Operator : SY/MD
 Sample : K6086-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLY8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	33	41	47	rBV2	39197	63920	2.77%	0.345%
2	1.319	64	71	79	rBV	270642	268916	11.64%	1.452%
3	1.573	143	150	164	rVB	287207	340269	14.72%	1.838%
4	2.126	313	322	335	rBV	578774	800214	34.63%	4.322%
5	2.306	371	378	392	rVB3	11016	21245	0.92%	0.115%
6	2.454	419	424	429	rBV8	1790	2195	0.09%	0.012%
7	2.573	459	461	465	rVB4	1425	1046	0.05%	0.006%
8	2.907	561	565	568	rVB5	1710	1265	0.05%	0.007%
9	2.933	568	573	576	rBV6	1464	1124	0.05%	0.006%
10	2.952	576	579	585	rBV5	1240	1450	0.06%	0.008%
11	2.987	585	590	593	rBV7	1158	1425	0.06%	0.008%
12	3.061	609	613	618	rVB7	1303	1165	0.05%	0.006%
13	3.219	658	662	667	rVV7	1351	1499	0.06%	0.008%
14	3.447	729	733	734	rBV4	1745	1066	0.05%	0.006%
15	3.589	772	777	780	rBV5	1457	943	0.04%	0.005%
16	3.614	780	785	788	rVB6	1766	1631	0.07%	0.009%
17	3.679	801	805	808	rBV4	1497	1002	0.04%	0.005%
18	3.923	867	881	915	rBV	186687	494395	21.39%	2.670%
19	4.267	985	988	992	rVB4	1278	1105	0.05%	0.006%
20	4.396	1011	1028	1052	rVV2	387510	924735	40.02%	4.995%
21	4.585	1082	1087	1090	rBV6	1392	1059	0.05%	0.006%
22	4.814	1155	1158	1161	rBV4	1421	995	0.04%	0.005%
23	5.090	1224	1244	1258	rBV2	906811	2310917	100.00%	12.481%
24	5.328	1315	1318	1323	rVV6	1340	1233	0.05%	0.007%
25	5.357	1325	1327	1334	rVB7	1979	1516	0.07%	0.008%
26	5.431	1346	1350	1354	rVB6	1148	1066	0.05%	0.006%
27	5.463	1358	1360	1365	rVB5	1873	1403	0.06%	0.008%
28	5.486	1365	1367	1372	rVB5	1686	1450	0.06%	0.008%
29	5.515	1372	1376	1378	rBV4	2859	1939	0.08%	0.010%
30	5.659	1405	1421	1442	rBV	691400	1365142	59.07%	7.373%
31	5.942	1498	1509	1527	rBV3	22534	52387	2.27%	0.283%
32	6.113	1547	1562	1585	rBV	504396	1017792	44.04%	5.497%
33	6.215	1592	1594	1597	rBV4	1789	991	0.04%	0.005%
34	6.547	1689	1697	1702	rVB9	1833	2782	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013891.D
 Acq On : 03 Dec 2019 14:15
 Operator : SY/MD
 Sample : K6086-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLY8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.611	1712	1717	1721	rBV6	2739	3024	0.13%	0.016%
36	6.881	1796	1801	1803	rBV4	1496	1365	0.06%	0.007%
37	6.923	1812	1814	1816	rBV3	1731	963	0.04%	0.005%
38	7.026	1831	1846	1865	rBV	275442	490901	21.24%	2.651%
39	7.177	1888	1893	1894	rBV4	2109	1803	0.08%	0.010%
40	7.354	1932	1948	1963	rVV	1082820	1853265	80.20%	10.010%
41	7.428	1965	1971	1987	rVB	53629	99825	4.32%	0.539%
42	7.659	2030	2043	2063	rBV	201522	346044	14.97%	1.869%
43	7.752	2068	2072	2073	rBV4	2641	1786	0.08%	0.010%
44	7.974	2137	2141	2146	rBV7	4035	4593	0.20%	0.025%
45	8.058	2164	2167	2171	rBV5	1362	1086	0.05%	0.006%
46	8.125	2176	2188	2215	rBV2	600108	1165003	50.41%	6.292%
47	8.421	2277	2280	2284	rBV5	2480	1782	0.08%	0.010%
48	8.637	2343	2347	2348	rBV4	1902	1252	0.05%	0.007%
49	8.785	2385	2393	2394	rBV7	3043	3734	0.16%	0.020%
50	8.891	2414	2426	2443	rBV	1181614	1892321	81.89%	10.220%
51	9.112	2493	2495	2498	rVV4	2002	1231	0.05%	0.007%
52	9.180	2507	2516	2527	rVB4	13831	24755	1.07%	0.134%
53	9.309	2552	2556	2559	rBV6	2345	1882	0.08%	0.010%
54	9.585	2631	2642	2643	rBV9	6954	8113	0.35%	0.044%
55	9.691	2671	2675	2677	rBV4	1329	1080	0.05%	0.006%
56	9.977	2761	2764	2765	rBV3	2029	1124	0.05%	0.006%
57	10.157	2817	2820	2823	rBV5	1701	1380	0.06%	0.007%
58	10.254	2838	2850	2872	rVB	851502	1324870	57.33%	7.156%
59	10.373	2883	2887	2892	rBV6	1972	2350	0.10%	0.013%
60	10.424	2894	2903	2912	rVB9	6166	11311	0.49%	0.061%
61	10.524	2930	2934	2939	rVB8	2274	1982	0.09%	0.011%
62	10.563	2943	2946	2948	rBV4	1717	1154	0.05%	0.006%
63	10.643	2969	2971	2977	rVB6	1558	954	0.04%	0.005%
64	10.881	3043	3045	3048	rBV4	2180	1093	0.05%	0.006%
65	10.916	3054	3056	3060	rVB4	2251	1767	0.08%	0.010%
66	10.955	3065	3068	3069	rBV3	1895	1054	0.05%	0.006%
67	11.016	3085	3087	3092	rVB6	1724	960	0.04%	0.005%
68	11.219	3139	3150	3155	rBV6	6977	14007	0.61%	0.076%
69	11.289	3160	3172	3190	rBV	938901	1449037	62.70%	7.826%
70	11.498	3233	3237	3240	rBV5	2718	2349	0.10%	0.013%
71	11.569	3252	3259	3269	rVB3	16135	25470	1.10%	0.138%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013891.D
 Acq On : 03 Dec 2019 14:15
 Operator : SY/MD
 Sample : K6086-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLY8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.665	3276	3289	3310	rBV	1155471	1819768	78.75%	9.829%
73	11.788	3319	3327	3338	rVB	29398	48136	2.08%	0.260%
74	12.061	3409	3412	3414	rBV5	1854	1086	0.05%	0.006%
75	12.373	3504	3509	3513	rBV7	2425	2646	0.11%	0.014%
76	12.399	3513	3517	3520	rVV5	1756	1299	0.06%	0.007%
77	12.450	3530	3533	3535	rBV3	2632	1660	0.07%	0.009%
78	12.701	3604	3611	3618	rVB3	2562	3923	0.17%	0.021%
79	12.733	3618	3621	3623	rBV4	1896	1014	0.04%	0.005%
80	12.765	3628	3631	3633	rBV3	2006	1371	0.06%	0.007%
81	12.874	3661	3665	3668	rVB4	2311	1659	0.07%	0.009%
82	12.926	3680	3681	3689	rVB7	2970	2783	0.12%	0.015%
83	13.048	3716	3719	3722	rBV4	1798	1242	0.05%	0.007%
84	13.122	3740	3742	3746	rVB5	2157	1371	0.06%	0.007%
85	13.183	3758	3761	3763	rBV4	2668	1446	0.06%	0.008%
86	13.231	3773	3776	3779	rVB5	2067	1185	0.05%	0.006%
87	13.283	3788	3792	3793	rBV3	1836	1156	0.05%	0.006%
88	13.312	3798	3801	3807	rVB7	3125	2565	0.11%	0.014%
89	13.511	3860	3863	3865	rBV4	1548	1121	0.05%	0.006%
90	13.550	3865	3875	3891	rVB	93904	160670	6.95%	0.868%
91	13.672	3909	3913	3919	rVB6	3157	3131	0.14%	0.017%
92	13.746	3931	3936	3939	rBV7	2607	1866	0.08%	0.010%
93	14.148	4058	4061	4066	rBV6	1404	1333	0.06%	0.007%
94	14.196	4074	4076	4079	rBV4	1437	1057	0.05%	0.006%
95	14.460	4156	4158	4162	rVB5	2335	1401	0.06%	0.008%
96	14.627	4204	4210	4212	rBV6	3461	3222	0.14%	0.017%
97	14.833	4272	4274	4278	rBV4	1790	1044	0.05%	0.006%
98	14.890	4289	4292	4295	rBV4	1979	1075	0.05%	0.006%
99	15.392	4443	4448	4449	rBV4	2897	2571	0.11%	0.014%
100	15.562	4495	4501	4505	rBV8	2998	4255	0.18%	0.023%


Sum of corrected areas: 18515008

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013891.D
Acq On : 03 Dec 2019 14:15
Operator : SY/MD
Sample : K6086-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BFLY8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

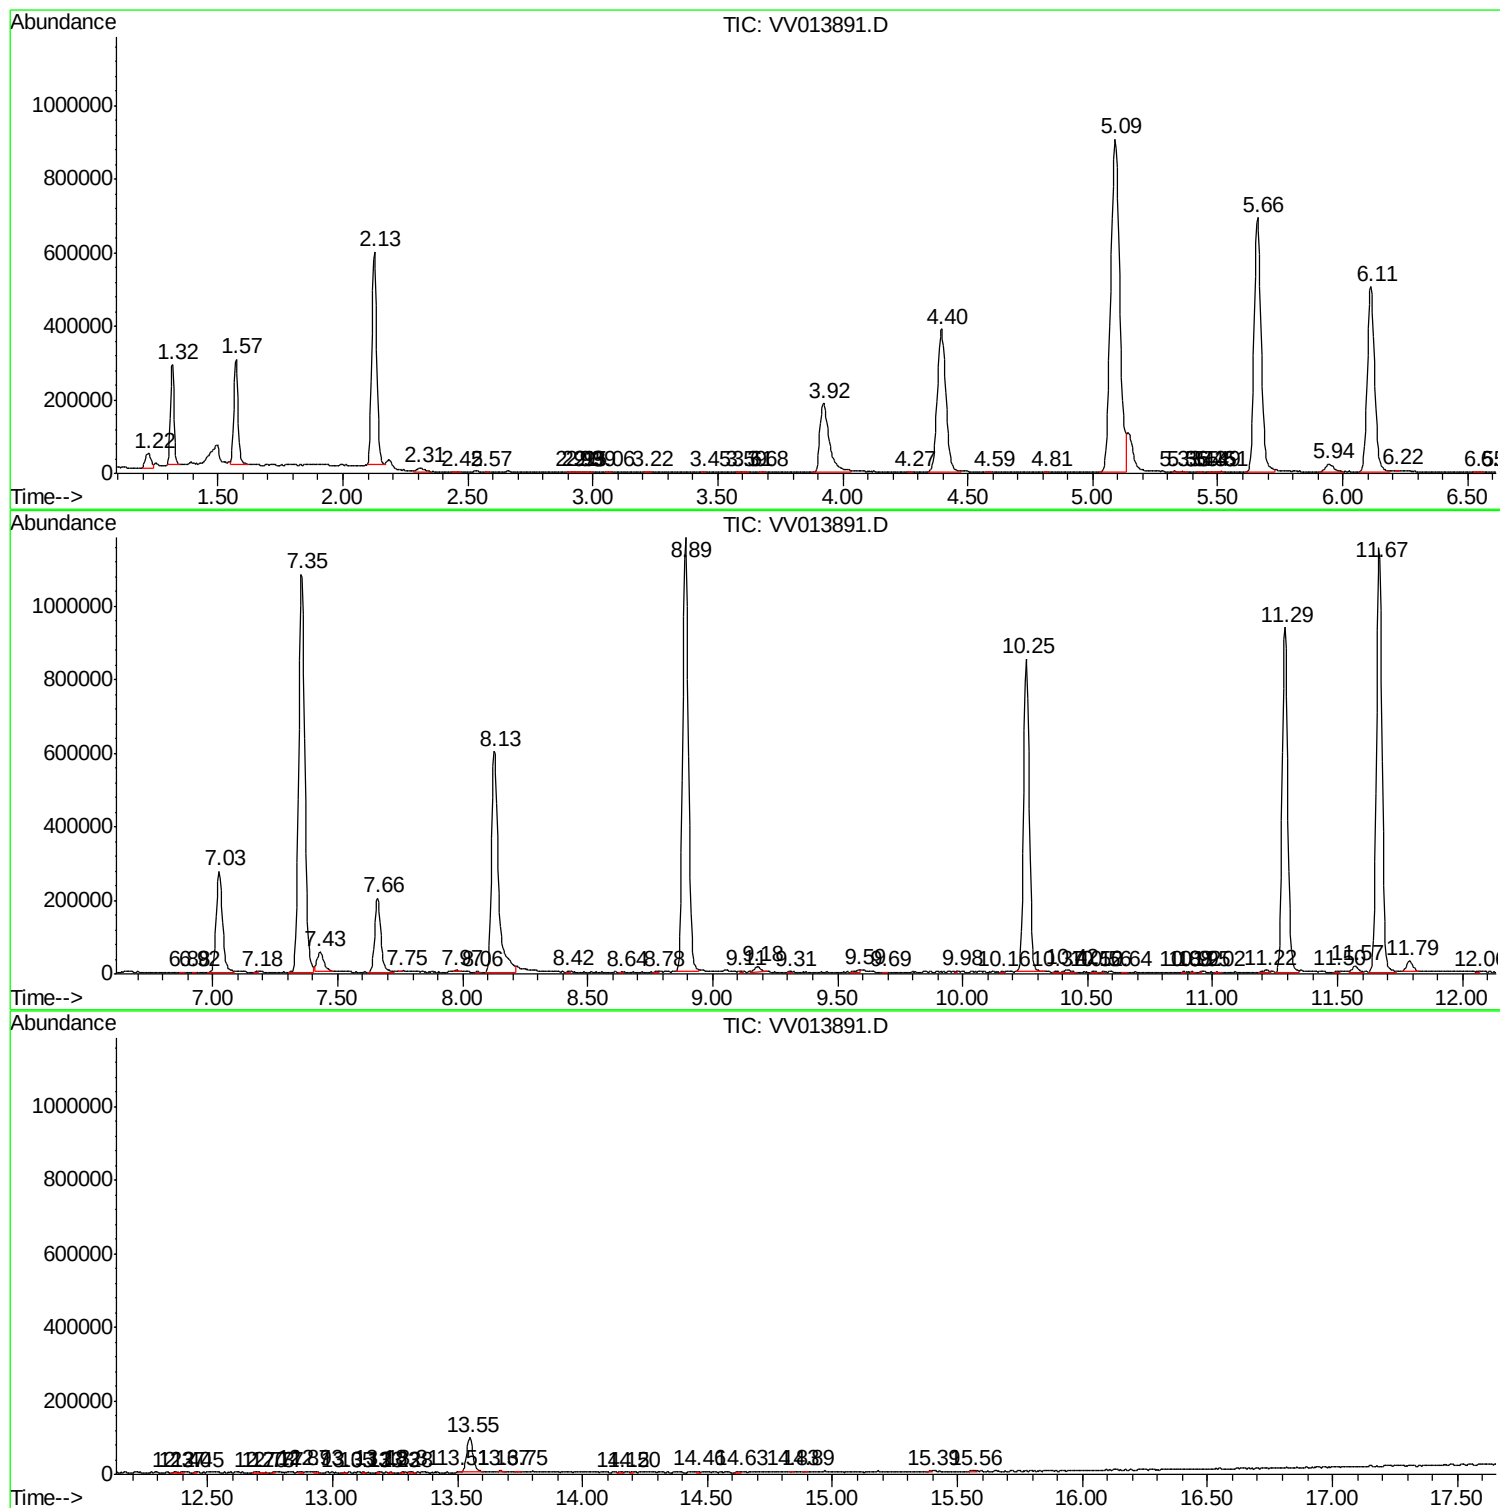

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013891.D
Acq On : 03 Dec 2019 14:15
Operator : SY/MD
Sample : K6086-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLY8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120319\
Data File : VV013891.D
Acq On : 03 Dec 2019 14:15
Operator : SY/MD
Sample : K6086-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFLY8

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc