

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013892.D
 Acq On : 03 Dec 2019 14:39
 Operator : SY/MD
 Sample : K6086-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	80	rVB	305331	297946	13.50%	1.768%
2	1.573	144	150	158	rVB	278172	315123	14.28%	1.870%
3	2.126	314	322	335	rVB	551726	764320	34.63%	4.535%
4	2.868	550	553	554	rBV2	1023	595	0.03%	0.004%
5	2.965	580	583	586	rBV3	1394	1225	0.06%	0.007%
6	3.039	603	606	608	rBV4	1055	659	0.03%	0.004%
7	3.074	615	617	620	rBV3	688	397	0.02%	0.002%
8	3.090	620	622	629	rVB9	1159	1135	0.05%	0.007%
9	3.119	629	631	632	rBV2	639	287	0.01%	0.002%
10	3.261	673	675	677	rBV4	738	361	0.02%	0.002%
11	3.299	685	687	688	rBV2	574	301	0.01%	0.002%
12	3.344	699	701	704	rBV2	612	336	0.02%	0.002%
13	3.364	704	707	708	rBV3	603	325	0.01%	0.002%
14	3.409	718	721	722	rBV3	1404	645	0.03%	0.004%
15	3.560	763	768	769	rBV4	866	740	0.03%	0.004%
16	3.592	776	778	779	rBV2	1302	533	0.02%	0.003%
17	3.611	782	784	787	rVB4	1786	990	0.04%	0.006%
18	3.676	802	804	806	rVB3	1185	452	0.02%	0.003%
19	3.704	808	813	816	rBV7	1039	885	0.04%	0.005%
20	3.740	821	824	827	rVB2	1281	913	0.04%	0.005%
21	3.766	827	832	834	rBV4	1881	1608	0.07%	0.010%
22	3.872	864	865	866	rBV	530	167	0.01%	0.001%
23	3.881	866	868	869	rBV2	711	229	0.01%	0.001%
24	3.923	870	881	902	rBV	169756	443530	20.09%	2.632%
25	4.296	996	997	999	rBV2	943	529	0.02%	0.003%
26	4.393	1013	1027	1053	rVB	367636	871590	39.49%	5.172%
27	4.794	1150	1152	1153	rBV2	812	220	0.01%	0.001%
28	4.888	1177	1181	1185	rBV7	950	1062	0.05%	0.006%
29	4.929	1193	1194	1196	rBV2	682	292	0.01%	0.002%
30	4.962	1200	1204	1208	rBV5	1692	1550	0.07%	0.009%
31	4.981	1208	1210	1211	rBV2	1172	480	0.02%	0.003%
32	5.090	1224	1244	1270	rBV2	870194	2207194	100.00%	13.097%
33	5.409	1340	1343	1345	rBV2	1509	1070	0.05%	0.006%
34	5.505	1371	1373	1375	rBV4	1578	763	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013892.D
 Acq On : 03 Dec 2019 14:39
 Operator : SY/MD
 Sample : K6086-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.659	1408	1421	1448	rBV	713503	1403742	63.60%	8.329%
36	5.946	1499	1510	1522	rBV3	24866	54588	2.47%	0.324%
37	6.113	1549	1562	1581	rBV	493391	986936	44.71%	5.856%
38	6.412	1651	1655	1659	rBV6	2400	2724	0.12%	0.016%
39	6.791	1771	1773	1775	rBV2	1056	448	0.02%	0.003%
40	6.807	1775	1778	1779	rBV3	954	438	0.02%	0.003%
41	6.849	1788	1791	1792	rBV3	1711	868	0.04%	0.005%
42	6.949	1820	1822	1825	rVB4	1175	527	0.02%	0.003%
43	6.968	1825	1828	1832	rBV5	1745	1425	0.06%	0.008%
44	7.026	1833	1846	1864	rBV	265949	479642	21.73%	2.846%
45	7.254	1913	1917	1921	rBV7	2108	2329	0.11%	0.014%
46	7.354	1936	1948	1968	rBV	992334	1724257	78.12%	10.231%
47	7.659	2032	2043	2061	rBV2	193422	333162	15.09%	1.977%
48	8.125	2178	2188	2221	rBV2	543074	1057716	47.92%	6.276%
49	8.730	2374	2376	2378	rBV2	1151	685	0.03%	0.004%
50	8.891	2415	2426	2445	rBV	1078659	1719095	77.89%	10.201%
51	9.444	2595	2598	2601	rBV5	2135	1647	0.07%	0.010%
52	9.566	2634	2636	2640	rVB4	1893	1275	0.06%	0.008%
53	9.765	2696	2698	2699	rBV2	1622	668	0.03%	0.004%
54	10.254	2839	2850	2866	rBV	751911	1172842	53.14%	6.959%
55	10.604	2955	2959	2964	rBV7	1992	2098	0.10%	0.012%
56	11.289	3160	3172	3190	rBV	898174	1409226	63.85%	8.362%
57	11.666	3277	3289	3308	rBV	981919	1570860	71.17%	9.321%
58	12.264	3474	3475	3479	rBV3	1553	913	0.04%	0.005%
59	12.698	3604	3610	3611	rBV5	2294	2134	0.10%	0.013%
60	12.739	3620	3623	3625	rBV3	1370	1026	0.05%	0.006%
61	13.238	3775	3778	3781	rBV3	1616	1422	0.06%	0.008%
62	13.434	3835	3839	3841	rBV4	2243	1858	0.08%	0.011%


Sum of corrected areas: 16853003

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013892.D
Acq On : 03 Dec 2019 14:39
Operator : SY/MD
Sample : K6086-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

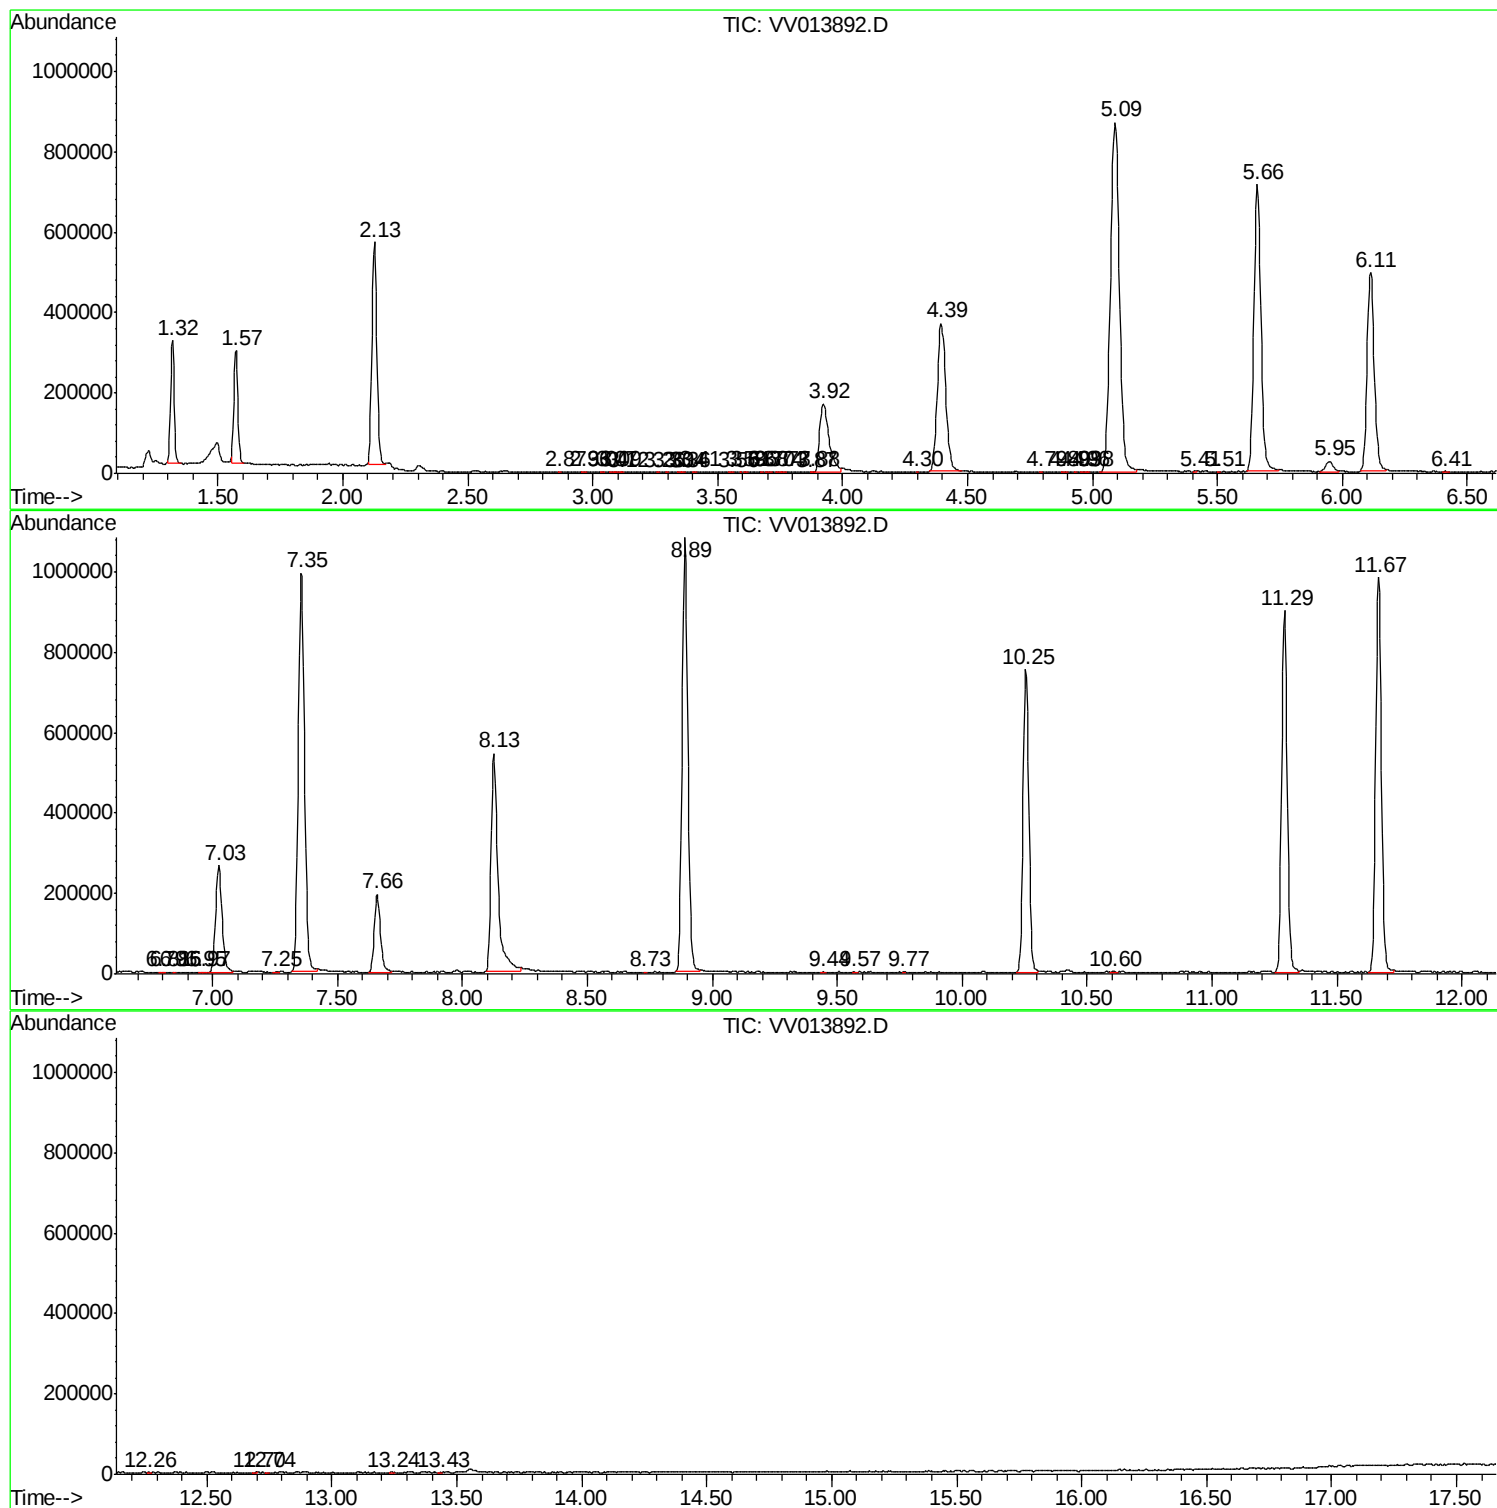

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013892.D
Acq On : 03 Dec 2019 14:39
Operator : SY/MD
Sample : K6086-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013892.D
Acq On : 03 Dec 2019 14:39
Operator : SY/MD
Sample : K6086-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLY9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc