

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013894.D
 Acq On : 03 Dec 2019 15:28
 Operator : SY/MD
 Sample : K6086-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLZ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	79	rVB	276905	260643	10.02%	1.480%
2	1.569	143	149	163	rVB	278124	325129	12.50%	1.847%
3	2.122	313	321	348	rVB	563432	843703	32.44%	4.792%
4	3.920	870	880	911	rBV2	204043	562227	21.62%	3.193%
5	4.389	1014	1026	1053	rVB	435888	1073644	41.28%	6.098%
6	5.090	1227	1244	1275	rBV2	1038030	2601009	100.00%	14.773%
7	5.659	1408	1421	1450	rBV	897440	1744033	67.05%	9.906%
8	6.113	1549	1562	1584	rBV	535541	1078064	41.45%	6.123%
9	6.344	1632	1634	1637	rBV4	2047	993	0.04%	0.006%
10	6.540	1693	1695	1698	rBV3	1916	1412	0.05%	0.008%
11	6.791	1769	1773	1776	rBV6	1364	1020	0.04%	0.006%
12	6.852	1787	1792	1797	rBV8	1835	1408	0.05%	0.008%
13	6.871	1797	1798	1801	rBV3	570	228	0.01%	0.001%
14	6.910	1807	1810	1817	rBV9	1640	1820	0.07%	0.010%
15	6.971	1827	1829	1830	rBV2	1100	556	0.02%	0.003%
16	7.026	1834	1846	1862	rVV	256031	461576	17.75%	2.622%
17	7.354	1935	1948	1969	rBV	973683	1670594	64.23%	9.488%
18	7.659	2033	2043	2058	rBV	178428	295419	11.36%	1.678%
19	7.862	2103	2106	2110	rBV4	2130	1138	0.04%	0.006%
20	8.129	2178	2189	2224	rBV3	468389	1006842	38.71%	5.719%
21	8.566	2322	2325	2327	rBV3	1261	985	0.04%	0.006%
22	8.685	2360	2362	2365	rBV3	1678	898	0.03%	0.005%
23	8.839	2408	2410	2411	rBV2	793	323	0.01%	0.002%
24	8.891	2413	2426	2448	rVV	1090248	1748272	67.22%	9.930%
25	9.219	2526	2528	2532	rBV3	1120	530	0.02%	0.003%
26	9.289	2548	2550	2552	rBV2	1602	903	0.03%	0.005%
27	9.376	2572	2577	2579	rBV4	1421	1503	0.06%	0.009%
28	9.415	2586	2589	2592	rVB4	1229	930	0.04%	0.005%
29	9.440	2592	2597	2600	rBV6	1839	1517	0.06%	0.009%
30	9.469	2601	2606	2609	rVB5	1437	1038	0.04%	0.006%
31	9.492	2611	2613	2617	rVV4	1359	963	0.04%	0.005%
32	9.547	2628	2630	2634	rVB5	1118	607	0.02%	0.003%
33	9.579	2636	2640	2641	rBV4	1128	613	0.02%	0.003%
34	9.640	2657	2659	2662	rBV3	773	453	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013894.D
 Acq On : 03 Dec 2019 15:28
 Operator : SY/MD
 Sample : K6086-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLZ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	9.659	2664	2665	2666	rVV3	685	140	0.01%	0.001%
36	9.701	2676	2678	2680	rBV3	1055	627	0.02%	0.004%
37	9.781	2699	2703	2704	rBV4	1159	618	0.02%	0.004%
38	9.842	2718	2722	2725	rBV4	1202	1053	0.04%	0.006%
39	9.858	2725	2727	2731	rBV5	1523	960	0.04%	0.005%
40	9.936	2748	2751	2757	rBV6	1641	1532	0.06%	0.009%
41	10.010	2770	2774	2777	rBV5	1350	950	0.04%	0.005%
42	10.029	2777	2780	2783	rBV3	930	589	0.02%	0.003%
43	10.055	2786	2788	2792	rVB5	1053	552	0.02%	0.003%
44	10.116	2804	2807	2809	rBV3	1236	554	0.02%	0.003%
45	10.129	2809	2811	2813	rVB3	782	255	0.01%	0.001%
46	10.157	2818	2820	2821	rVV	866	281	0.01%	0.002%
47	10.180	2825	2827	2828	rVB2	661	152	0.01%	0.001%
48	10.190	2828	2830	2832	rBV3	1318	720	0.03%	0.004%
49	10.254	2839	2850	2867	rBV	658704	1021974	39.29%	5.804%
50	10.421	2896	2902	2906	rVB6	3120	3280	0.13%	0.019%
51	10.508	2926	2929	2931	rBV4	1629	1089	0.04%	0.006%
52	10.540	2937	2939	2942	rVB3	1617	602	0.02%	0.003%
53	10.556	2942	2944	2945	rBV2	759	307	0.01%	0.002%
54	10.579	2949	2951	2952	rBV2	619	311	0.01%	0.002%
55	10.633	2965	2968	2971	rBV3	1284	878	0.03%	0.005%
56	10.672	2977	2980	2984	rVB4	1272	975	0.04%	0.006%
57	10.694	2984	2987	2990	rBV3	719	593	0.02%	0.003%
58	10.727	2994	2997	3000	rBV3	1583	957	0.04%	0.005%
59	10.746	3000	3003	3006	rVV4	1886	1170	0.04%	0.007%
60	10.823	3023	3027	3033	rBV7	1246	1526	0.06%	0.009%
61	10.865	3038	3040	3042	rBV3	1062	580	0.02%	0.003%
62	10.891	3046	3048	3054	rVB6	1494	1287	0.05%	0.007%
63	10.916	3054	3056	3059	rBV3	1411	967	0.04%	0.005%
64	10.977	3072	3075	3077	rBV3	1283	750	0.03%	0.004%
65	11.003	3081	3083	3084	rBV2	893	440	0.02%	0.002%
66	11.042	3093	3095	3097	rBV	843	435	0.02%	0.002%
67	11.058	3097	3100	3106	rVV6	2199	1905	0.07%	0.011%
68	11.122	3118	3120	3121	rBV	460	141	0.01%	0.001%
69	11.151	3127	3129	3131	rBV2	1324	693	0.03%	0.004%
70	11.177	3133	3137	3139	rBV4	1116	617	0.02%	0.004%
71	11.202	3139	3145	3147	rBV7	1573	1485	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013894.D
Acq On : 03 Dec 2019 15:28
Operator : SY/MD
Sample : K6086-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLZ1

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

72	11.212	3147	3148	3150	rBV2	844	359	0.01%	0.002%
73	11.244	3157	3158	3160	rBV2	911	454	0.02%	0.003%
74	11.289	3160	3172	3193	rVV	896057	1399002	53.79%	7.946%
75	11.665	3277	3289	3309	rBV	935491	1453858	55.90%	8.257%
76	12.064	3410	3413	3416	rBV3	1467	1049	0.04%	0.006%
77	12.100	3422	3424	3425	rBV3	1111	455	0.02%	0.003%
78	12.283	3480	3481	3482	rBV	879	262	0.01%	0.001%
79	12.337	3495	3498	3501	rBV4	1051	642	0.02%	0.004%
80	12.382	3510	3512	3514	rBV3	1866	943	0.04%	0.005%
81	12.604	3579	3581	3583	rBV2	1371	809	0.03%	0.005%
82	12.617	3583	3585	3587	rVB2	1186	508	0.02%	0.003%
83	13.453	3842	3845	3846	rBV3	1816	803	0.03%	0.005%
84	13.691	3917	3919	3924	rBV5	1889	1270	0.05%	0.007%
85	13.897	3982	3983	3984	rBV	967	350	0.01%	0.002%
86	13.948	3997	3999	4001	rBV2	1761	1044	0.04%	0.006%
87	14.042	4023	4028	4032	rBV7	1524	1899	0.07%	0.011%




Sum of corrected areas: 17606645

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013894.D
Acq On : 03 Dec 2019 15:28
Operator : SY/MD
Sample : K6086-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLZ1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

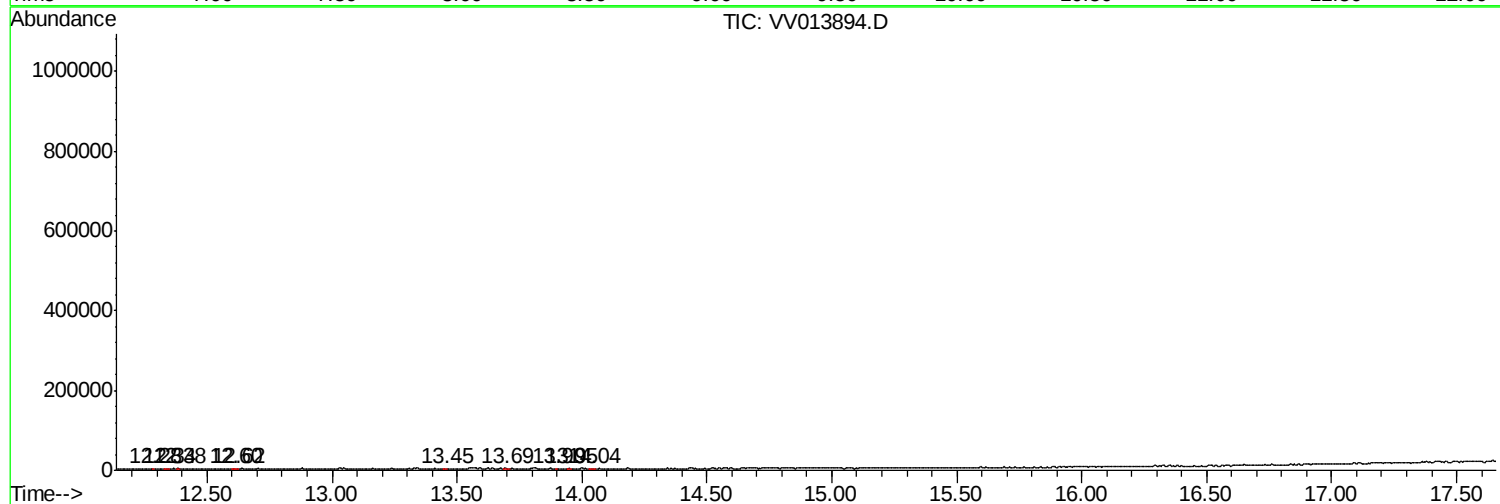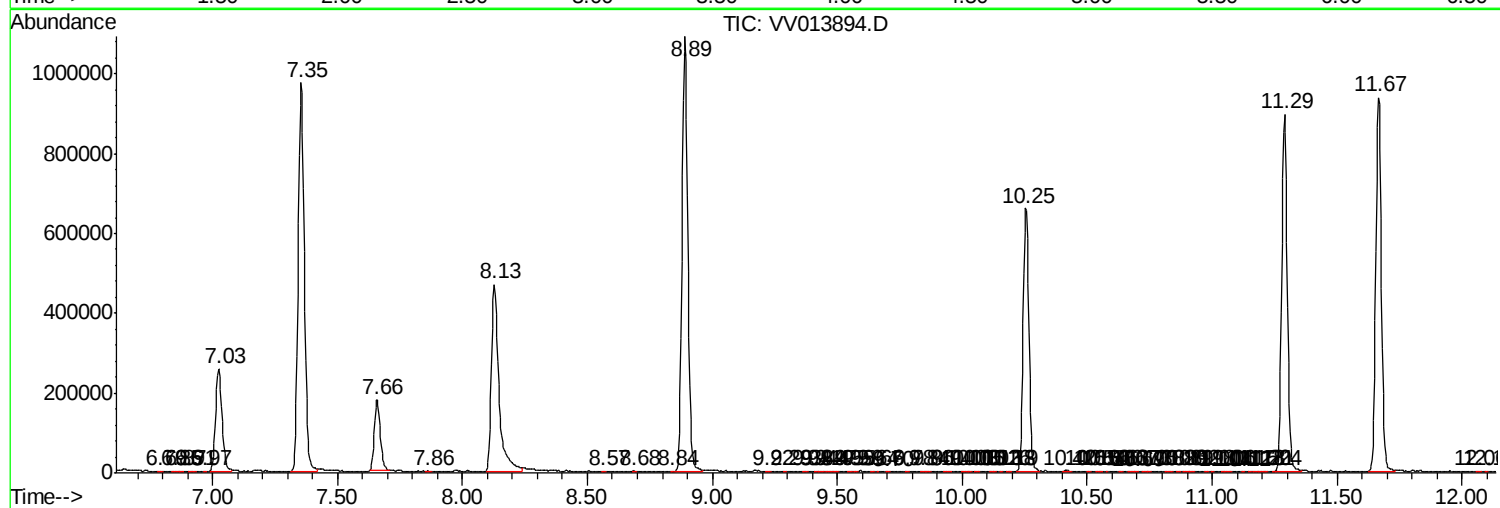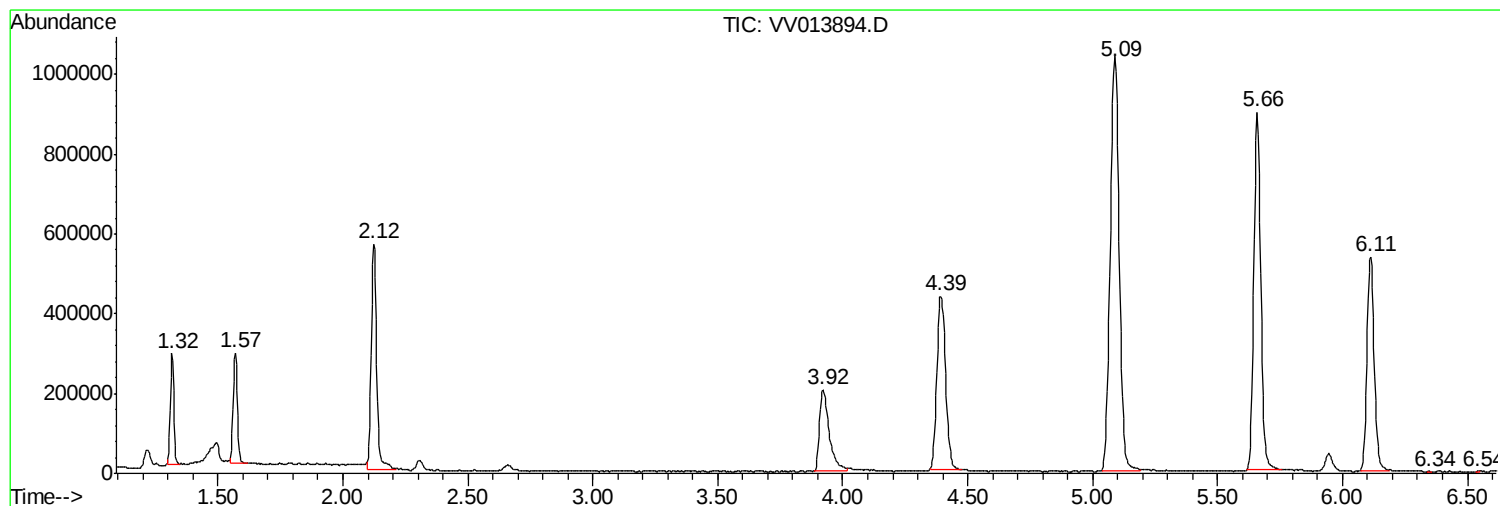

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013894.D
Acq On : 03 Dec 2019 15:28
Operator : SY/MD
Sample : K6086-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLZ1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013894.D
Acq On : 03 Dec 2019 15:28
Operator : SY/MD
Sample : K6086-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLZ1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc