

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013896.D
 Acq On : 03 Dec 2019 16:20
 Operator : SY/MD
 Sample : K6028-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB	277576	270302	10.23%	1.374%
2	1.573	144	150	164	rVB	276432	323550	12.25%	1.645%
3	2.126	314	322	337	rVB	542910	761850	28.84%	3.873%
4	2.740	511	513	515	rBV3	1290	558	0.02%	0.003%
5	2.759	515	519	521	rBV5	2077	1664	0.06%	0.008%
6	2.955	578	580	583	rBV4	1349	773	0.03%	0.004%
7	2.984	587	589	593	rBV5	2130	1862	0.07%	0.009%
8	3.209	655	659	661	rBV4	2442	1644	0.06%	0.008%
9	3.306	686	689	692	rBV4	1724	905	0.03%	0.005%
10	3.318	692	693	696	rBV3	1049	520	0.02%	0.003%
11	3.396	715	717	718	rBV2	1400	442	0.02%	0.002%
12	3.508	750	752	757	rBV4	1594	1614	0.06%	0.008%
13	3.540	760	762	766	rVB3	2047	1136	0.04%	0.006%
14	3.560	766	768	769	rBV	1681	816	0.03%	0.004%
15	3.643	791	794	795	rBV3	1346	674	0.03%	0.003%
16	3.672	801	803	807	rBV5	1387	855	0.03%	0.004%
17	3.749	822	827	828	rBV4	1654	1149	0.04%	0.006%
18	3.810	845	846	850	rVB4	1722	658	0.02%	0.003%
19	3.852	857	859	860	rBV2	1047	520	0.02%	0.003%
20	3.923	870	881	913	rBV2	244524	854805	32.36%	4.346%
21	4.396	1013	1028	1054	rVB	445931	1066317	40.37%	5.421%
22	4.846	1166	1168	1169	rBV2	1349	562	0.02%	0.003%
23	4.900	1180	1185	1186	rBV3	1178	1067	0.04%	0.005%
24	5.026	1222	1224	1225	rBV2	1849	793	0.03%	0.004%
25	5.090	1227	1244	1261	rBV2	1060703	2641610	100.00%	13.430%
26	5.659	1406	1421	1446	rBV	833924	1660406	62.86%	8.441%
27	6.113	1549	1562	1585	rBV	599868	1187013	44.94%	6.035%
28	6.412	1652	1655	1656	rBV3	1254	694	0.03%	0.004%
29	6.608	1714	1716	1717	rBV2	1622	731	0.03%	0.004%
30	6.823	1780	1783	1784	rBV3	2172	1226	0.05%	0.006%
31	7.026	1833	1846	1863	rBV	305869	541510	20.50%	2.753%
32	7.357	1936	1949	1968	rBV	1146205	1972852	74.68%	10.030%
33	7.659	2032	2043	2062	rBV	218729	364948	13.82%	1.855%
34	8.125	2178	2188	2222	rBV2	714313	1439047	54.48%	7.316%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013896.D
 Acq On : 03 Dec 2019 16:20
 Operator : SY/MD
 Sample : K6028-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	8.588	2328	2332	2333	rBV4	2498	1601	0.06%	0.008%
36	8.891	2414	2426	2446	rBV	1209787	1943489	73.57%	9.881%
37	9.437	2593	2596	2597	rBV3	1704	1071	0.04%	0.005%
38	9.768	2696	2699	2702	rBV5	2269	1188	0.04%	0.006%
39	9.807	2709	2711	2712	rBV2	1130	466	0.02%	0.002%
40	9.836	2717	2720	2722	rBV4	2184	1460	0.06%	0.007%
41	9.929	2747	2749	2753	rVB5	1498	627	0.02%	0.003%
42	10.254	2839	2850	2865	rBV	882798	1362787	51.59%	6.928%
43	10.453	2909	2912	2916	rVB	24440	13745	0.52%	0.070%
44	10.659	2973	2976	2977	rBV2	1188	782	0.03%	0.004%
45	10.714	2988	2993	2994	rBV4	2223	1802	0.07%	0.009%
46	10.755	3004	3006	3007	rBV2	1779	751	0.03%	0.004%
47	10.820	3023	3026	3031	rBV6	1621	1738	0.07%	0.009%
48	10.868	3038	3041	3042	rBV3	1810	865	0.03%	0.004%
49	11.289	3160	3172	3192	rBV	983567	1535465	58.13%	7.806%
50	11.492	3233	3235	3237	rVB3	2130	949	0.04%	0.005%
51	11.665	3277	3289	3305	rBV	1086786	1683999	63.75%	8.561%
52	12.386	3510	3513	3516	rBV5	3029	2057	0.08%	0.010%
53	12.415	3519	3522	3527	rBV7	1545	1611	0.06%	0.008%
54	12.508	3548	3551	3554	rBV5	2804	1786	0.07%	0.009%
55	12.640	3589	3592	3594	rBV4	1144	787	0.03%	0.004%
56	12.652	3594	3596	3598	rVB3	1849	815	0.03%	0.004%
57	12.694	3606	3609	3611	rBV4	3002	2093	0.08%	0.011%
58	12.945	3685	3687	3689	rBV3	1719	837	0.03%	0.004%
59	13.112	3734	3739	3741	rBV4	2348	1946	0.07%	0.010%


Sum of corrected areas: 19669790

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013896.D
Acq On : 03 Dec 2019 16:20
Operator : SY/MD
Sample : K6028-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

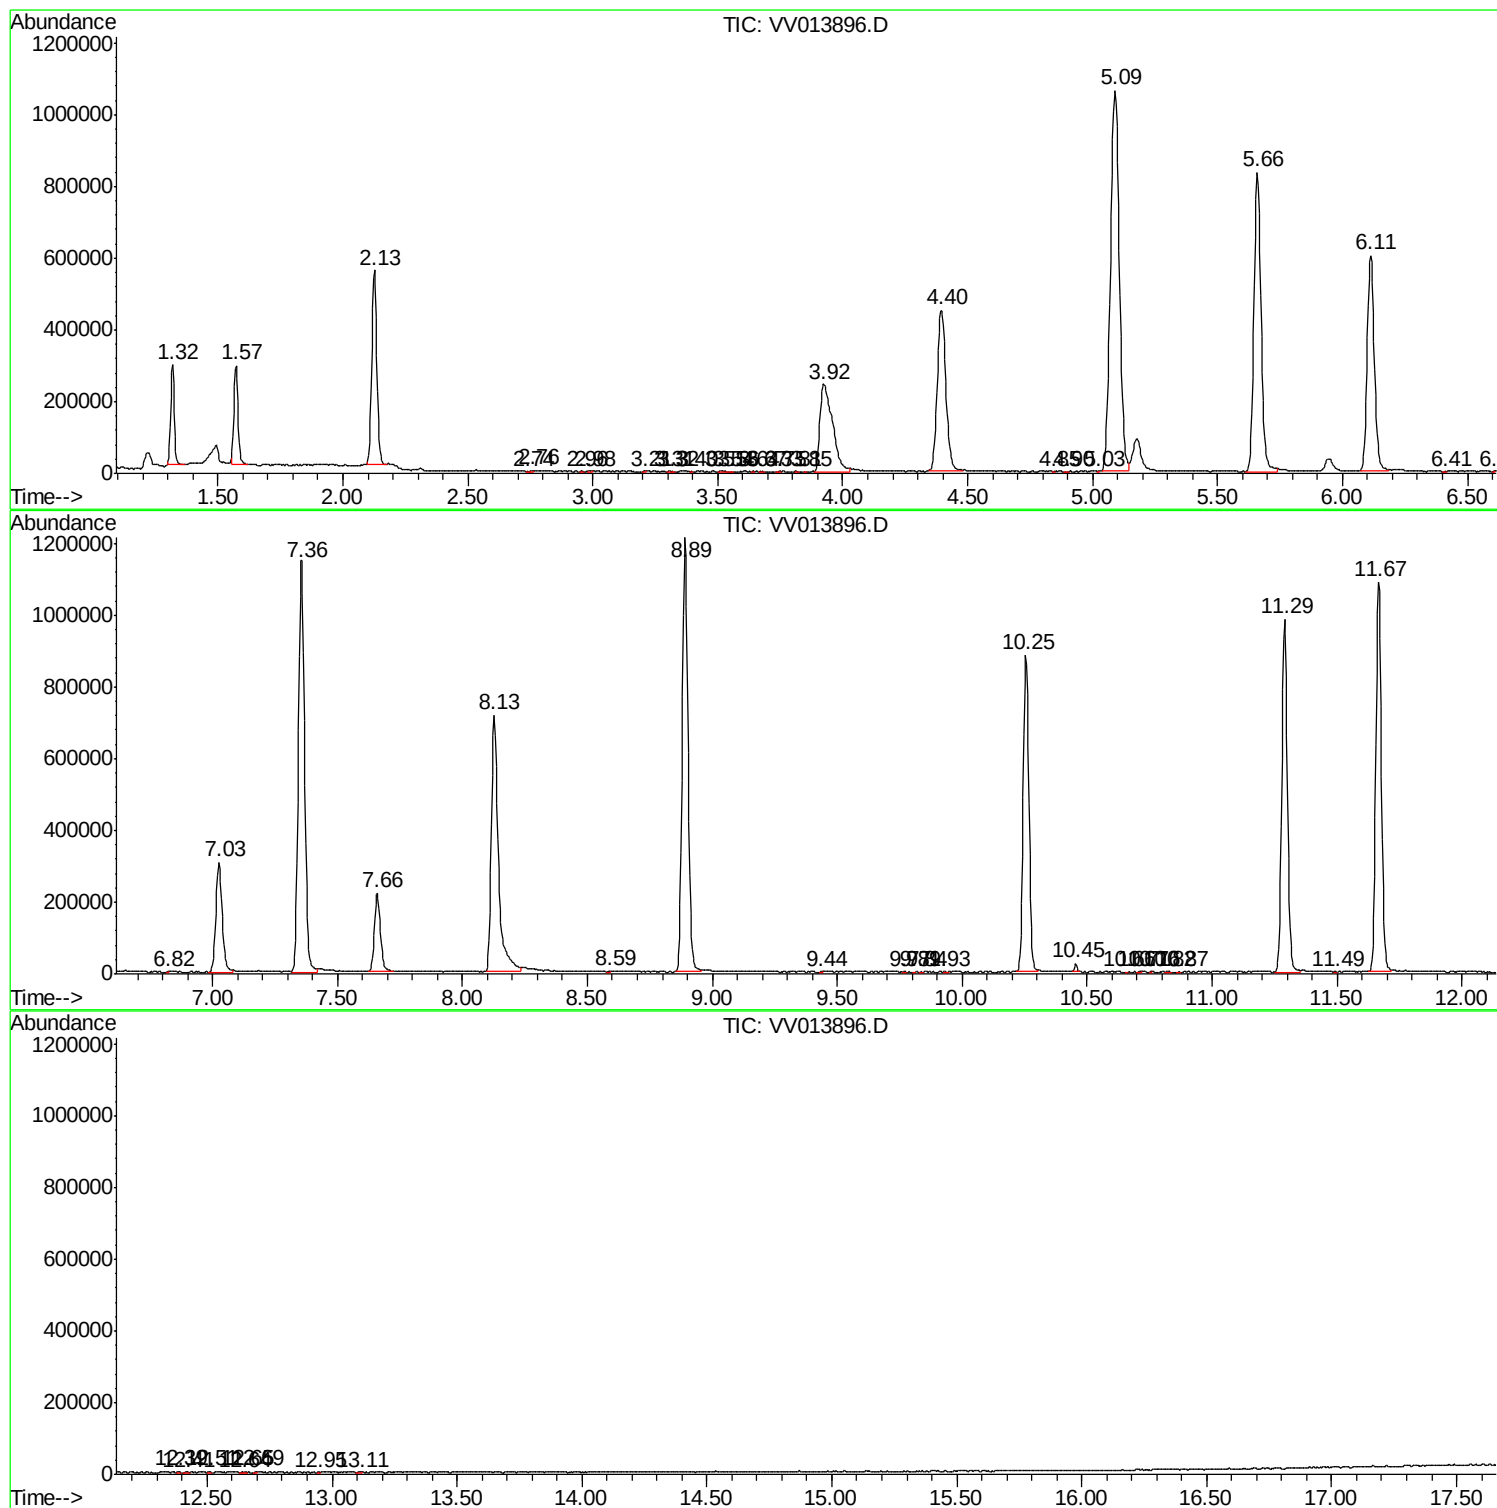

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013896.D
Acq On : 03 Dec 2019 16:20
Operator : SY/MD
Sample : K6028-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120319\
Data File : VV013896.D
Acq On : 03 Dec 2019 16:20
Operator : SY/MD
Sample : K6028-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc