


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120319\
 Data File : VV013881.D
 Acq On : 03 Dec 2019 09:20
 Operator : SY/MD
 Sample : BFB75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 04 01:11:22 2019

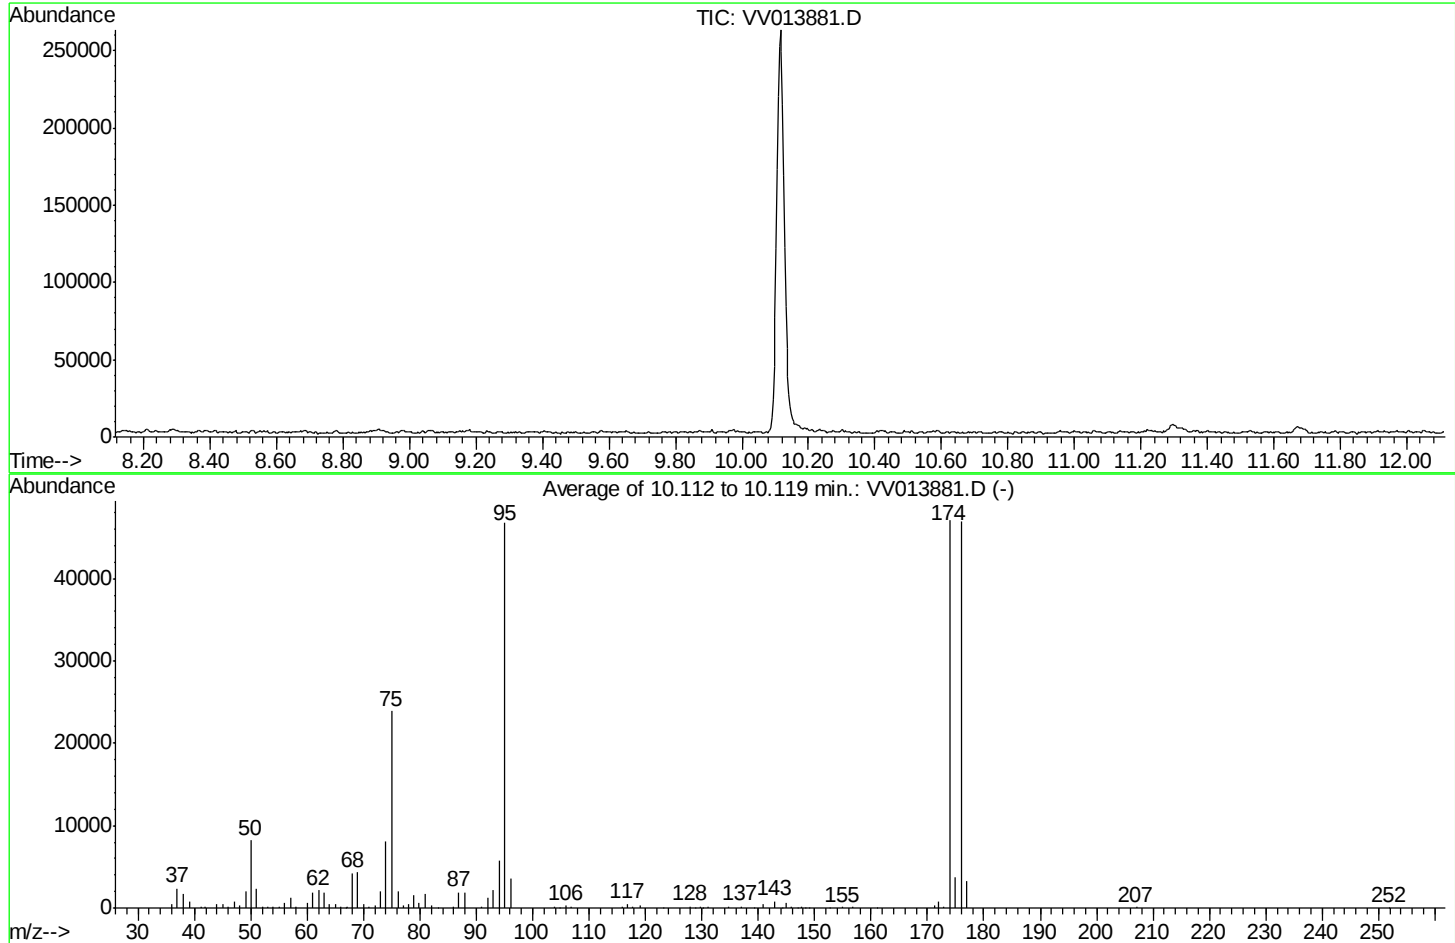

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	8164	PASS
75	95	30	80	51.0	23864	PASS
95	95	100	100	100.0	46821	PASS
96	95	5	9	7.6	3565	PASS
173	174	0.00	2	0.4	189	PASS
174	95	50	120	100.5	47066	PASS
175	174	5	9	7.9	3712	PASS
176	174	95	101	99.7	46917	PASS
177	176	5	9	7.0	3268	PASS

m/z	Abundance
36.00	510.0
37.00	2640.0
38.10	1632.0
39.00	781.0
40.10	660.0
41.10	132.0
41.80	184.0
44.00	845.0
45.00	423.0
45.90	185.0
47.10	707.0
48.00	377.0
49.10	1919.0
50.00	8284.0
51.00	2300.0
52.00	241.0
52.90	196.0
53.80	127.0
55.00	202.0
56.00	694.0
57.10	1403.0
58.10	101.0
58.60	110.0
60.00	597.0
61.00	1801.0
62.10	2225.0
63.00	1960.0
64.00	419.0
65.00	512.0
66.10	166.0
67.20	310.0
68.10	4417.0
69.00	4440.0
70.00	411.0
70.80	154.0
72.10	290.0
73.00	1897.0
74.00	8225.0
75.00	24192.0
76.10	1893.0
77.10	298.0
78.00	528.0
78.90	1523.0
79.90	517.0
80.90	1577.0
82.00	417.0
86.10	201.0
86.90	1844.0
87.90	1742.0
91.10	159.0
92.00	1222.0
93.00	2005.0
94.00	5791.0
95.10	47264.0
96.00	3617.0
103.90	189.0
104.80	118.0
105.90	270.0
115.80	212.0
116.90	530.0
117.80	142.0
119.10	422.0
128.00	208.0
129.60	241.0
131.20	116.0
134.80	149.0
136.90	213.0
140.90	501.0
143.00	777.0
144.20	122.0
145.00	612.0
145.80	124.0
147.60	115.0
152.80	117.0
155.10	177.0
171.20	276.0
172.00	887.0
174.00	45864.0
175.00	3733.0
175.90	45792.0
177.00	3299.0
207.10	135.0
251.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	525.0
37.00	2557.0
38.00	1908.0
39.00	864.0
40.00	715.0
41.10	187.0
41.90	193.0
44.00	1045.0
45.00	432.0
45.90	203.0
47.10	741.0
47.90	362.0
49.10	1919.0
50.00	8330.0
51.00	2504.0
52.00	183.0
52.90	229.0
53.80	168.0
55.00	229.0
56.10	678.0
57.00	1313.0
58.00	137.0
58.70	124.0
60.00	676.0
61.10	1905.0
62.10	2205.0
63.00	1950.0
64.00	468.0
65.10	568.0
66.10	161.0
67.10	230.0
68.00	4373.0
69.00	4516.0
70.00	445.0
70.90	194.0
72.10	345.0
73.00	2004.0
74.00	8332.0
75.00	25064.0
76.10	2060.0
77.10	345.0
78.00	417.0
78.90	1550.0
79.80	584.0
80.90	1838.0
82.00	398.0
85.90	192.0
86.90	1945.0
87.90	1931.0
90.90	236.0
92.00	1346.0
93.00	2111.0
94.00	5945.0
95.10	48040.0
96.10	3744.0
104.00	214.0
104.70	103.0
105.90	282.0
106.80	131.0
115.80	218.0
116.90	550.0
117.80	155.0
119.10	394.0
128.00	224.0
129.70	176.0
130.20	118.0
131.10	115.0
134.80	120.0
136.90	197.0
140.90	510.0
143.00	813.0
144.10	118.0
145.00	649.0
145.70	155.0
147.60	207.0
148.30	105.0
152.70	102.0
155.00	117.0
156.70	131.0
161.00	104.0
171.20	299.0
172.00	841.0
174.00	48592.0
175.00	3786.0
176.00	48632.0
177.00	3402.0
207.10	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	508.0
37.00	2184.0
38.00	2055.0
39.10	877.0
39.90	738.0
41.10	178.0
41.90	212.0
42.80	109.0
44.00	1034.0
44.90	425.0
45.90	180.0
47.00	724.0
47.90	308.0
49.10	2020.0
50.00	7879.0
51.00	2410.0
52.00	173.0
53.00	181.0
53.90	178.0
54.90	202.0
56.10	679.0
57.00	1050.0
58.00	213.0
60.00	631.0
61.10	1834.0
62.00	2033.0
63.00	1804.0
64.00	446.0
65.10	563.0
66.00	133.0
66.90	203.0
68.00	3957.0
69.00	4344.0
70.00	418.0
70.90	137.0
72.20	412.0
73.00	2014.0
74.00	7526.0
75.00	22336.0
76.00	2134.0
77.00	419.0
78.10	300.0
78.80	1519.0
79.90	587.0
80.90	1877.0
82.00	339.0
83.10	111.0
85.80	221.0
86.90	1854.0
87.90	1777.0
90.90	280.0
92.00	1341.0
93.00	2301.0
94.00	5355.0
95.10	45160.0
96.10	3334.0
104.00	238.0
106.00	234.0
106.80	153.0
115.90	218.0
116.90	504.0
117.80	169.0
118.90	319.0
123.10	118.0
128.00	224.0
128.90	115.0
129.80	170.0
131.00	162.0
137.00	192.0
139.20	107.0
140.90	468.0
143.00	957.0
145.00	535.0
145.80	131.0
146.90	115.0
147.70	224.0
149.00	146.0
154.90	112.0
156.60	174.0
161.00	117.0
171.20	269.0
172.00	719.0
172.80	569.0
174.00	46744.0
175.00	3619.0
176.00	46328.0
176.90	3104.0
207.10	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

Scan 2792 (10.067 min): VV013881.D
BFB75

m/z	Abundance
35.20	140.0
36.80	113.0
38.20	117.0
38.80	125.0
40.00	734.0
42.70	156.0
43.30	119.0
43.90	498.0
45.50	113.0
48.70	107.0
51.40	113.0
58.60	112.0
76.80	144.0
90.60	193.0
197.30	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75