

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019469.D
 Acq On : 03 Dec 2020 20:31
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Quant Time: Dec 04 08:45:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 04 08:04:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	323377	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	332010	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	148596	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	105097	32.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	65.08%
7) Chloroethane-d5	1.58	69	102535	39.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.02%
11) 1,1-Dichloroethene-d2	2.12	63	186013	32.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.72%
21) 2-Butanone-d5	3.89	46	206041	104.67	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.67%
24) Chloroform-d	4.37	84	252087	48.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.56%
26) 1,2-Dichloroethane-d4	5.05	65	180496	52.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.62%
32) Benzene-d6	5.07	84	479722	48.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.74%
36) 1,2-Dichloropropane-d6	6.09	67	167298	51.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.44%
41) Toluene-d8	7.33	98	401666	45.68	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.36%
43) trans-1,3-Dichloropropene-	7.64	79	72537	45.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.96%
47) 2-Hexanone-d5	8.10	63	99603	77.40	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.40%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	186276	44.06	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.12%
64) 1,2-Dichlorobenzene-d4	11.64	152	149958	51.97	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.94%


Target Compounds					Ovalue
46) Tetrachloroethene	7.99	164	1629	0.847 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120320\
Data File : VV019469.D
Acq On : 03 Dec 2020 20:31
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Time: Dec 04 08:45:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 04 08:04:03 2020
Response via : Initial Calibration

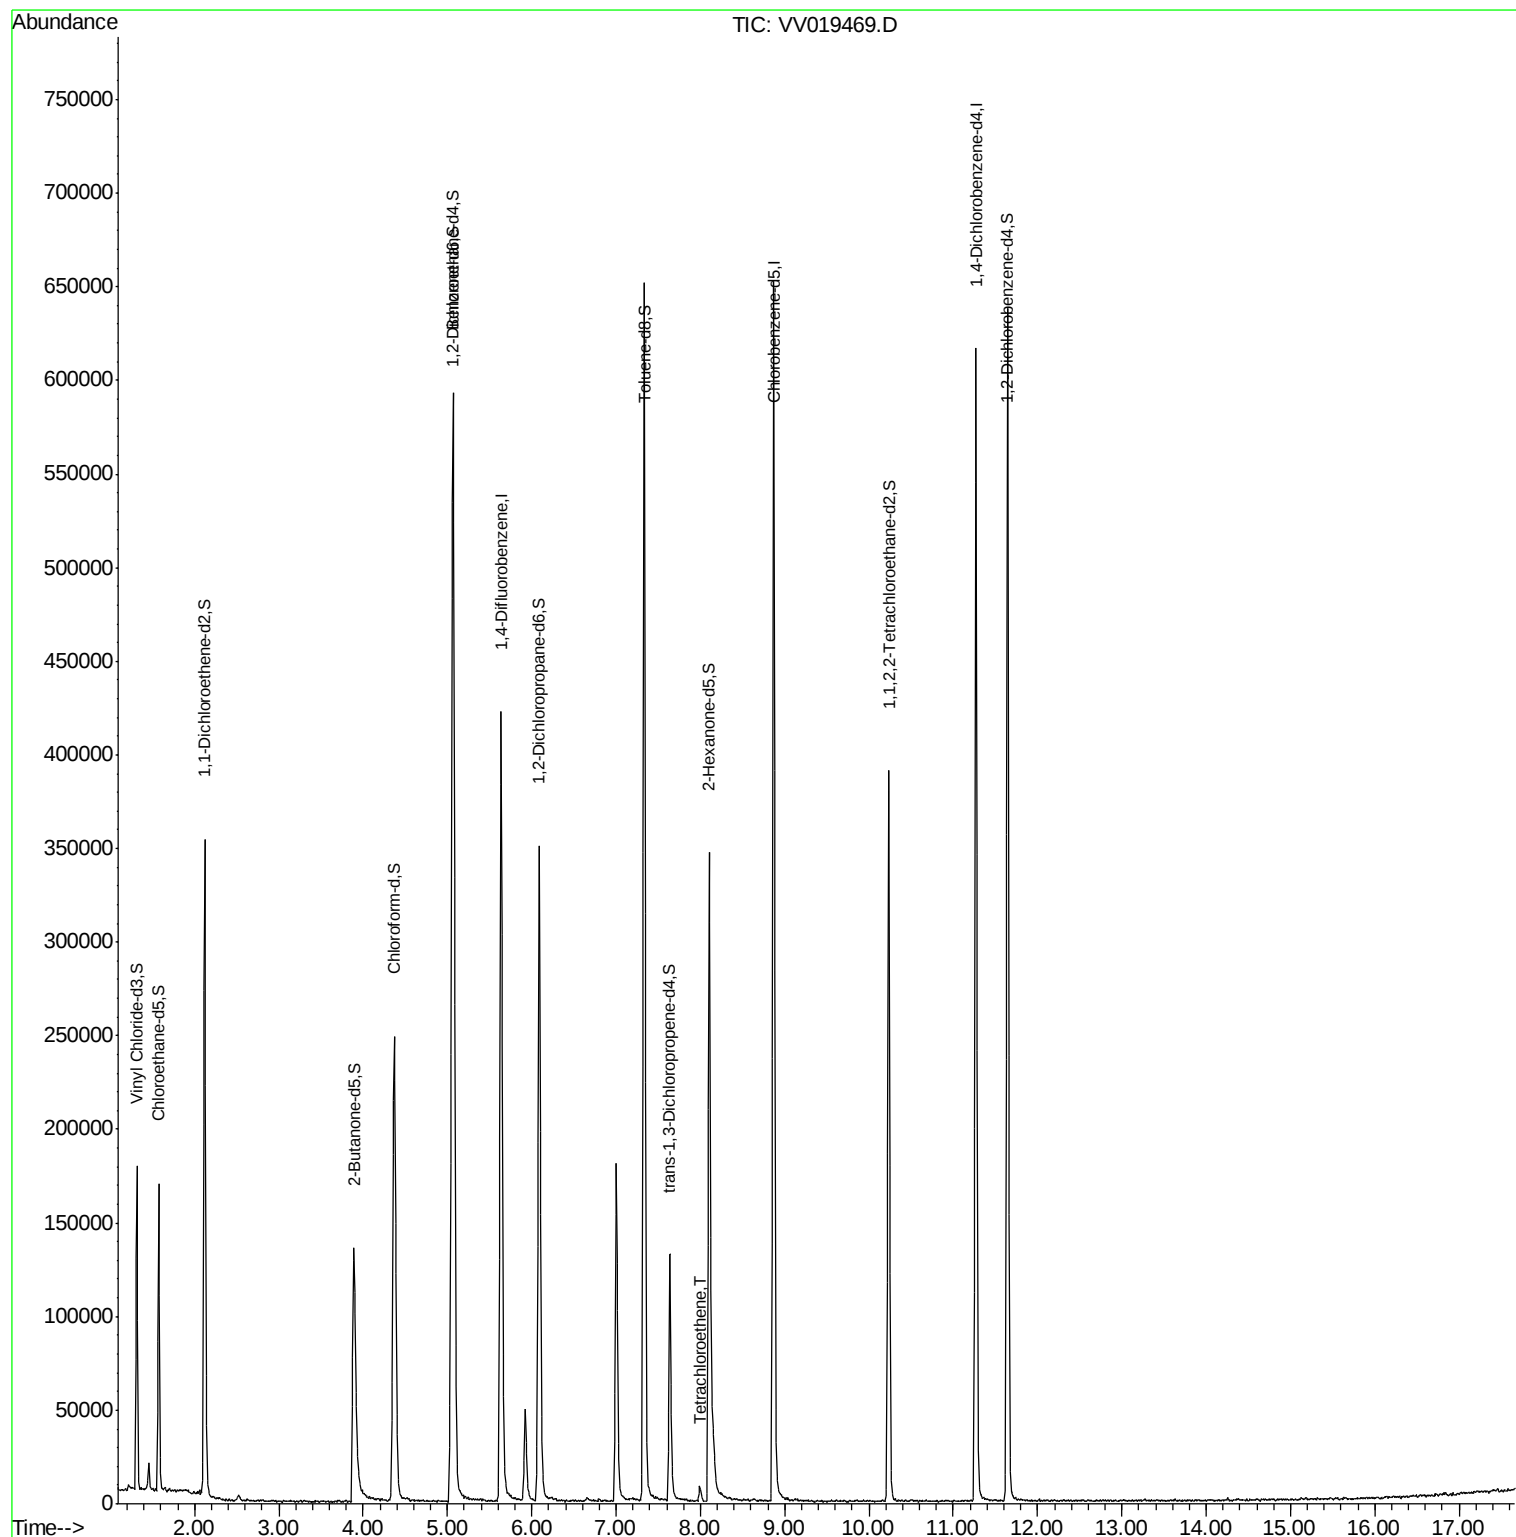

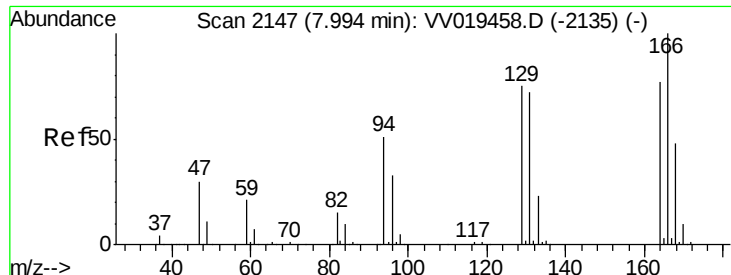

#46

Tetrachloroethene

Concen: 0.847 ug/L

RT: 7.99 min Scan# 2147

Delta R.T. 0.00 min

Lab File: VV019469.D


Acq: 03 Dec 2020 20:31

Instrument :

MSVOA_V

ClientSampleId :

VIBLK80

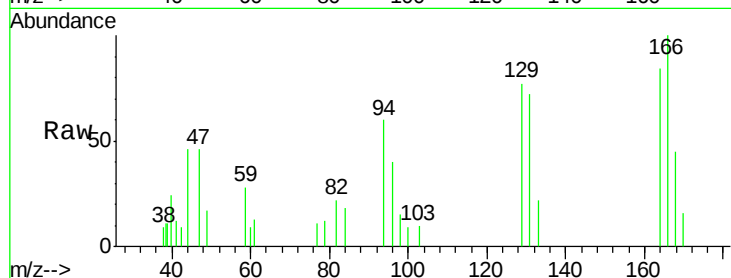

Tot Ion:164 Resp: 1629

Ion Ratio Lower Upper

164 100

129 90.8 62.9 116.7

131 85.2 61.1 113.5

166 118.6 86.5 160.6

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

