

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019459.D
 Acq On : 03 Dec 2020 16:02
 Operator : SY/MD
 Sample : VV1203WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	167072	175077	11.76%	1.574%
2	1.576	144	151	165	rVB	161079	186013	12.49%	1.673%
3	2.119	311	320	347	rVB	334419	515730	34.64%	4.638%
4	2.521	438	445	454	rVV7	4843	7921	0.53%	0.071%
5	2.557	454	456	460	rVB3	737	323	0.02%	0.003%
6	2.682	492	495	497	rBV2	830	614	0.04%	0.006%
7	2.704	500	502	505	rVV4	654	451	0.03%	0.004%
8	2.814	535	536	540	rBV3	817	507	0.03%	0.005%
9	2.901	560	563	566	rVB3	864	536	0.04%	0.005%
10	2.923	566	570	573	rBV3	588	439	0.03%	0.004%
11	3.036	603	605	610	rVB4	691	455	0.03%	0.004%
12	3.061	610	613	615	rBV3	561	314	0.02%	0.003%
13	3.110	623	628	632	rBV2	653	616	0.04%	0.006%
14	3.161	642	644	647	rBV2	528	400	0.03%	0.004%
15	3.200	653	656	660	rBV2	950	754	0.05%	0.007%
16	3.319	688	693	695	rVV3	629	616	0.04%	0.006%
17	3.357	703	705	709	rVB3	468	290	0.02%	0.003%
18	3.377	709	711	714	rBV2	569	383	0.03%	0.003%
19	3.412	718	722	725	rBV2	565	405	0.03%	0.004%
20	3.444	729	732	734	rBV2	841	441	0.03%	0.004%
21	3.531	756	759	765	rVB5	930	557	0.04%	0.005%
22	3.566	765	770	771	rBV2	615	372	0.02%	0.003%
23	3.614	780	785	787	rVB3	690	547	0.04%	0.005%
24	3.643	791	794	798	rVB4	491	354	0.02%	0.003%
25	3.669	798	802	806	rBV3	607	527	0.04%	0.005%
26	3.801	840	843	845	rBV3	425	304	0.02%	0.003%
27	3.897	862	873	904	rBV	144160	398028	26.73%	3.579%
28	4.373	1006	1021	1047	rBV	241513	593924	39.89%	5.341%
29	4.884	1178	1180	1184	rVB3	832	436	0.03%	0.004%
30	4.913	1184	1189	1192	rBV5	934	765	0.05%	0.007%
31	5.068	1219	1237	1262	rBV2	571628	1488797	100.00%	13.388%
32	5.528	1378	1380	1383	rVB	791	338	0.02%	0.003%
33	5.553	1385	1388	1392	rVB3	998	648	0.04%	0.006%
34	5.576	1392	1395	1397	rBV4	554	425	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019459.D
 Acq On : 03 Dec 2020 16:02
 Operator : SY/MD
 Sample : VV1203WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	5.637	1403	1414	1443	rBV	427573	861794	57.89%	7.749%
36	5.926	1492	1504	1526	rBV2	44934	95085	6.39%	0.855%
37	6.090	1538	1555	1582	rBV	349211	713467	47.92%	6.416%
38	6.370	1638	1642	1646	rBV5	793	719	0.05%	0.006%
39	6.389	1646	1648	1651	rBV3	858	444	0.03%	0.004%
40	6.470	1672	1673	1676	rBV3	743	325	0.02%	0.003%
41	6.511	1684	1686	1689	rBV	764	403	0.03%	0.004%
42	6.547	1694	1697	1700	rBV3	666	412	0.03%	0.004%
43	6.576	1700	1706	1709	rBV4	740	667	0.04%	0.006%
44	6.785	1769	1771	1774	rVB	703	278	0.02%	0.002%
45	7.007	1828	1840	1866	rBV	170388	321148	21.57%	2.888%
46	7.335	1931	1942	1962	rBV	599153	1030859	69.24%	9.270%
47	7.640	2027	2037	2065	rBV	128483	228527	15.35%	2.055%
48	7.814	2089	2091	2092	rBV2	864	372	0.02%	0.003%
49	7.849	2100	2102	2104	rBV3	712	255	0.02%	0.002%
50	7.920	2122	2124	2128	rBV3	577	458	0.03%	0.004%
51	7.997	2144	2148	2150	rBV3	1304	1189	0.08%	0.011%
52	8.032	2157	2159	2162	rBV2	429	274	0.02%	0.002%
53	8.106	2171	2182	2212	rBV2	390968	794055	53.34%	7.140%
54	8.540	2315	2317	2321	rBV5	721	525	0.04%	0.005%
55	8.598	2333	2335	2340	rBV4	569	540	0.04%	0.005%
56	8.640	2346	2348	2352	rVB4	683	317	0.02%	0.003%
57	8.807	2395	2400	2402	rBV4	734	552	0.04%	0.005%
58	8.871	2407	2420	2446	rBV	658747	1078247	72.42%	9.696%
59	9.084	2484	2486	2488	rVB3	638	238	0.02%	0.002%
60	9.244	2533	2536	2538	rBV3	761	484	0.03%	0.004%
61	9.322	2557	2560	2564	rVB3	714	584	0.04%	0.005%
62	9.341	2564	2566	2568	rBV3	650	395	0.03%	0.004%
63	9.460	2600	2603	2605	rBV3	586	348	0.02%	0.003%
64	9.543	2625	2629	2631	rBV3	791	675	0.05%	0.006%
65	9.650	2661	2662	2668	rVB2	745	395	0.03%	0.004%
66	9.698	2676	2677	2680	rBV2	448	243	0.02%	0.002%
67	9.791	2703	2706	2709	rBV3	659	494	0.03%	0.004%
68	9.807	2709	2711	2715	rBV4	798	487	0.03%	0.004%
69	9.826	2715	2717	2720	rBV3	734	450	0.03%	0.004%
70	9.952	2753	2756	2759	rBV5	1232	914	0.06%	0.008%
71	10.006	2766	2773	2775	rBV5	1044	826	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019459.D
 Acq On : 03 Dec 2020 16:02
 Operator : SY/MD
 Sample : VV1203WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

72	10.039	2781	2783	2785	rBV	484	296	0.02%	0.003%
73	10.174	2822	2825	2827	rBV3	455	316	0.02%	0.003%
74	10.235	2832	2844	2871	rVB	405940	638699	42.90%	5.743%
75	10.396	2892	2894	2899	rBV2	369	371	0.02%	0.003%
76	10.457	2910	2913	2918	rBV4	719	747	0.05%	0.007%
77	10.691	2981	2986	2987	rBV2	524	447	0.03%	0.004%
78	10.717	2993	2994	2997	rBV2	412	259	0.02%	0.002%
79	10.830	3026	3029	3031	rBV3	518	369	0.02%	0.003%
80	10.846	3032	3034	3038	rVB4	1041	571	0.04%	0.005%
81	10.871	3040	3042	3045	rBV	537	280	0.02%	0.003%
82	10.910	3052	3054	3058	rVB4	461	311	0.02%	0.003%
83	10.939	3058	3063	3066	rBV5	797	729	0.05%	0.007%
84	11.119	3117	3119	3122	rVB2	679	269	0.02%	0.002%
85	11.164	3132	3133	3139	rVB2	658	454	0.03%	0.004%
86	11.203	3141	3145	3146	rBV2	1923	1201	0.08%	0.011%
87	11.270	3154	3166	3192	rBV	619627	970730	65.20%	8.729%
88	11.466	3225	3227	3230	rBV2	820	498	0.03%	0.004%
89	11.643	3270	3282	3304	rBV	611087	971354	65.24%	8.735%
90	12.672	3596	3602	3614	rVB8	2702	4526	0.30%	0.041%
91	12.852	3656	3658	3660	rBV2	647	311	0.02%	0.003%
92	13.119	3738	3741	3742	rBV2	734	384	0.03%	0.003%
93	13.215	3768	3771	3774	rBV2	788	611	0.04%	0.005%
94	13.534	3864	3870	3873	rBV7	3587	4241	0.28%	0.038%
95	13.672	3910	3913	3915	rBV3	1158	717	0.05%	0.006%
96	13.736	3930	3933	3935	rBV2	627	395	0.03%	0.004%
97	13.772	3939	3944	3951	rVB8	2522	3304	0.22%	0.030%
98	14.225	4081	4085	4088	rBV4	717	628	0.04%	0.006%
99	14.460	4156	4158	4162	rBV3	802	560	0.04%	0.005%
100	15.093	4353	4355	4363	rBV6	1417	1401	0.09%	0.013%


Sum of corrected areas: 11120731

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120320\
Data File : VV019459.D
Acq On : 03 Dec 2020 16:02
Operator : SY/MD
Sample : VV1203WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

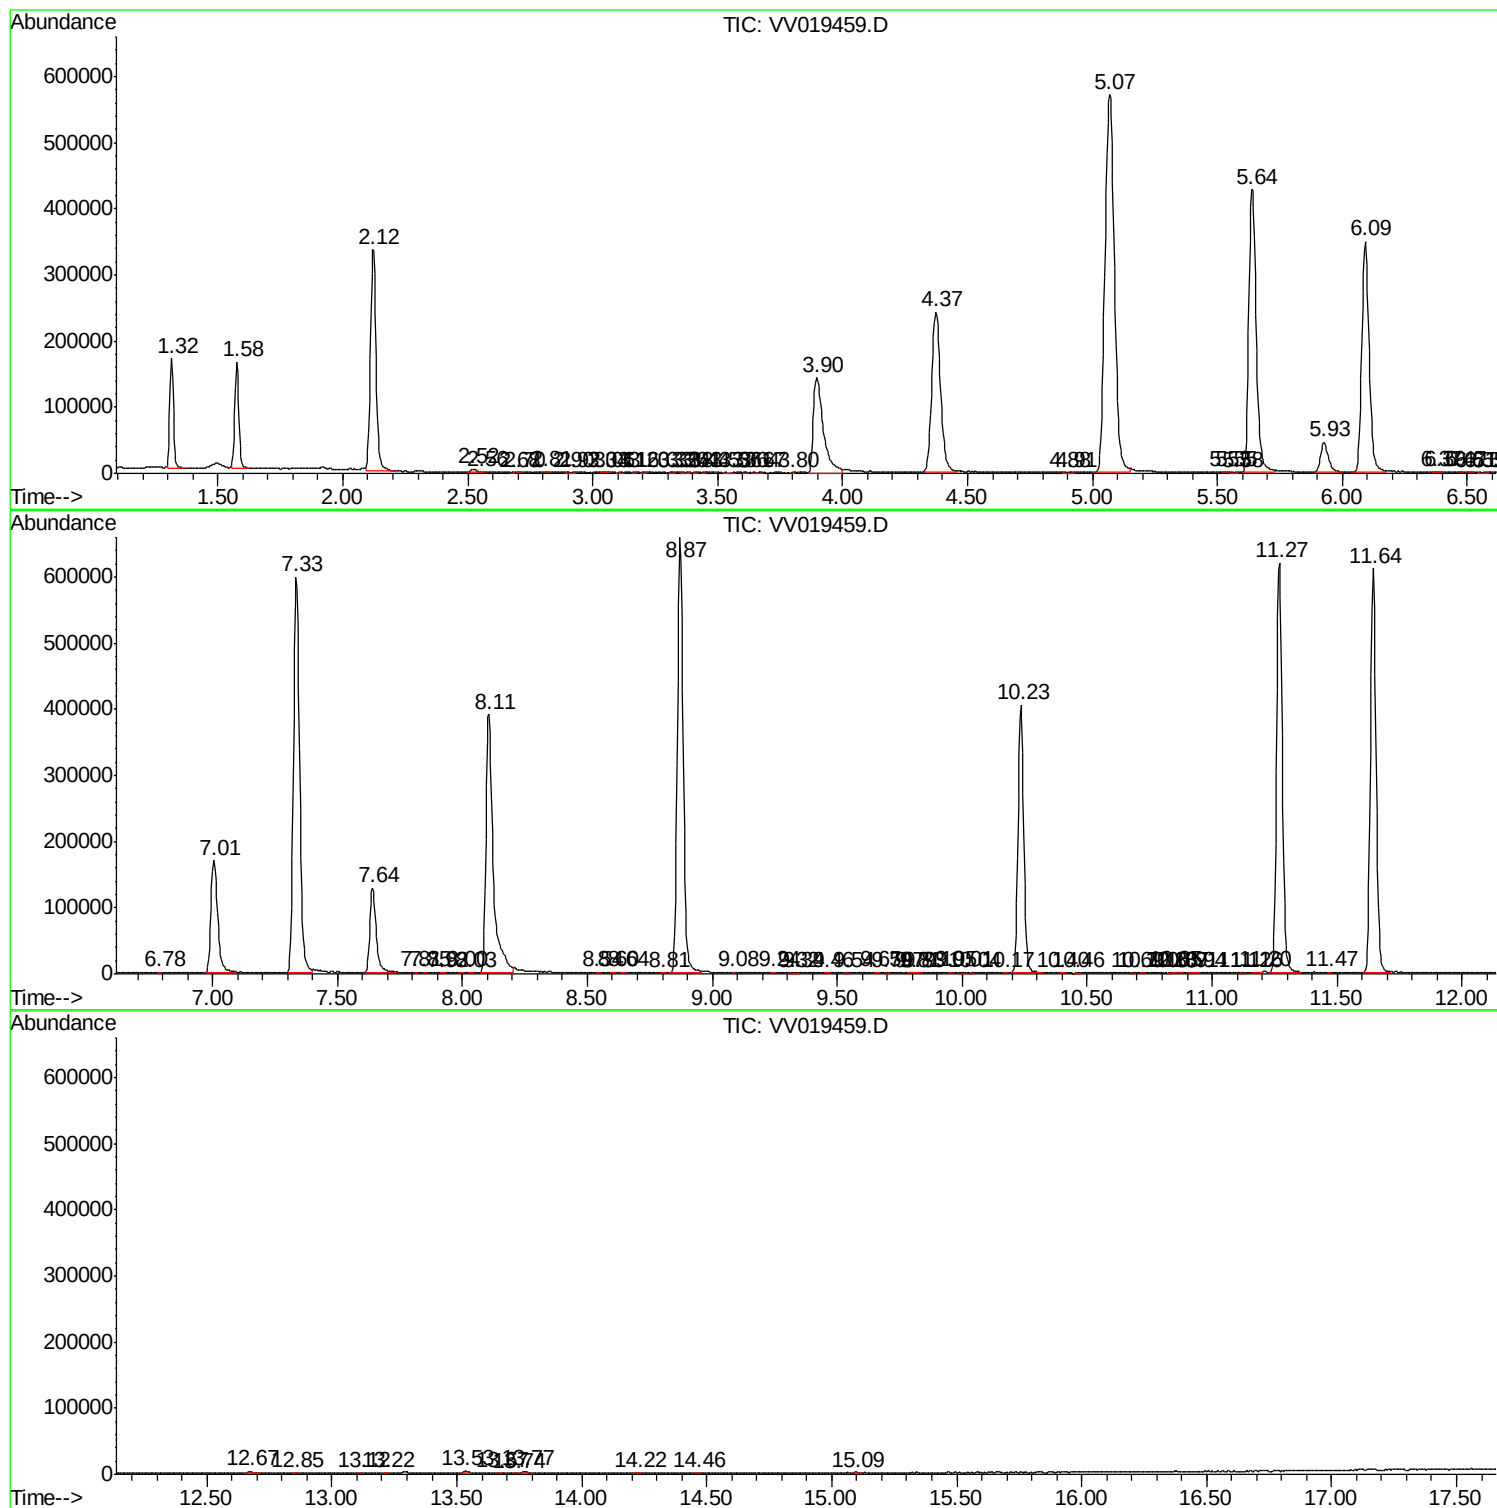

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120320\
Data File : VV019459.D
Acq On : 03 Dec 2020 16:02
Operator : SY/MD
Sample : VV1203WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK91

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120320\
Data File : VV019459.D
Acq On : 03 Dec 2020 16:02
Operator : SY/MD
Sample : VV1203WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK91

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc