

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019462.D
 Acq On : 03 Dec 2020 17:18
 Operator : SY/MD
 Sample : L4920-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	61	70	86	rVB	183339	220792	13.98%	1.917%
2	1.576	144	151	161	rVB	169459	192262	12.18%	1.669%
3	2.119	312	320	334	rBV	356743	522681	33.10%	4.538%
4	2.563	455	458	463	rVB4	933	778	0.05%	0.007%
5	2.605	468	471	474	rBV4	613	374	0.02%	0.003%
6	2.621	474	476	478	rBV3	1348	758	0.05%	0.007%
7	2.778	523	525	530	rBV4	908	622	0.04%	0.005%
8	2.826	536	540	543	rBV3	748	615	0.04%	0.005%
9	2.843	543	545	547	rBV2	412	257	0.02%	0.002%
10	2.881	555	557	562	rBV2	764	414	0.03%	0.004%
11	2.962	577	582	583	rBV4	625	471	0.03%	0.004%
12	3.048	607	609	613	rBV4	476	303	0.02%	0.003%
13	3.090	618	622	626	rVB3	796	628	0.04%	0.005%
14	3.126	631	633	635	rBV	698	339	0.02%	0.003%
15	3.154	639	642	643	rBV2	712	363	0.02%	0.003%
16	3.177	647	649	651	rBV2	462	245	0.02%	0.002%
17	3.225	662	664	667	rBV2	521	246	0.02%	0.002%
18	3.318	690	693	694	rBV2	620	211	0.01%	0.002%
19	3.360	702	706	708	rBV3	518	548	0.03%	0.005%
20	3.386	712	714	717	rVB2	350	177	0.01%	0.002%
21	3.415	719	723	728	rVB5	613	573	0.04%	0.005%
22	3.444	728	732	733	rBV4	432	335	0.02%	0.003%
23	3.521	752	756	760	rBV4	975	882	0.06%	0.008%
24	3.553	764	766	771	rBV2	633	375	0.02%	0.003%
25	3.579	771	774	775	rBV	775	440	0.03%	0.004%
26	3.627	787	789	793	rVB3	723	427	0.03%	0.004%
27	3.650	793	796	800	rVB2	500	451	0.03%	0.004%
28	3.675	800	804	807	rBV3	1042	1008	0.06%	0.009%
29	3.826	848	851	853	rBV	559	328	0.02%	0.003%
30	3.852	853	859	862	rBV4	845	1082	0.07%	0.009%
31	3.897	863	873	904	rBV	126809	346259	21.93%	3.006%
32	4.373	1004	1021	1043	rBV	254169	631408	39.99%	5.482%
33	4.714	1125	1127	1131	rVB4	1157	745	0.05%	0.006%
34	4.740	1132	1135	1137	rBV4	1057	607	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019462.D
 Acq On : 03 Dec 2020 17:18
 Operator : SY/MD
 Sample : L4920-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	4.769	1142	1144	1148	rVB2	483	362	0.02%	0.003%
36	4.797	1149	1153	1157	rBV4	844	619	0.04%	0.005%
37	4.833	1162	1164	1166	rBV3	863	475	0.03%	0.004%
38	4.936	1193	1196	1197	rBV3	624	337	0.02%	0.003%
39	5.071	1220	1238	1264	rBV2	607778	1578971	100.00%	13.710%
40	5.273	1299	1301	1304	rBV3	987	735	0.05%	0.006%
41	5.450	1352	1356	1357	rBV3	821	622	0.04%	0.005%
42	5.556	1386	1389	1393	rBV4	834	805	0.05%	0.007%
43	5.640	1403	1415	1444	rBV	434983	875660	55.46%	7.603%
44	5.923	1492	1503	1519	rBV2	61057	126167	7.99%	1.095%
45	6.090	1542	1555	1578	rBV	366571	740007	46.87%	6.425%
46	6.878	1799	1800	1804	rBV3	391	262	0.02%	0.002%
47	7.006	1829	1840	1859	rBV	186481	339361	21.49%	2.947%
48	7.334	1931	1942	1965	rBV	677585	1165000	73.78%	10.115%
49	7.640	2027	2037	2059	rBV	136525	240477	15.23%	2.088%
50	7.997	2144	2148	2153	rBV6	1339	1238	0.08%	0.011%
51	8.106	2172	2182	2220	rBV2	346273	738736	46.79%	6.414%
52	8.530	2312	2314	2317	rBV2	817	573	0.04%	0.005%
53	8.694	2362	2365	2368	rBV3	1128	935	0.06%	0.008%
54	8.871	2408	2420	2440	rBV	695775	1111558	70.40%	9.651%
55	9.254	2537	2539	2541	rBV2	711	296	0.02%	0.003%
56	9.350	2567	2569	2572	rBV3	659	452	0.03%	0.004%
57	9.395	2581	2583	2584	rBV	497	158	0.01%	0.001%
58	9.418	2588	2590	2591	rBV	555	213	0.01%	0.002%
59	9.485	2609	2611	2613	rBV2	540	310	0.02%	0.003%
60	9.518	2619	2621	2623	rBV	506	265	0.02%	0.002%
61	9.540	2623	2628	2630	rBV4	810	717	0.05%	0.006%
62	9.659	2664	2665	2669	rBV2	599	461	0.03%	0.004%
63	9.701	2675	2678	2681	rBV3	868	653	0.04%	0.006%
64	9.923	2743	2747	2749	rBV2	821	741	0.05%	0.006%
65	10.003	2770	2772	2773	rBV	435	220	0.01%	0.002%
66	10.141	2813	2815	2819	rVB4	812	432	0.03%	0.004%
67	10.235	2833	2844	2866	rVB	370455	580475	36.76%	5.040%
68	10.370	2884	2886	2889	rBV3	933	512	0.03%	0.004%
69	10.405	2890	2897	2904	rVB8	2855	4730	0.30%	0.041%
70	10.456	2910	2913	2919	rVB6	964	820	0.05%	0.007%
71	10.508	2925	2929	2931	rBV3	706	564	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019462.D
 Acq On : 03 Dec 2020 17:18
 Operator : SY/MD
 Sample : L4920-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

72	10.611	2956	2961	2962	rBV4	522	405	0.03%	0.004%
73	10.672	2977	2980	2984	rVB3	847	620	0.04%	0.005%
74	10.743	2998	3002	3006	rVB5	1037	879	0.06%	0.008%
75	10.765	3006	3009	3011	rBV2	806	584	0.04%	0.005%
76	10.820	3022	3026	3027	rBV	694	417	0.03%	0.004%
77	10.897	3048	3050	3052	rBV	364	139	0.01%	0.001%
78	10.923	3056	3058	3061	rBV3	479	267	0.02%	0.002%
79	10.955	3067	3068	3069	rBV	591	210	0.01%	0.002%
80	10.974	3072	3074	3077	rVV3	683	411	0.03%	0.004%
81	10.997	3078	3081	3087	rVB6	1297	1091	0.07%	0.009%
82	11.048	3096	3097	3099	rBV6	430	170	0.01%	0.001%
83	11.071	3099	3104	3105	rBV3	882	809	0.05%	0.007%
84	11.270	3154	3166	3187	rBV	652334	1004705	63.63%	8.724%
85	11.643	3270	3282	3303	rBV	668327	1057540	66.98%	9.182%
86	11.929	3368	3371	3373	rBV3	1129	743	0.05%	0.006%
87	12.128	3431	3433	3438	rBV2	667	492	0.03%	0.004%
88	12.707	3611	3613	3616	rBV2	1122	794	0.05%	0.007%
89	12.897	3670	3672	3677	rBV4	785	553	0.04%	0.005%
90	13.074	3724	3727	3732	rVB4	1025	706	0.04%	0.006%
91	13.157	3751	3753	3757	rBV	712	389	0.02%	0.003%
92	13.328	3802	3806	3808	rBV3	819	500	0.03%	0.004%
93	13.379	3818	3822	3827	rBV6	629	603	0.04%	0.005%
94	13.437	3838	3840	3845	rBV5	918	599	0.04%	0.005%
95	13.501	3857	3860	3862	rBV	551	323	0.02%	0.003%
96	13.514	3862	3864	3867	rVV3	695	302	0.02%	0.003%


Sum of corrected areas: 11517174

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120320\
Data File : VV019462.D
Acq On : 03 Dec 2020 17:18
Operator : SY/MD
Sample : L4920-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4C6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

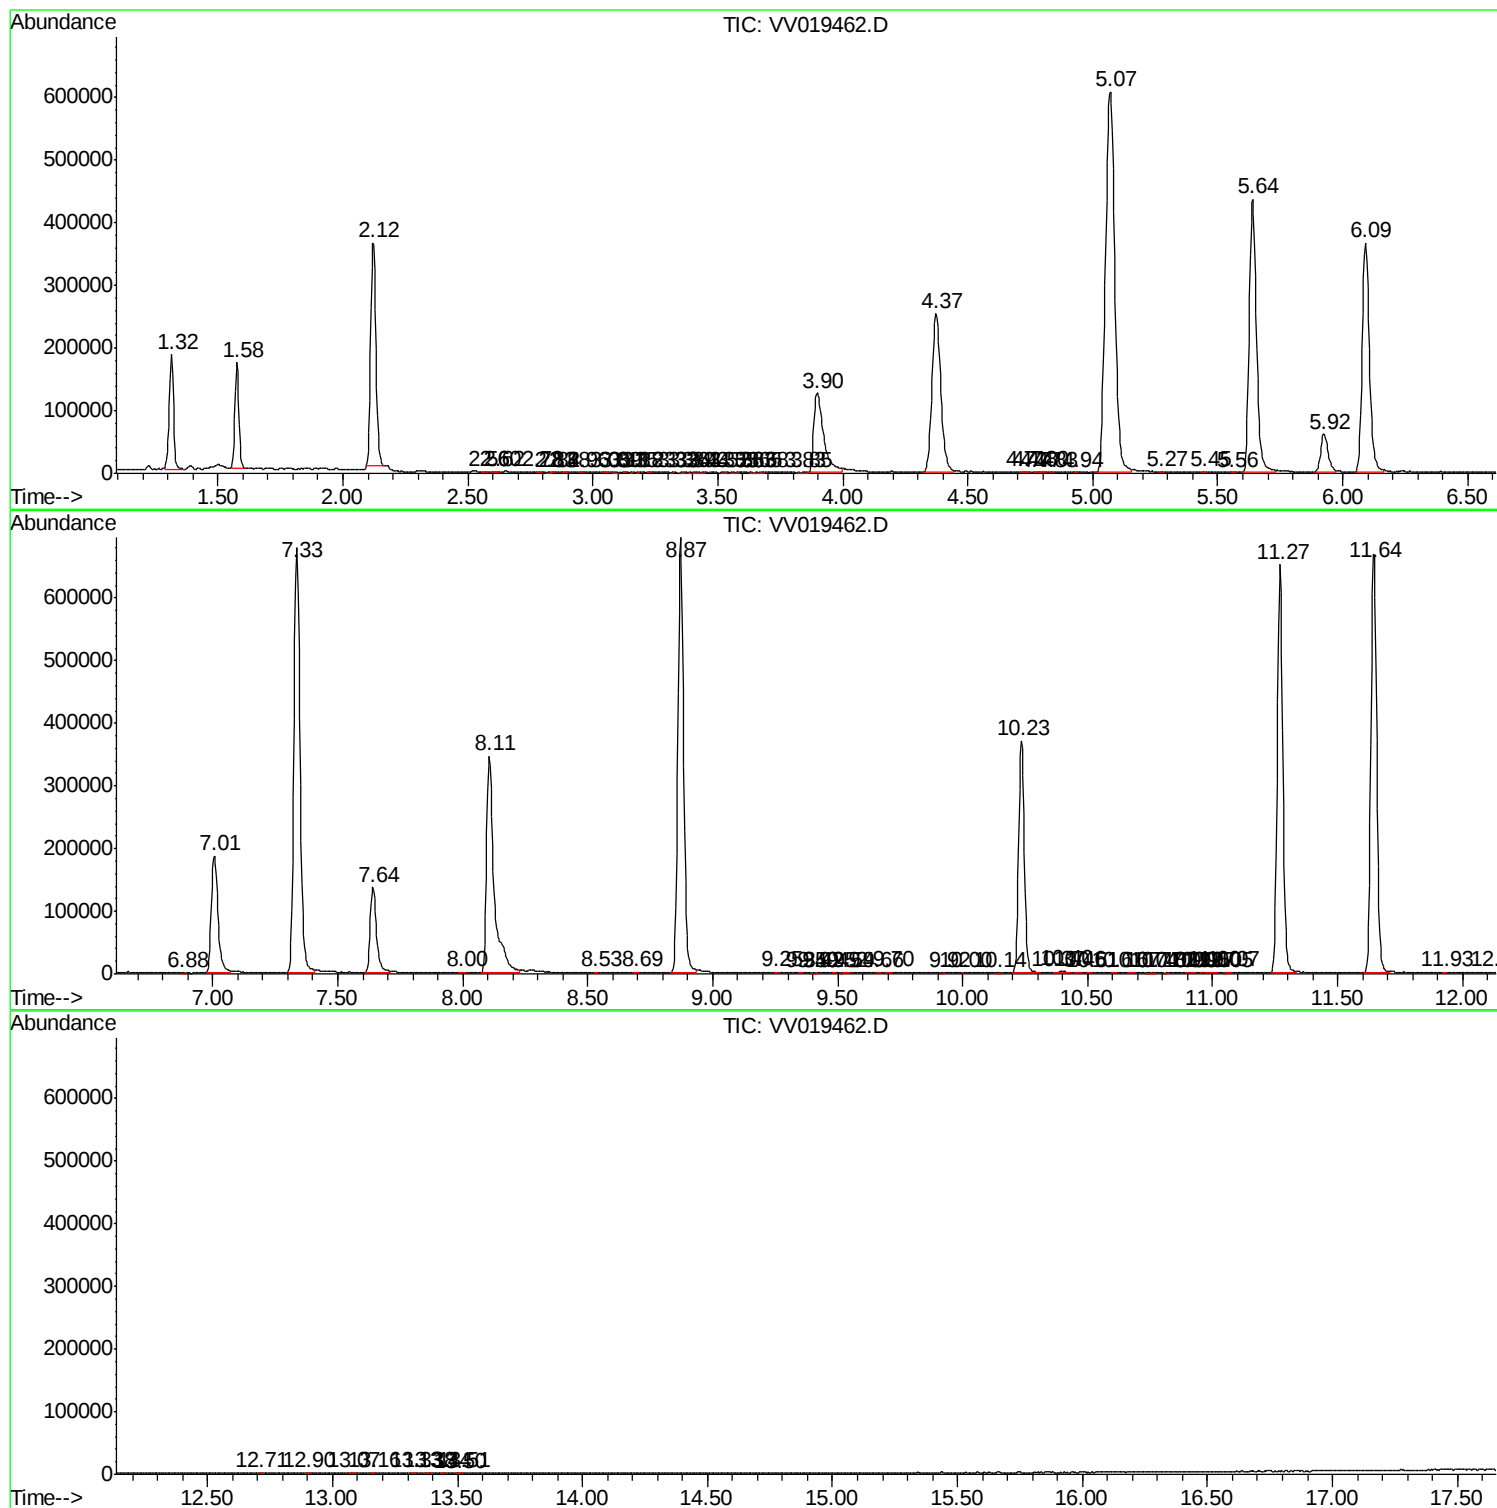

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120320\
Data File : VV019462.D
Acq On : 03 Dec 2020 17:18
Operator : SY/MD
Sample : L4920-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4C6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120320\
Data File : VV019462.D
Acq On : 03 Dec 2020 17:18
Operator : SY/MD
Sample : L4920-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4C6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc