

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019464.D
 Acq On : 03 Dec 2020 18:09
 Operator : SY/MD
 Sample : L4941-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	177452	180776	11.61%	1.595%
2	1.576	144	151	165	rVB	161648	186999	12.01%	1.650%
3	2.119	311	320	343	rVB	362259	544024	34.93%	4.799%
4	2.521	439	445	448	rBV6	1979	2471	0.16%	0.022%
5	2.601	466	470	471	rBV3	731	522	0.03%	0.005%
6	2.833	541	542	544	rBV	500	248	0.02%	0.002%
7	2.926	564	571	573	rBV4	928	1084	0.07%	0.010%
8	2.991	589	591	594	rVB2	802	329	0.02%	0.003%
9	3.016	594	599	602	rBV3	729	838	0.05%	0.007%
10	3.052	607	610	611	rBV	576	304	0.02%	0.003%
11	3.116	624	630	633	rBV4	863	1014	0.07%	0.009%
12	3.132	633	635	638	rVB3	644	347	0.02%	0.003%
13	3.171	644	647	649	rBV2	809	394	0.03%	0.003%
14	3.216	659	661	663	rVB	450	196	0.01%	0.002%
15	3.228	663	665	667	rBV2	395	242	0.02%	0.002%
16	3.335	696	698	700	rBV2	418	152	0.01%	0.001%
17	3.364	704	707	709	rVB3	491	206	0.01%	0.002%
18	3.396	716	717	720	rBV2	370	186	0.01%	0.002%
19	3.434	727	729	732	rVB4	620	337	0.02%	0.003%
20	3.454	732	735	737	rBV3	446	261	0.02%	0.002%
21	3.473	737	741	746	rVB4	639	464	0.03%	0.004%
22	3.708	812	814	815	rBV2	487	182	0.01%	0.002%
23	3.736	821	823	824	rBV2	236	67	0.00%	0.001%
24	3.759	828	830	833	rBV	398	212	0.01%	0.002%
25	3.781	833	837	840	rVB4	880	690	0.04%	0.006%
26	3.801	840	843	845	rBV3	669	425	0.03%	0.004%
27	3.820	845	849	853	rVB5	372	333	0.02%	0.003%
28	3.839	853	855	857	rBV2	350	210	0.01%	0.002%
29	3.894	861	872	902	rBV	124923	336109	21.58%	2.965%
30	4.373	1004	1021	1045	rBV	250260	621952	39.94%	5.486%
31	4.804	1152	1155	1157	rVB2	709	366	0.02%	0.003%
32	4.839	1157	1166	1167	rBV5	1001	1414	0.09%	0.012%
33	4.910	1184	1188	1191	rBV3	540	425	0.03%	0.004%
34	4.974	1205	1208	1209	rBV3	540	328	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019464.D
 Acq On : 03 Dec 2020 18:09
 Operator : SY/MD
 Sample : L4941-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	5.068	1220	1237	1268	rBV2	599432	1557350	100.00%	13.737%
36	5.537	1381	1383	1388	rBV6	911	699	0.04%	0.006%
37	5.637	1402	1414	1443	rBV	422153	861438	55.31%	7.599%
38	5.923	1492	1503	1525	rBV3	56922	123394	7.92%	1.088%
39	6.090	1541	1555	1577	rBV	356293	726212	46.63%	6.406%
40	6.306	1619	1622	1624	rBV2	775	536	0.03%	0.005%
41	6.386	1645	1647	1648	rBV	677	290	0.02%	0.003%
42	6.415	1653	1656	1657	rBV3	552	328	0.02%	0.003%
43	6.444	1663	1665	1671	rVB5	961	582	0.04%	0.005%
44	6.469	1671	1673	1677	rVB5	679	484	0.03%	0.004%
45	6.489	1677	1679	1682	rBV2	865	559	0.04%	0.005%
46	6.547	1694	1697	1699	rBV4	859	473	0.03%	0.004%
47	6.605	1712	1715	1716	rBV3	538	205	0.01%	0.002%
48	6.894	1800	1805	1806	rVB3	549	440	0.03%	0.004%
49	6.910	1806	1810	1812	rBV3	746	552	0.04%	0.005%
50	7.006	1828	1840	1858	rBV	178289	328970	21.12%	2.902%
51	7.334	1930	1942	1964	rBV	670038	1148316	73.74%	10.129%
52	7.640	2027	2037	2056	rBV	134663	233123	14.97%	2.056%
53	8.106	2172	2182	2220	rBV2	337391	720221	46.25%	6.353%
54	8.666	2354	2356	2357	rBV2	613	273	0.02%	0.002%
55	8.784	2387	2393	2397	rBV6	1004	1212	0.08%	0.011%
56	8.871	2408	2420	2445	rBV	671200	1092614	70.16%	9.638%
57	9.289	2546	2550	2551	rBV	758	612	0.04%	0.005%
58	9.383	2576	2579	2581	rBV2	506	334	0.02%	0.003%
59	9.530	2623	2625	2627	rBV2	486	208	0.01%	0.002%
60	9.585	2632	2642	2643	rBV5	1711	1778	0.11%	0.016%
61	9.665	2664	2667	2674	rVB6	982	806	0.05%	0.007%
62	9.897	2735	2739	2742	rBV5	912	869	0.06%	0.008%
63	10.032	2778	2781	2784	rBV4	847	509	0.03%	0.004%
64	10.048	2784	2786	2788	rVV2	369	218	0.01%	0.002%
65	10.067	2791	2792	2794	rBV2	363	139	0.01%	0.001%
66	10.093	2797	2800	2801	rBV3	939	483	0.03%	0.004%
67	10.103	2801	2803	2806	rVB2	700	371	0.02%	0.003%
68	10.138	2812	2814	2815	rBV	448	244	0.02%	0.002%
69	10.161	2818	2821	2822	rBV2	664	367	0.02%	0.003%
70	10.193	2829	2831	2832	rBV	691	235	0.02%	0.002%
71	10.235	2832	2844	2861	rBV	365139	580476	37.27%	5.120%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019464.D
 Acq On : 03 Dec 2020 18:09
 Operator : SY/MD
 Sample : L4941-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

72	10.492	2922	2924	2926	rBV2	690	419	0.03%	0.004%
73	10.566	2943	2947	2951	rVB3	896	721	0.05%	0.006%
74	10.624	2964	2965	2966	rBV3	389	131	0.01%	0.001%
75	10.746	3001	3003	3004	rVB2	421	147	0.01%	0.001%
76	10.755	3004	3006	3007	rBV	252	83	0.01%	0.001%
77	10.813	3019	3024	3027	rBV2	1301	1208	0.08%	0.011%
78	11.019	3086	3088	3091	rBV3	683	417	0.03%	0.004%
79	11.083	3106	3108	3109	rBV3	675	324	0.02%	0.003%
80	11.141	3124	3126	3128	rBV3	480	169	0.01%	0.001%
81	11.270	3153	3166	3188	rBV	643055	1002464	64.37%	8.843%
82	11.646	3271	3283	3304	rBV	666220	1052572	67.59%	9.285%
83	11.977	3384	3386	3390	rVB2	838	511	0.03%	0.005%
84	11.997	3390	3392	3396	rVB3	728	439	0.03%	0.004%
85	12.099	3421	3424	3427	rBV3	558	471	0.03%	0.004%
86	12.283	3477	3481	3483	rBV4	759	524	0.03%	0.005%
87	12.579	3571	3573	3579	rVB2	791	714	0.05%	0.006%
88	12.604	3579	3581	3583	rVB2	701	324	0.02%	0.003%
89	12.624	3583	3587	3590	rBV3	536	521	0.03%	0.005%
90	12.952	3687	3689	3693	rBV4	559	394	0.03%	0.003%
91	13.045	3714	3718	3722	rBV4	777	884	0.06%	0.008%
92	13.064	3722	3724	3730	rVB5	1221	1188	0.08%	0.010%
93	13.096	3730	3734	3736	rBV2	879	800	0.05%	0.007%
94	13.746	3934	3936	3940	rBV3	752	595	0.04%	0.005%
95	13.842	3964	3966	3970	rBV2	558	373	0.02%	0.003%
96	13.987	4010	4011	4012	rBV	614	197	0.01%	0.002%


Sum of corrected areas: 11336617

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120320\
Data File : VV019464.D
Acq On : 03 Dec 2020 18:09
Operator : SY/MD
Sample : L4941-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BH8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

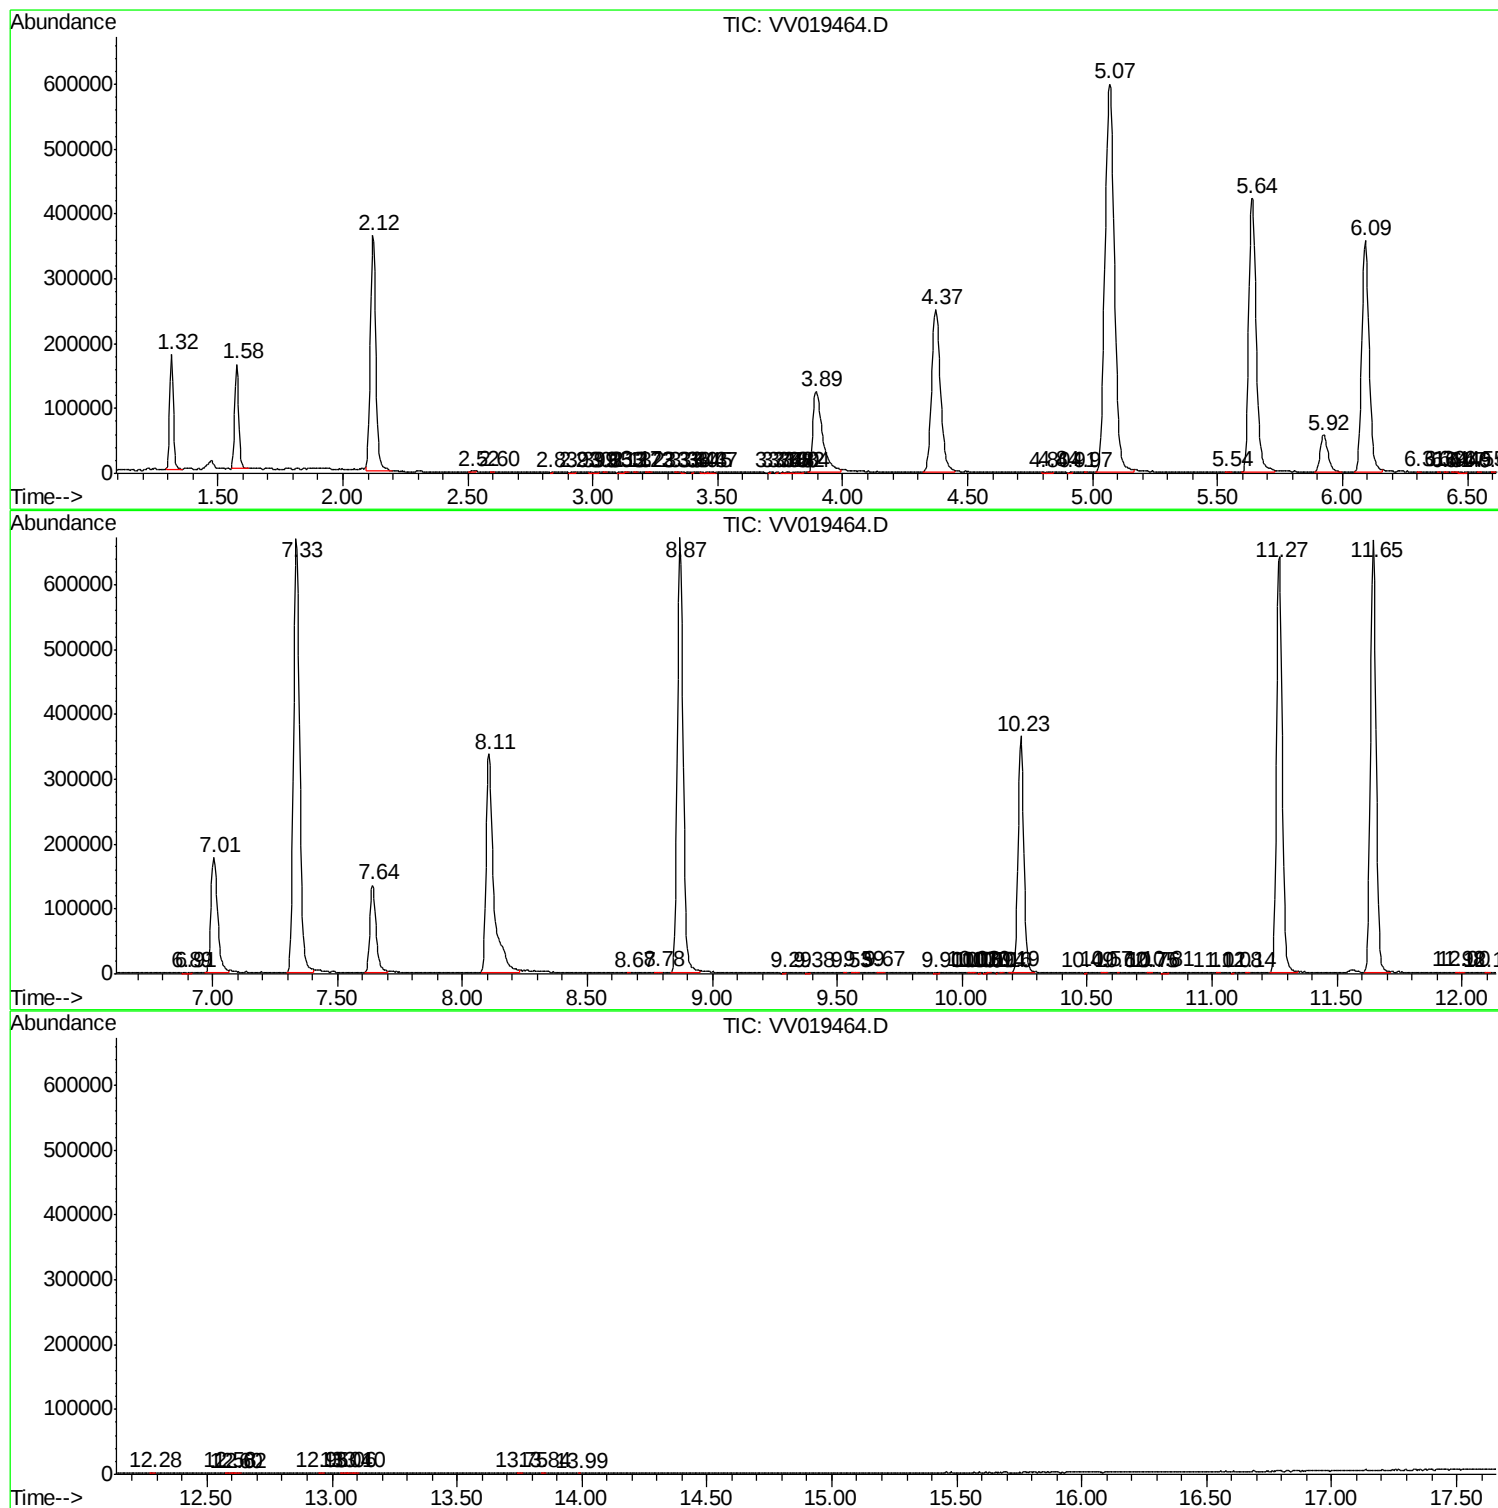

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120320\
Data File : VV019464.D
Acq On : 03 Dec 2020 18:09
Operator : SY/MD
Sample : L4941-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BH8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120320\
Data File : VV019464.D
Acq On : 03 Dec 2020 18:09
Operator : SY/MD
Sample : L4941-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BH8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc