

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019469.D
 Acq On : 03 Dec 2020 20:31
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	172540	173506	11.22%	1.553%
2	1.573	144	150	161	rVB	163124	186407	12.05%	1.668%
3	2.119	311	320	341	rVB	350799	520517	33.65%	4.658%
4	2.479	431	432	437	rBV3	711	597	0.04%	0.005%
5	2.624	473	477	480	rBV4	1215	1172	0.08%	0.010%
6	2.765	519	521	522	rBV	551	282	0.02%	0.003%
7	2.798	529	531	532	rBV	771	343	0.02%	0.003%
8	2.846	544	546	547	rBV	523	209	0.01%	0.002%
9	2.965	579	583	585	rVB3	850	570	0.04%	0.005%
10	2.984	587	589	593	rBV	594	432	0.03%	0.004%
11	3.055	606	611	614	rBV5	876	1074	0.07%	0.010%
12	3.196	654	655	659	rBV2	321	220	0.01%	0.002%
13	3.219	659	662	666	rVB2	730	444	0.03%	0.004%
14	3.290	681	684	685	rBV2	627	390	0.03%	0.003%
15	3.367	704	708	713	rBV4	751	682	0.04%	0.006%
16	3.386	713	714	716	rVB	568	161	0.01%	0.001%
17	3.412	720	722	726	rVB3	595	361	0.02%	0.003%
18	3.431	726	728	734	rBV2	802	773	0.05%	0.007%
19	3.502	749	750	751	rBV	425	102	0.01%	0.001%
20	3.524	755	757	758	rBV	513	142	0.01%	0.001%
21	3.566	767	770	773	rBV2	617	512	0.03%	0.005%
22	3.579	773	774	780	rVB	633	352	0.02%	0.003%
23	3.614	782	785	789	rVB2	972	729	0.05%	0.007%
24	3.637	789	792	798	rBV4	610	755	0.05%	0.007%
25	3.663	798	800	801	rBV	360	165	0.01%	0.001%
26	3.701	808	812	815	rBV4	1100	903	0.06%	0.008%
27	3.749	824	827	830	rVB5	665	399	0.03%	0.004%
28	3.781	830	837	838	rBV4	647	666	0.04%	0.006%
29	3.849	856	858	859	rVB	308	109	0.01%	0.001%
30	3.891	859	871	900	rBV2	135767	373058	24.12%	3.338%
31	4.206	968	969	971	rBV	983	447	0.03%	0.004%
32	4.370	1006	1020	1047	rVB	246942	608368	39.33%	5.444%
33	4.740	1133	1135	1137	rBV3	424	192	0.01%	0.002%
34	4.830	1159	1163	1167	rBV4	739	695	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
 Data File : VV019469.D
 Acq On : 03 Dec 2020 20:31
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	4.891	1179	1182	1188	rBV6	932	959	0.06%	0.009%
36	4.978	1204	1209	1210	rBV3	592	413	0.03%	0.004%
37	5.064	1219	1236	1269	rBV2	592653	1546883	100.00%	13.843%
38	5.572	1387	1394	1397	rVB4	773	811	0.05%	0.007%
39	5.589	1397	1399	1400	rBV	744	373	0.02%	0.003%
40	5.637	1401	1414	1436	rBV	420965	838629	54.21%	7.505%
41	5.923	1493	1503	1523	rVB2	48145	97982	6.33%	0.877%
42	6.087	1541	1554	1577	rBV	349505	722917	46.73%	6.469%
43	6.408	1650	1654	1655	rBV3	894	623	0.04%	0.006%
44	6.579	1705	1707	1709	rBV3	631	305	0.02%	0.003%
45	6.794	1770	1774	1777	rBV4	1286	1125	0.07%	0.010%
46	6.859	1792	1794	1795	rBV2	882	382	0.02%	0.003%
47	6.916	1810	1812	1815	rBV2	575	295	0.02%	0.003%
48	6.936	1815	1818	1819	rBV	625	315	0.02%	0.003%
49	7.003	1828	1839	1858	rBV	180576	325806	21.06%	2.916%
50	7.334	1930	1942	1966	rBV	649732	1107820	71.62%	9.914%
51	7.637	2026	2036	2061	rBV	131753	233107	15.07%	2.086%
52	7.994	2140	2147	2161	rVB6	8266	15514	1.00%	0.139%
53	8.103	2171	2181	2211	rBV2	346480	721064	46.61%	6.453%
54	8.678	2356	2360	2364	rVB4	945	748	0.05%	0.007%
55	8.701	2364	2367	2370	rBV5	900	841	0.05%	0.008%
56	8.820	2402	2404	2407	rBV3	818	359	0.02%	0.003%
57	8.871	2407	2420	2444	rBV	651534	1080518	69.85%	9.669%
58	9.357	2569	2571	2573	rBV2	633	336	0.02%	0.003%
59	9.466	2601	2605	2609	rBV5	779	763	0.05%	0.007%
60	9.511	2616	2619	2621	rBV2	690	502	0.03%	0.004%
61	9.662	2664	2666	2670	rBV2	793	599	0.04%	0.005%
62	9.739	2688	2690	2691	rBV	375	146	0.01%	0.001%
63	9.797	2706	2708	2711	rVB3	413	157	0.01%	0.001%
64	9.823	2714	2716	2717	rBV2	412	134	0.01%	0.001%
65	10.087	2796	2798	2799	rBV2	524	197	0.01%	0.002%
66	10.235	2832	2844	2863	rBV	390216	620724	40.13%	5.555%
67	10.386	2889	2891	2892	rBV2	605	155	0.01%	0.001%
68	10.463	2914	2915	2916	rBV	322	112	0.01%	0.001%
69	10.633	2966	2968	2969	rBV2	619	208	0.01%	0.002%
70	10.675	2977	2981	2985	rBV5	1054	954	0.06%	0.009%
71	10.836	3027	3031	3034	rBV3	694	655	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120320\
Data File : VV019469.D
Acq On : 03 Dec 2020 20:31
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Title : VOC Analysis

72	10.855	3034	3037	3039	rBV2	489	358	0.02%	0.003%
73	11.000	3078	3082	3083	rBV2	843	595	0.04%	0.005%
74	11.119	3116	3119	3120	rBV2	451	209	0.01%	0.002%
75	11.270	3154	3166	3190	rBV	615560	962760	62.24%	8.616%
76	11.534	3246	3248	3251	rBV2	598	290	0.02%	0.003%
77	11.643	3270	3282	3308	rBV	637200	1008391	65.19%	9.024%
78	12.257	3469	3473	3474	rBV2	576	394	0.03%	0.004%
79	12.588	3574	3576	3579	rBV3	789	459	0.03%	0.004%
80	12.900	3671	3673	3675	rBV2	708	401	0.03%	0.004%
81	12.977	3695	3697	3698	rBV	593	224	0.01%	0.002%
82	13.466	3846	3849	3853	rBV3	982	742	0.05%	0.007%
83	13.675	3912	3914	3920	rBV5	793	751	0.05%	0.007%


Sum of corrected areas: 11174739

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120320\
Data File : VV019469.D
Acq On : 03 Dec 2020 20:31
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

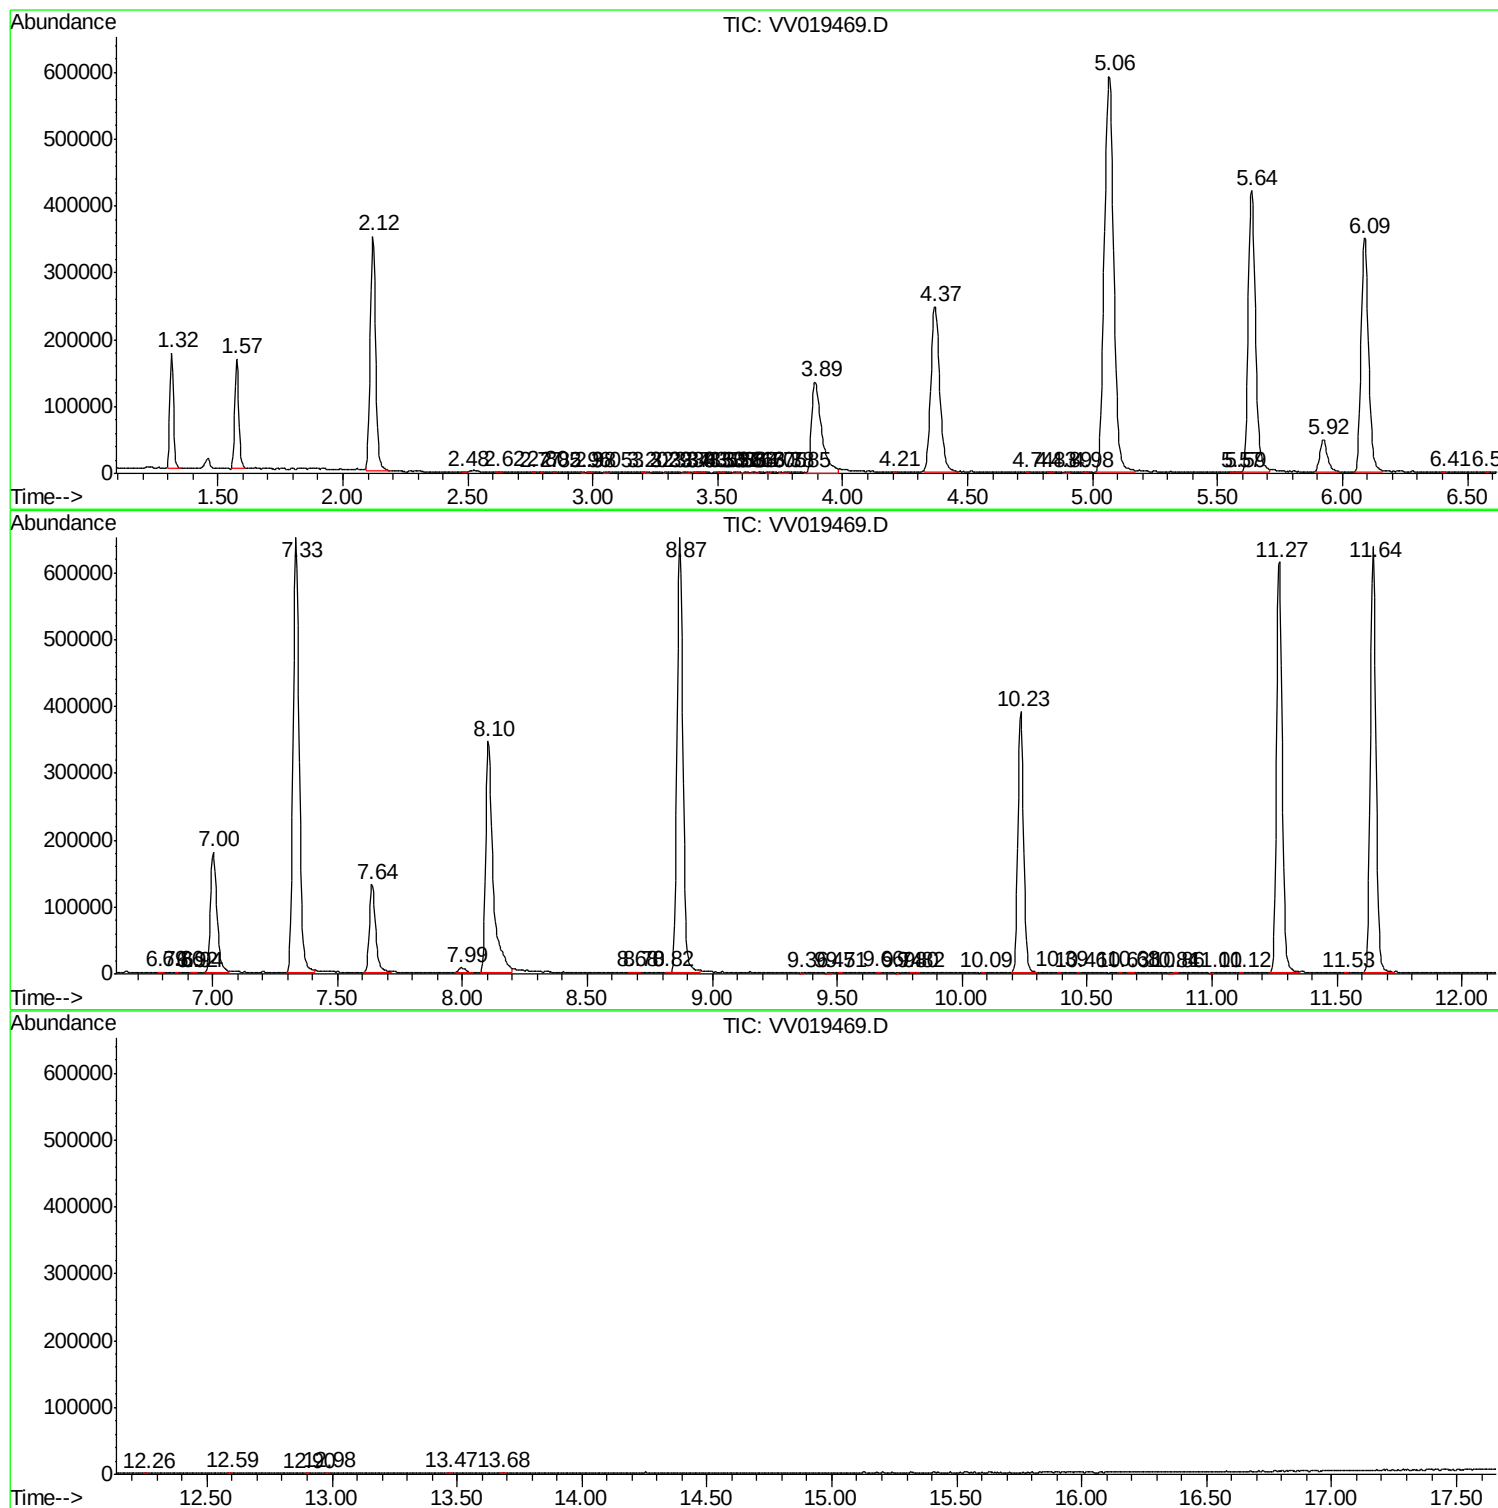

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120320\
Data File : VV019469.D
Acq On : 03 Dec 2020 20:31
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK80

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120320\
Data File : VV019469.D
Acq On : 03 Dec 2020 20:31
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK80

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc