


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120320\
 Data File : VV019457.D
 Acq On : 03 Dec 2020 13:59
 Operator : SY/MD
 Sample : BFB99
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB99

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 04 08:04:03 2020

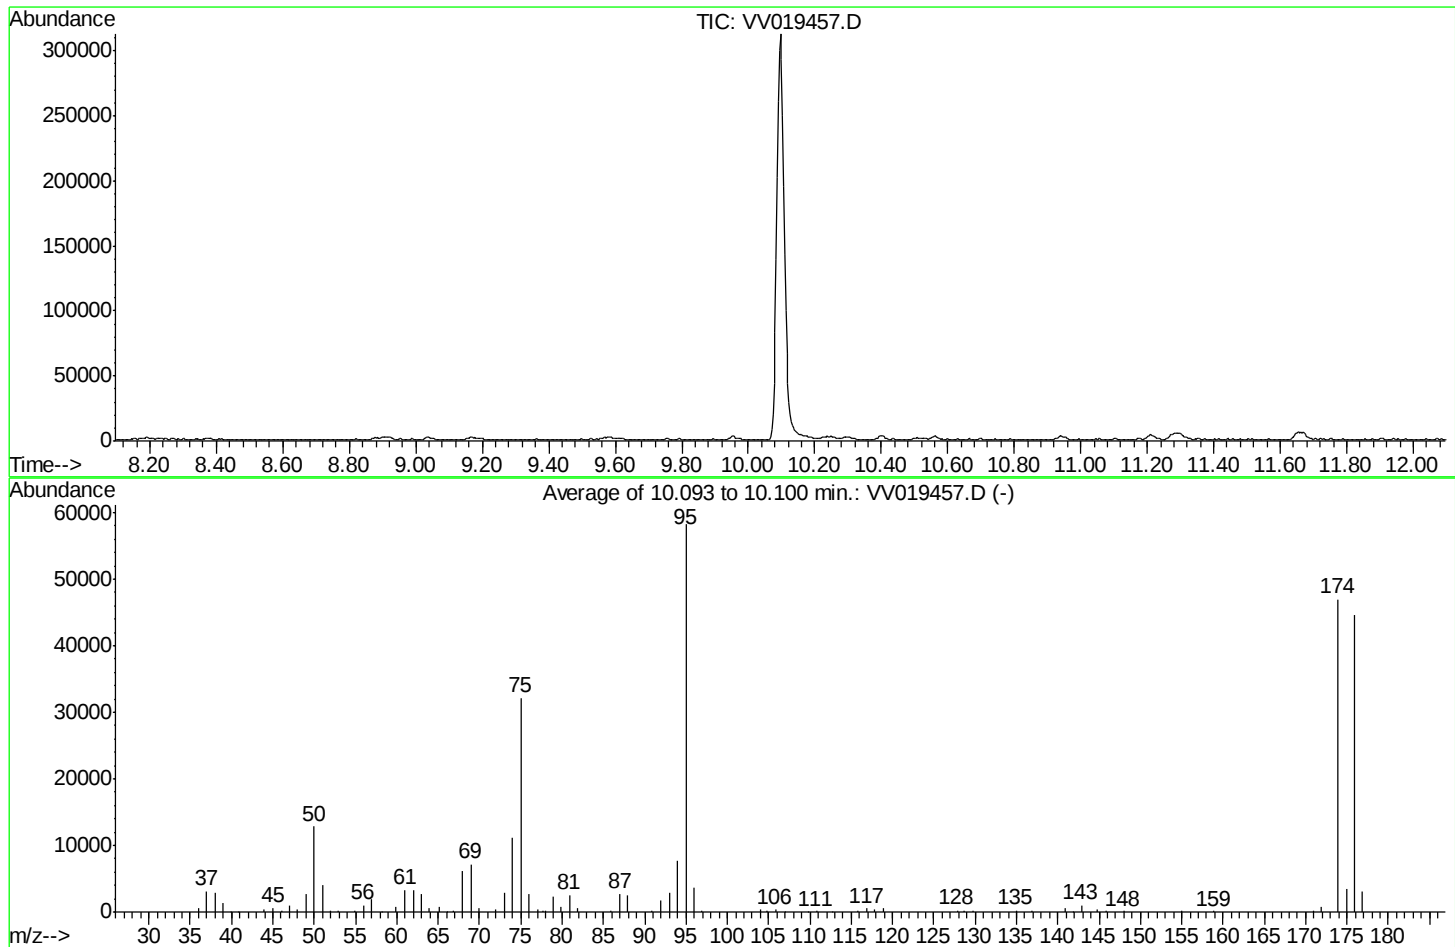

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	12861	PASS
75	95	30	80	55.2	32165	PASS
95	95	100	100	100.0	58240	PASS
96	95	5	9	6.4	3702	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.6	46930	PASS
175	174	5	9	7.3	3446	PASS
176	174	95	101	95.2	44666	PASS
177	176	5	9	6.8	3057	PASS

m/z	Abundance
35.90	642.0
37.00	3299.0
38.00	2972.0
39.00	1299.0
39.80	274.0
40.80	104.0
42.70	101.0
44.00	946.0
45.10	629.0
46.10	154.0
47.00	929.0
48.00	427.0
49.00	2712.0
50.00	12645.0
51.00	4250.0
52.00	330.0
53.00	210.0
54.90	195.0
56.00	1066.0
57.00	1829.0
59.90	799.0
61.00	3467.0
62.00	3377.0
63.00	2772.0
64.00	583.0
65.10	826.0
66.00	133.0
66.90	211.0
68.00	6195.0
69.00	7131.0
70.00	563.0
72.00	397.0
73.00	3011.0
74.00	11303.0
75.00	32816.0
76.00	2707.0
77.00	374.0
77.80	230.0
78.00	232.0
78.90	2368.0
79.90	683.0
80.90	2585.0
81.90	539.0
85.90	152.0
87.00	2540.0
87.90	2588.0
90.90	292.0
92.00	1729.0
93.00	2772.0
94.00	7853.0
95.00	57952.0
96.00	3770.0
96.90	177.0
103.90	331.0
104.80	136.0
105.80	330.0
110.80	130.0
115.80	261.0
116.90	575.0
117.80	280.0
118.90	489.0
127.80	264.0
128.60	111.0
129.80	241.0
135.00	196.0
136.80	116.0
140.90	701.0
141.80	103.0
142.90	859.0
144.80	367.0
146.00	123.0
147.90	145.0
155.00	142.0
158.90	132.0
170.90	151.0
172.00	777.0
173.90	45552.0
174.90	3434.0
175.90	43232.0
176.90	3050.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	609.0
37.00	3256.0
38.00	2972.0
39.00	1301.0
39.90	264.0
44.00	981.0
45.00	611.0
46.00	128.0
47.00	899.0
48.00	502.0
49.00	2779.0
50.00	13312.0
51.00	4166.0
52.00	317.0
53.00	178.0
55.00	171.0
56.00	1101.0
57.00	1904.0
58.10	108.0
59.90	849.0
61.00	3495.0
62.00	3269.0
63.00	2716.0
63.90	546.0
65.10	750.0
66.00	105.0
66.90	236.0
68.00	6333.0
69.00	7458.0
70.00	668.0
72.00	412.0
73.00	3049.0
74.00	11717.0
75.00	33280.0
76.00	2856.0
77.00	349.0
77.70	255.0
78.00	220.0
78.90	2496.0
79.80	730.0
80.90	2633.0
81.90	573.0
85.80	165.0
87.00	2899.0
87.90	2581.0
90.90	301.0
92.00	1800.0
93.00	3040.0
94.00	7835.0
95.00	60360.0
96.00	3774.0
96.90	162.0
104.00	324.0
104.90	125.0
105.90	415.0
106.90	111.0
109.80	130.0
110.80	136.0
115.90	285.0
116.90	575.0
117.80	351.0
118.90	545.0
127.80	288.0
128.60	144.0
129.80	260.0
134.90	212.0
136.70	105.0
136.90	107.0
141.00	678.0
141.80	112.0
142.90	1043.0
144.80	417.0
145.90	143.0
148.00	171.0
155.00	136.0
158.90	156.0
170.90	183.0
171.90	785.0
173.90	48480.0
174.90	3574.0
175.90	46128.0
176.90	3197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	642.0
37.00	2922.0
38.00	2704.0
39.00	1329.0
40.00	276.0
44.00	942.0
45.00	551.0
46.00	124.0
47.00	838.0
48.00	473.0
49.00	2522.0
50.00	12626.0
51.00	3646.0
52.00	221.0
52.90	146.0
55.00	145.0
56.00	1003.0
57.00	1839.0
58.20	123.0
59.90	757.0
61.00	3113.0
62.00	2968.0
63.00	2356.0
63.90	530.0
65.10	615.0
66.80	211.0
68.00	5875.0
69.00	6895.0
70.00	680.0
72.00	417.0
73.00	2768.0
74.00	10743.0
75.00	30400.0
76.00	2738.0
77.00	329.0
77.70	244.0
78.10	212.0
78.90	2327.0
79.80	724.0
80.90	2417.0
81.90	563.0
85.80	169.0
87.00	2838.0
87.90	2217.0
90.90	270.0
92.00	1640.0
93.00	2932.0
94.00	7222.0
95.00	56408.0
96.00	3562.0
97.00	165.0
103.90	304.0
104.90	121.0
105.90	391.0
106.90	129.0
109.80	125.0
110.80	140.0
112.70	106.0
115.90	283.0
116.90	491.0
117.80	334.0
118.90	479.0
127.80	224.0
128.60	132.0
129.80	252.0
134.90	208.0
136.90	115.0
141.00	619.0
142.90	1052.0
144.80	410.0
145.80	123.0
148.00	180.0
155.00	108.0
158.90	122.0
170.90	168.0
171.80	833.0
173.90	46760.0
174.90	3331.0
175.90	44640.0
176.90	2926.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

Scan 2789 (10.058 min): VV019457.D
BFB99

m/z	Abundance
36.40	121.0
39.90	268.0
42.70	143.0
43.90	587.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99