

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120324\
 Data File : VV038405.D
 Acq On : 03 Dec 2024 14:01
 Operator : SY/MD
 Sample : VSTDCCC0.5EC
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 03 21:48:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 03 21:43:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8101	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	8116	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3810	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	4085	0.546	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 110.000%			
4) 1,2-Dichloroethane-d4	4.969	65	3370	0.587	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 118.000%			
7) 1,2-Dichloropropane-d6	5.995	67	4129	0.543	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 108.000%			
8) Toluene-d8	7.253	98	8926	0.501	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 100.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3396	0.575	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 116.000%			
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	5057	0.527	ug/L	98
6) Trichloroethene	5.852	95	3422	0.497	ug/L	98
9) 1,2-Dibromoethane	8.305	107	2363	0.532	ug/L	99
12) 1,2,3-Trichloropropane	10.197	75	2103	0.530	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.357	75	369	0.542	ug/L #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120324\
Data File : VV038405.D
Acq On : 03 Dec 2024 14:01
Operator : SY/MD
Sample : VSTDCCC0.5EC
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 03 21:48:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 03 21:43:44 2024
Response via : Initial Calibration

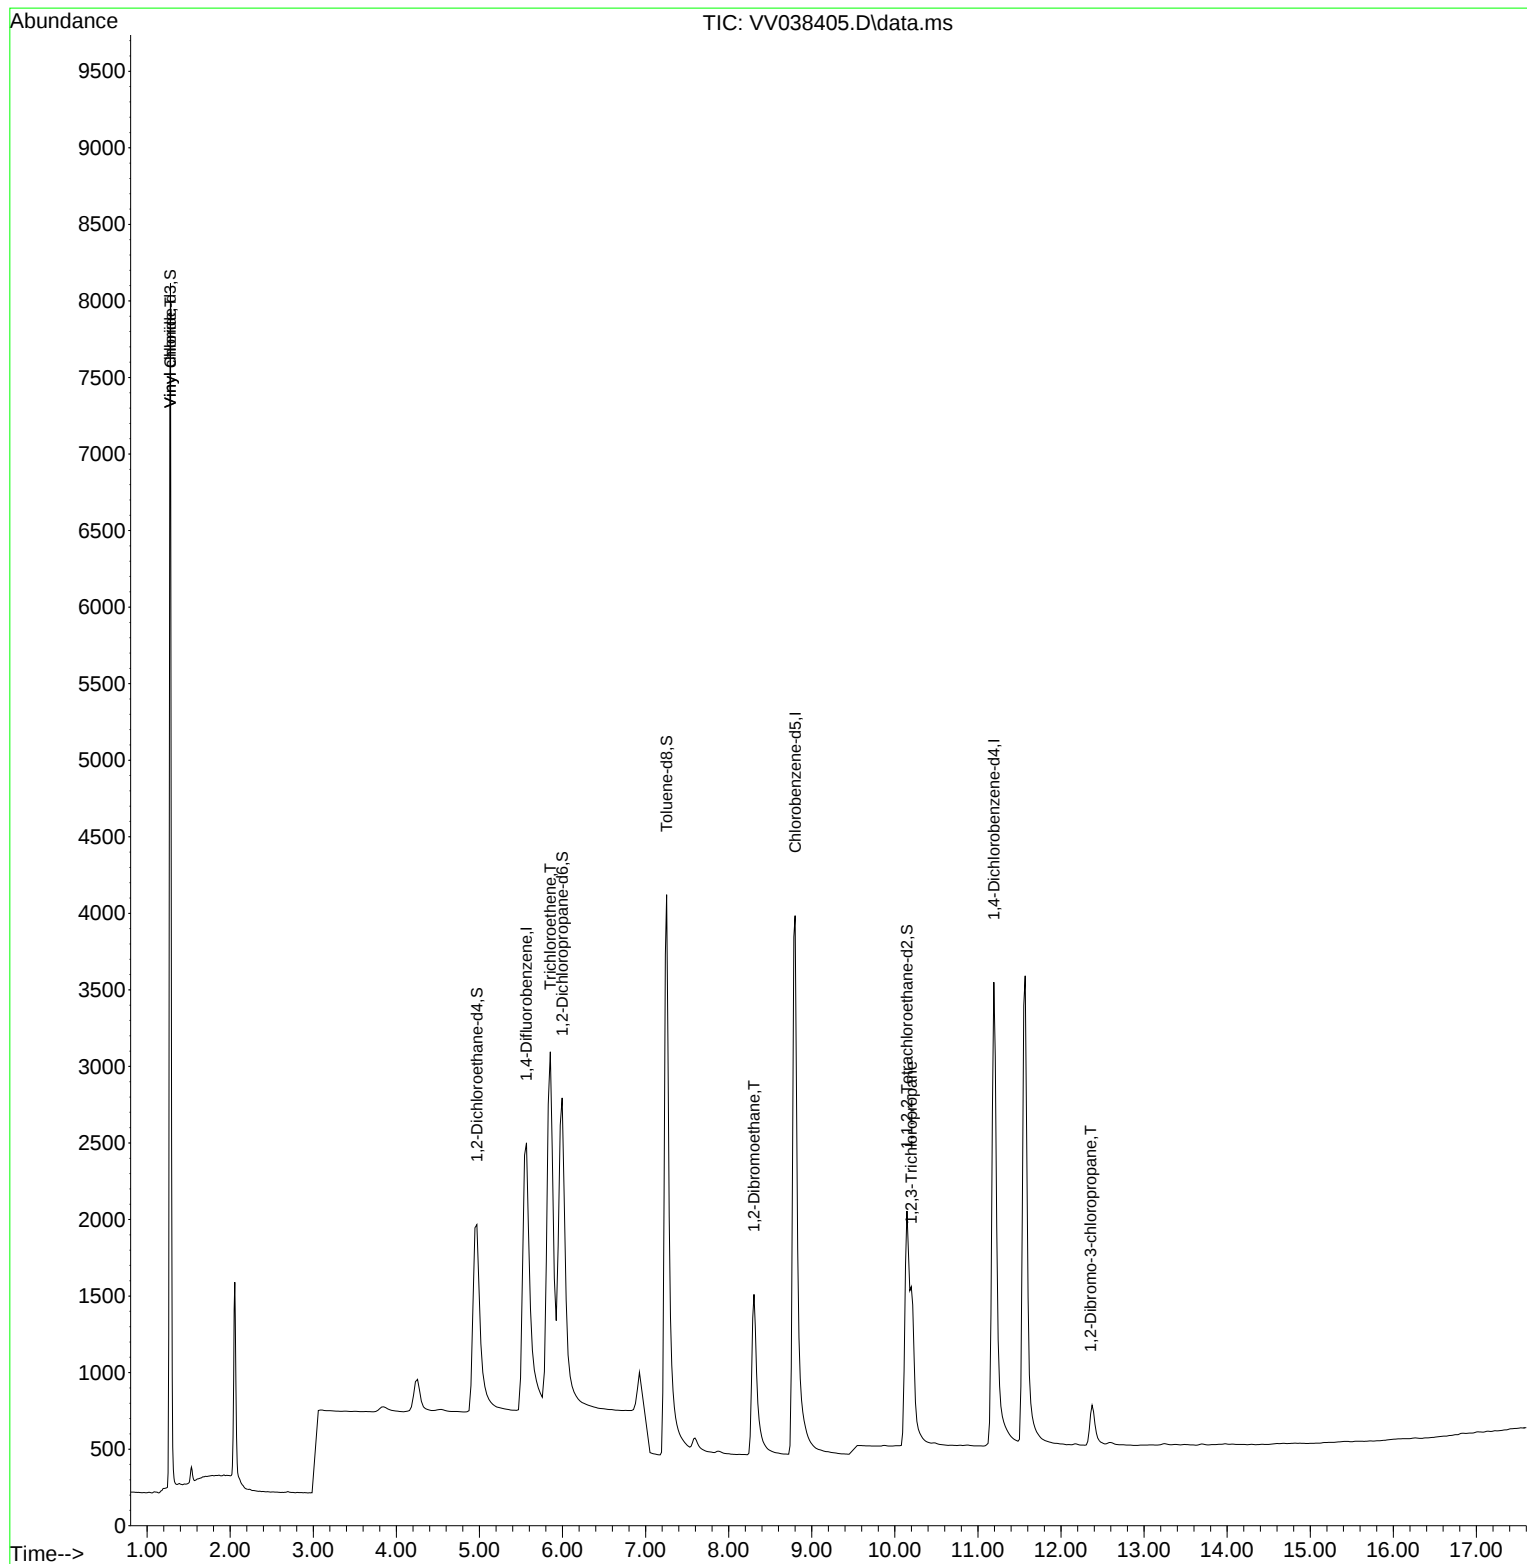

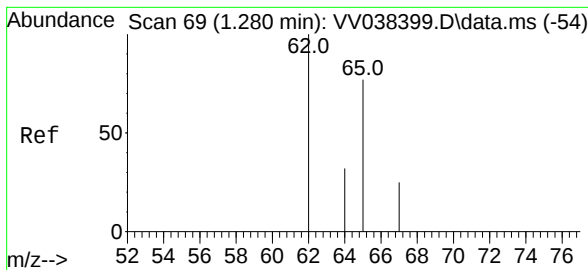

#3

Vinyl chloride

Concen: 0.527 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV038405.D

Acq: 03 Dec 2024 14:01

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 62 Resp: 5057

Ion Ratio Lower Upper

62 100

64 34.8 23.4 43.4

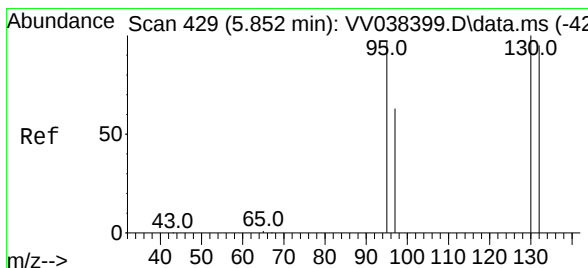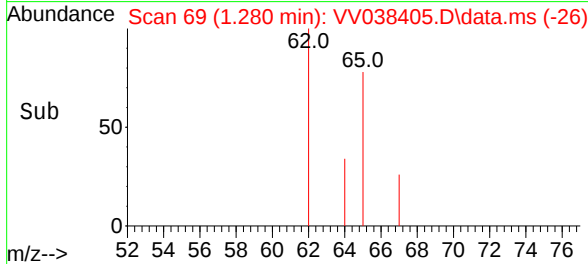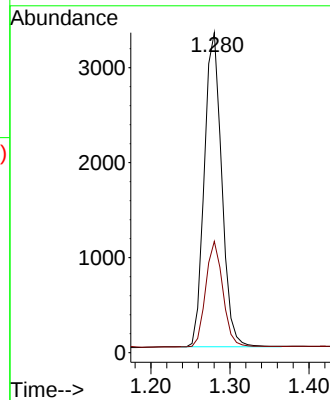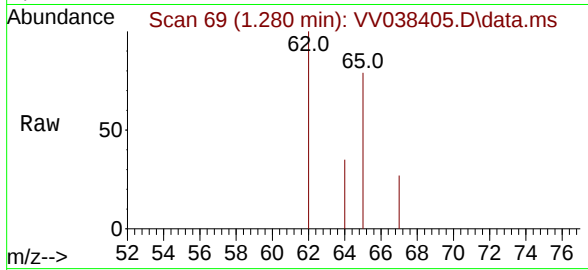

#6

Trichloroethene

Concen: 0.497 ug/L

RT: 5.852 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV038405.D

Acq: 03 Dec 2024 14:01

Tgt Ion: 95 Resp: 3422




Ion Ratio Lower Upper


95 100

97 67.4 46.5 86.5

132 100.1 68.4 127.0


130 103.1 71.6 133.0

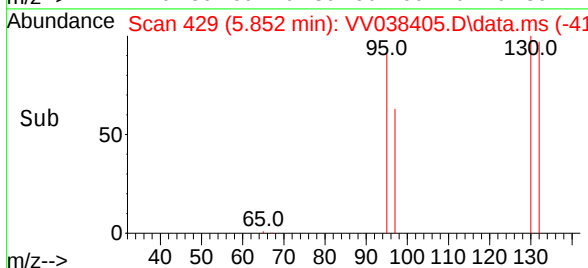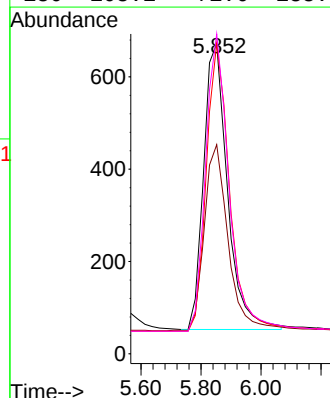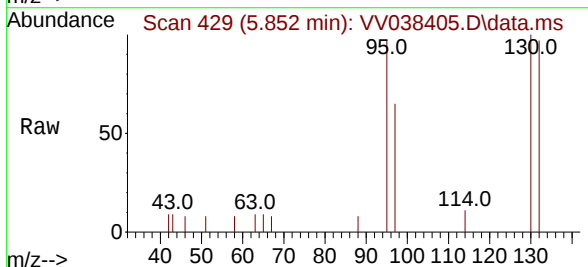



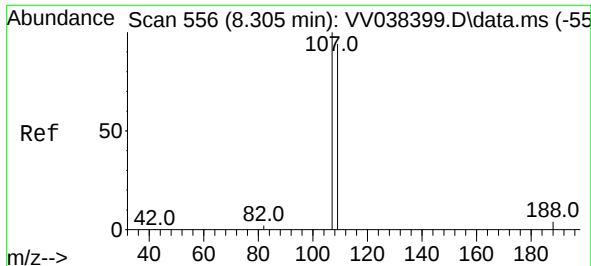


#9
1,2-Dibromoethane
Concen: 0.532 ug/L
RT: 8.305 min Scan# 556
Delta R.T. 0.000 min
Lab File: VV038405.D
Acq: 03 Dec 2024 14:01

Instrument :
MSVOA_V
ClientSampleId :



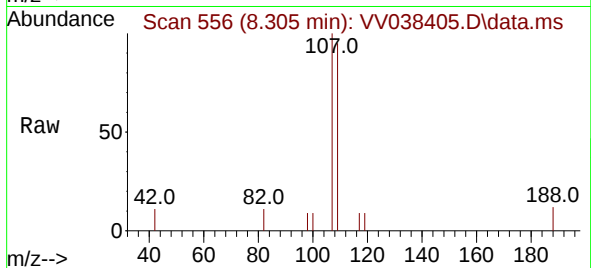



Tgt Ion:107 Resp: 2363
Ion Ratio Lower Upper
107 100
109 95.1 66.4 123.2
188 11.7 8.6 13.0

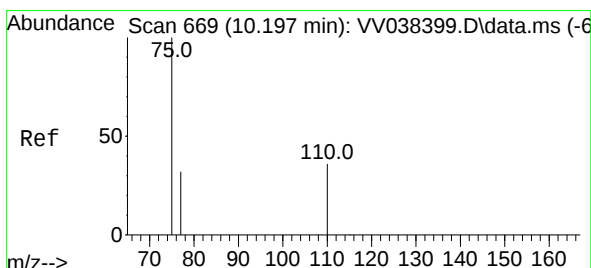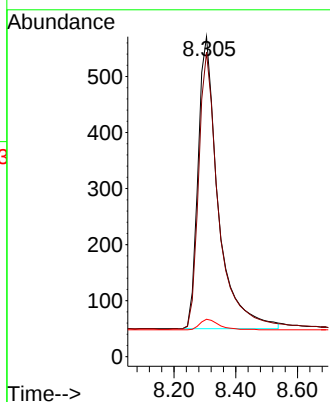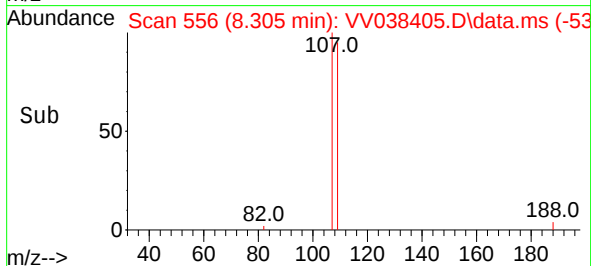

#12
1,2,3-Trichloropropane
Concen: 0.530 ug/L
RT: 10.197 min Scan# 669
Delta R.T. 0.000 min
Lab File: VV038405.D
Acq: 03 Dec 2024 14:01


Tgt Ion: 75 Resp: 2103
Ion Ratio Lower Upper
75 100
110 41.3 33.4 50.0
77 33.2 27.0 40.6

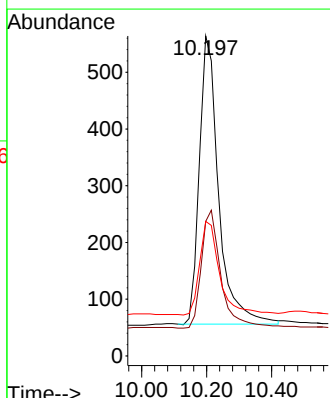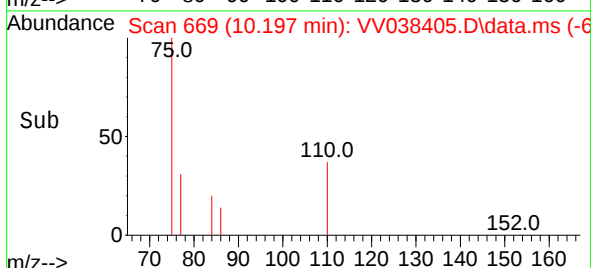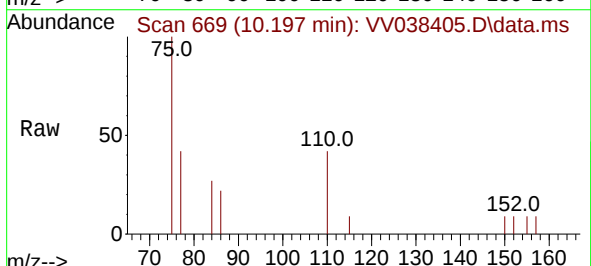

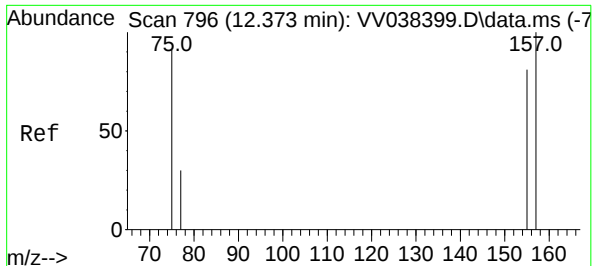

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.542 ug/L
 RT: 12.357 min Scan# 796
 Delta R.T. -0.017 min
 Lab File: VV038405.D
 Acq: 03 Dec 2024 14:01

Instrument :
 MSVOA_V
 ClientSampleId :

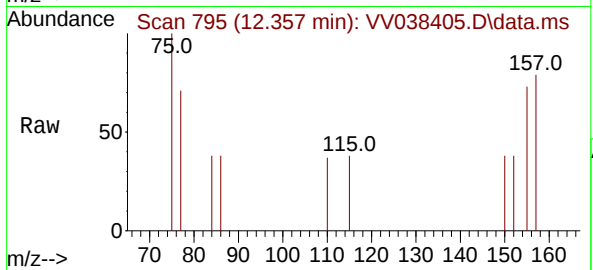

Tgt Ion: 75	Resp:	369
Ion Ratio	Lower	Upper
75	100	
157	78.9	81.1 121.7#
155	72.9	70.3 105.5

