
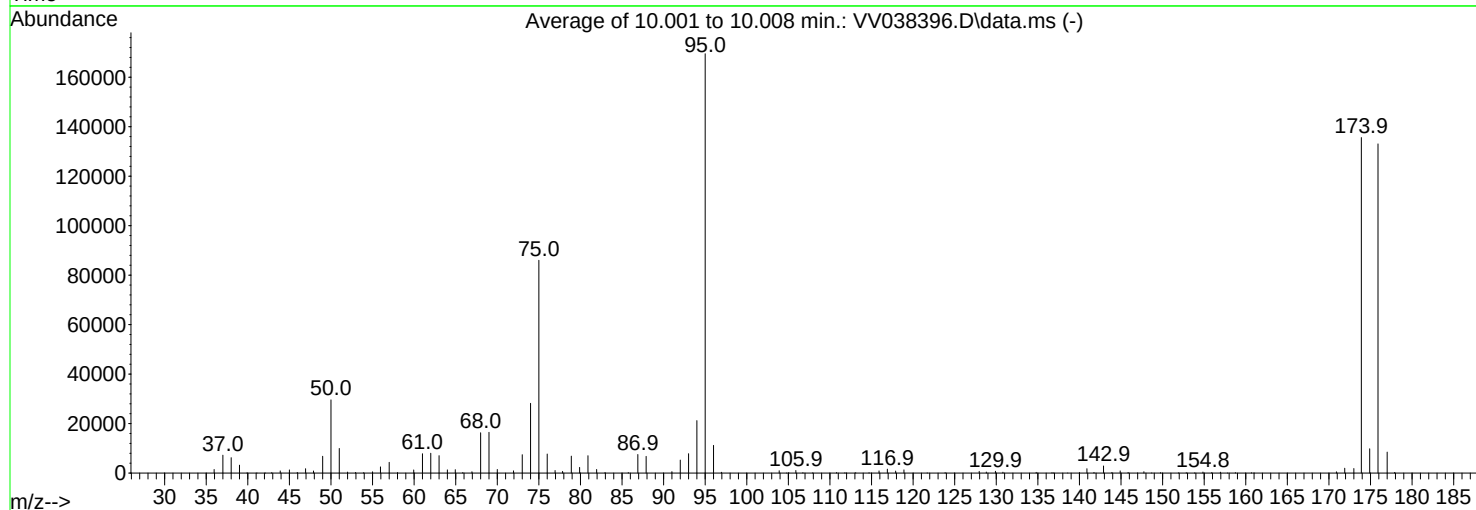


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120324\
Data File : VV038396.D
Acq On : 03 Dec 2024 08:32
Operator : SY/MD
Sample : BFB226
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB226

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120324.M
Title : TRACE VOA SOM01.0
Last Update : Tue Dec 03 21:43:44 2024

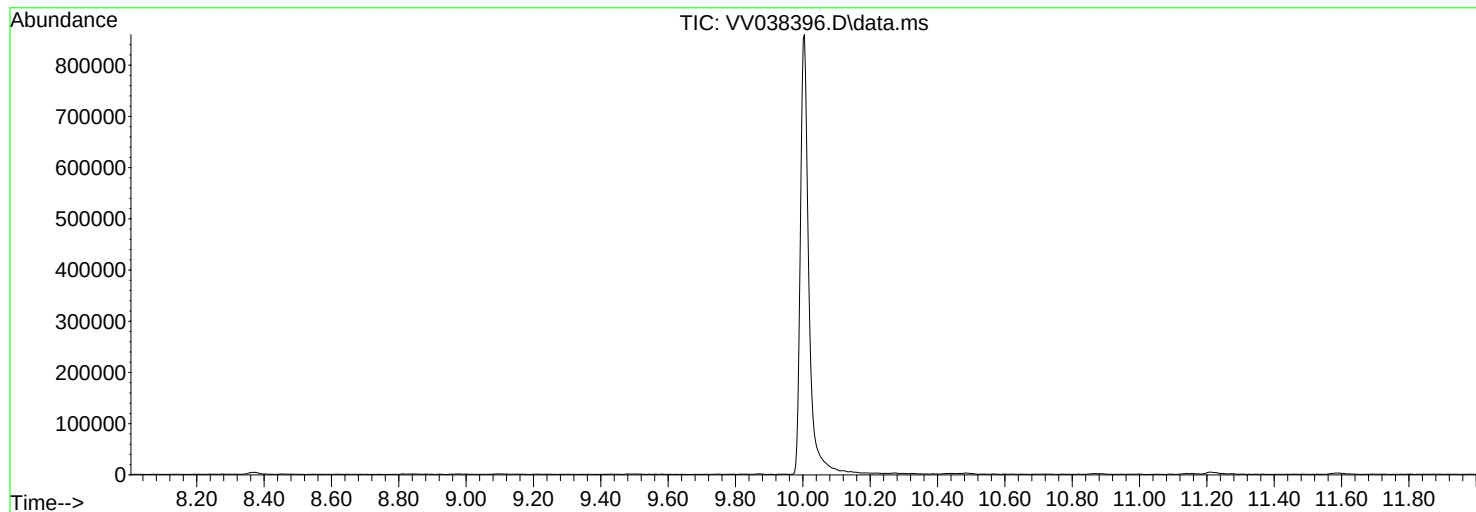

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	29595	PASS
75	95	30	80	50.7	86003	PASS
95	95	100	100	100.0	169493	PASS
96	95	5	9	6.6	11197	PASS
173	174	0.00	2	1.4	1843	PASS
174	95	50	120	80.0	135621	PASS
175	174	5	9	7.2	9825	PASS
176	174	95	101	98.1	133053	PASS
177	176	5	9	6.4	8495	PASS

Scan 2775 (9.963 min): VV038396.D\data.ms
BFB226

m/z	Abundance
39.90	472.0
41.50	108.0
43.90	565.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
35.90	1468.0
37.00	7856.0
38.00	6478.0
39.00	3242.0
39.90	519.0
41.10	110.0
42.90	125.0
44.00	1448.0
45.00	1343.0
46.10	256.0
47.00	1984.0
47.90	836.0
49.00	6942.0
50.00	30216.0
51.00	10381.0
52.00	413.0
52.90	239.0
53.90	168.0
55.00	549.0
56.00	2558.0
57.00	4491.0
58.00	207.0
59.90	1431.0
61.00	8125.0
62.00	8391.0
63.00	7146.0
64.00	1428.0
64.90	1444.0
65.80	211.0
66.90	557.0
68.00	16544.0
69.00	17432.0
70.00	1627.0
72.00	900.0
73.00	7521.0
74.00	29336.0
75.00	89312.0
76.00	8348.0
77.00	1049.0
77.90	712.0
78.90	6949.0
79.90	2189.0
80.90	7196.0
81.90	1403.0
82.90	201.0
85.70	201.0
86.90	7793.0
87.90	6989.0
91.00	631.0
92.00	5429.0
93.00	8178.0
94.00	21880.0
95.00	173760.0
96.00	11661.0
96.90	363.0
103.90	1025.0
104.80	154.0
105.00	143.0
105.90	1001.0
106.70	155.0
107.90	116.0
110.80	279.0
111.80	229.0
113.10	181.0
114.70	195.0
115.90	1023.0
116.90	1522.0
117.90	765.0
118.90	1323.0
123.90	157.0
127.90	752.0
128.80	370.0
129.90	841.0
130.80	374.0
134.80	333.0
136.70	295.0
138.60	106.0
140.00	240.0
140.90	1735.0
141.80	297.0
142.90	3041.0
143.90	210.0
144.80	878.0
146.00	206.0
147.70	598.0
149.80	190.0
151.90	160.0
152.80	159.0
153.90	117.0
154.90	475.0
155.90	130.0
157.00	394.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

158.80	199.0
161.00	132.0
170.90	497.0
171.90	1796.0
173.00	2016.0
173.90	136704.0
174.90	9906.0
175.90	133056.0
177.00	8670.0
177.90	261.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	1480.0
37.00	7496.0
38.00	6463.0
39.00	3354.0
40.00	524.0
42.80	141.0
44.00	1436.0
45.00	1343.0
45.90	274.0
46.90	1753.0
47.90	860.0
49.00	7013.0
50.00	30600.0
51.00	10376.0
52.00	418.0
52.90	262.0
53.90	160.0
55.00	532.0
56.00	2592.0
57.00	4566.0
58.00	228.0
59.90	1303.0
61.00	8127.0
62.00	8263.0
63.00	7319.0
64.00	1337.0
64.90	1421.0
65.90	220.0
66.90	569.0
68.00	16784.0
69.00	17096.0
70.00	1482.0
72.00	936.0
73.00	7671.0
74.00	29016.0
75.00	88728.0
76.00	7946.0
76.90	1036.0
77.90	677.0
78.90	7019.0
79.90	2399.0
80.90	7213.0
82.00	1507.0
82.90	219.0
85.70	214.0
86.90	7794.0
87.90	6816.0
91.00	609.0
92.00	5527.0
93.00	8077.0
94.00	22024.0
95.00	175104.0
96.00	11527.0
96.90	376.0
103.90	1007.0
105.10	146.0
105.90	1139.0
106.80	178.0
107.90	109.0
110.80	255.0
111.80	164.0
113.10	176.0
114.70	166.0
115.90	960.0
116.90	1700.0
117.90	839.0
118.90	1366.0
121.70	124.0
123.80	210.0
128.00	727.0
128.80	468.0
129.90	759.0
130.80	381.0
134.80	297.0
136.70	262.0
140.00	186.0
140.90	1809.0
141.80	256.0
142.90	2997.0
143.90	264.0
144.90	893.0
145.80	295.0
147.00	106.0
147.70	575.0
148.70	132.0
149.80	187.0
151.90	123.0
152.80	171.0
153.80	105.0
154.80	432.0
155.90	186.0
157.00	382.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

158.70	183.0
160.70	162.0
170.90	550.0
171.90	1990.0
173.00	1873.0
173.90	139520.0
174.90	10221.0
175.90	137280.0
177.00	8848.0
177.90	272.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	1430.0
37.00	6355.0
38.00	5754.0
39.00	3039.0
40.00	546.0
42.10	109.0
42.80	118.0
43.90	1473.0
45.00	1136.0
45.90	243.0
47.00	1556.0
47.90	868.0
49.00	6433.0
50.00	27968.0
51.00	9138.0
52.00	392.0
53.00	221.0
53.90	144.0
55.00	500.0
55.90	2404.0
57.00	4017.0
58.00	182.0
60.00	1062.0
61.00	7241.0
62.00	7371.0
63.00	6683.0
64.00	1148.0
65.00	1299.0
65.90	223.0
67.00	511.0
68.00	15599.0
69.00	14882.0
70.00	1280.0
71.90	923.0
73.00	7132.0
74.00	26232.0
75.00	79968.0
76.00	6837.0
76.90	1038.0
77.80	667.0
78.90	6554.0
79.90	2295.0
80.90	6641.0
82.00	1458.0
83.00	197.0
85.80	179.0
86.90	6962.0
87.90	6475.0
91.00	522.0
92.00	4843.0
93.00	7270.0
94.00	19704.0
95.00	159616.0
96.00	10402.0
97.00	276.0
103.90	813.0
105.00	153.0
105.90	1035.0
106.80	180.0
110.80	150.0
112.00	129.0
113.10	143.0
114.80	117.0
115.90	661.0
116.90	1552.0
117.90	890.0
118.90	1245.0
121.70	113.0
123.80	195.0
128.00	618.0
128.80	472.0
129.90	646.0
130.80	361.0
134.80	273.0
136.90	208.0
140.00	146.0
140.90	1779.0
141.70	241.0
142.90	2599.0
143.90	268.0
145.00	875.0
145.80	321.0
147.80	506.0
148.70	129.0
149.70	150.0
152.90	152.0
154.80	393.0
155.90	240.0
156.90	321.0
157.80	110.0
158.70	146.0
160.70	241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

170.90	526.0
171.90	2071.0
173.00	1640.0
173.90	130640.0
174.90	9349.0
175.90	128824.0
177.00	7968.0
177.90	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226