
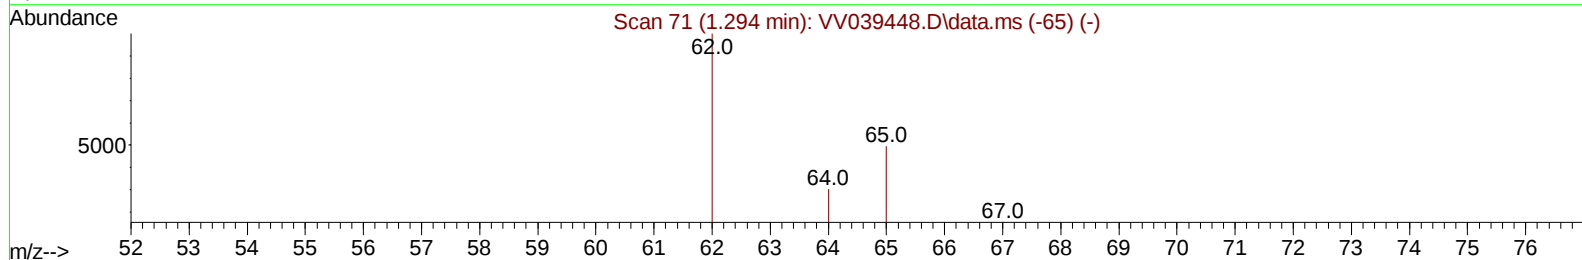
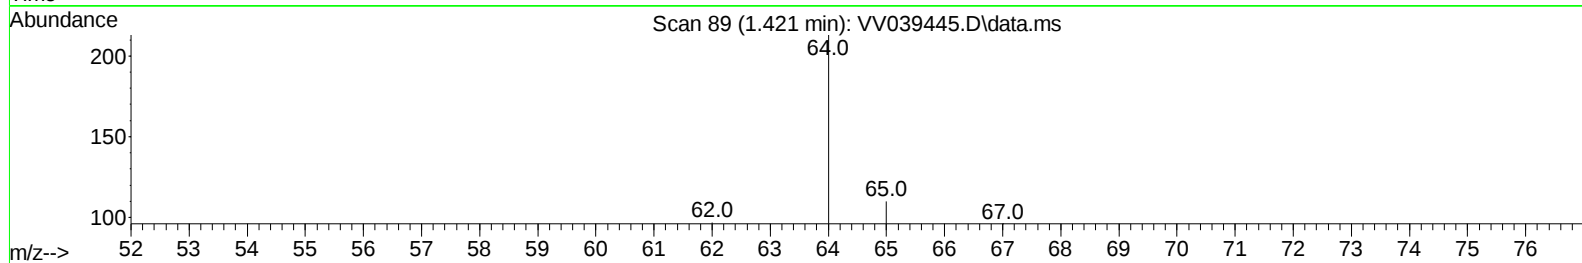


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120325\
Data File : VV039445.D
Acq On : 03 Dec 2025 09:55
Operator : SY/MD
Sample : VSTD0.0269
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 04 00:43:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:43:25 2025
Response via : Initial Calibration

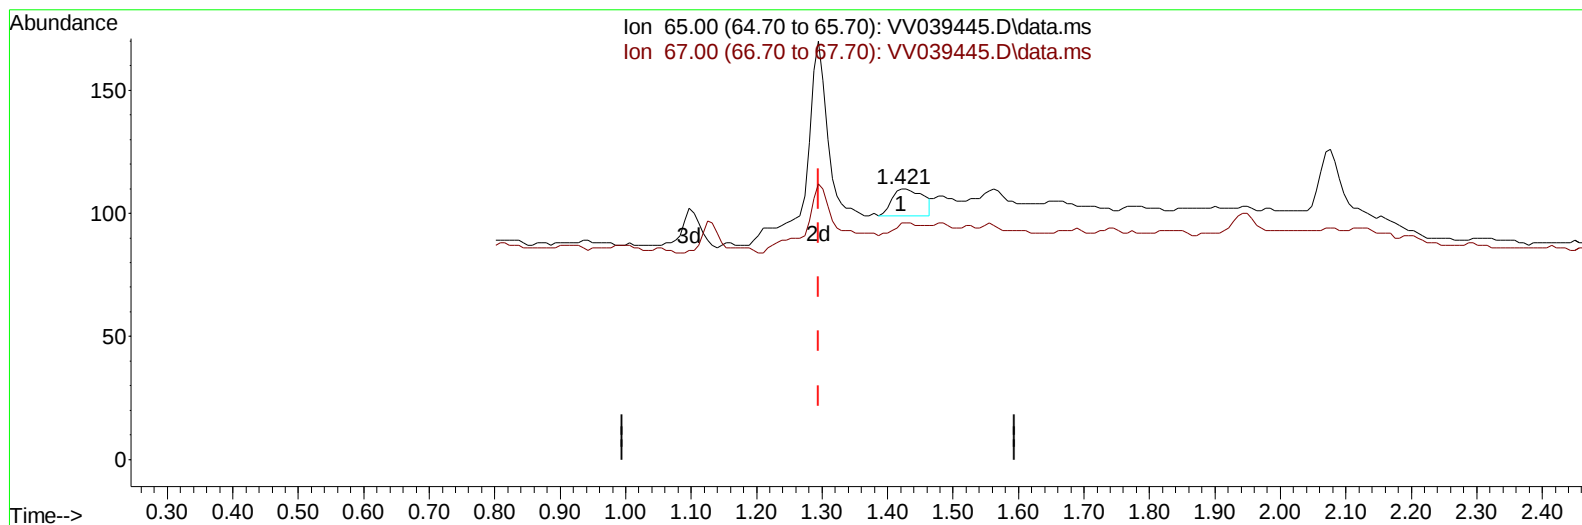

TIC: VV039445.D\data.ms

(2) Vinyl Chloride-d3 (S)




1.421min (+ 0.127) 0.01 ug/L

response 36

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	38.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120325\
Data File : VV039445.D
Acq On : 03 Dec 2025 09:55
Operator : SY/MD
Sample : VSTD0.0269
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 04 00:43:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:43:25 2025
Response via : Initial Calibration

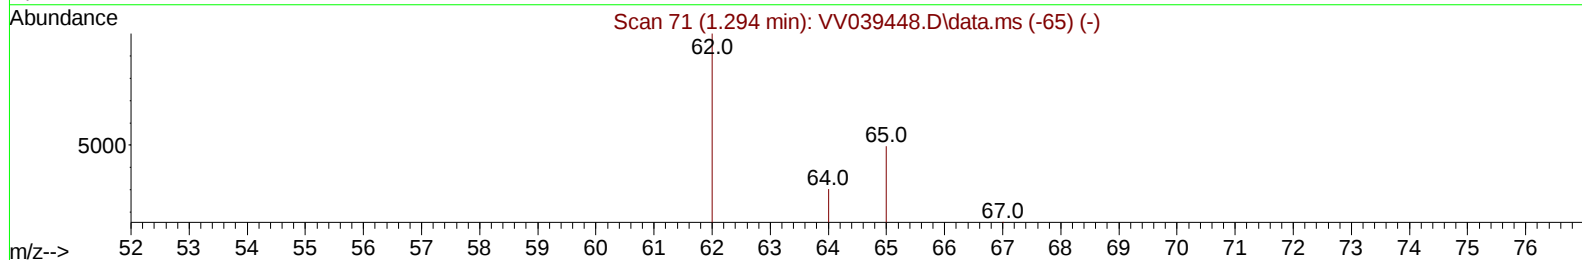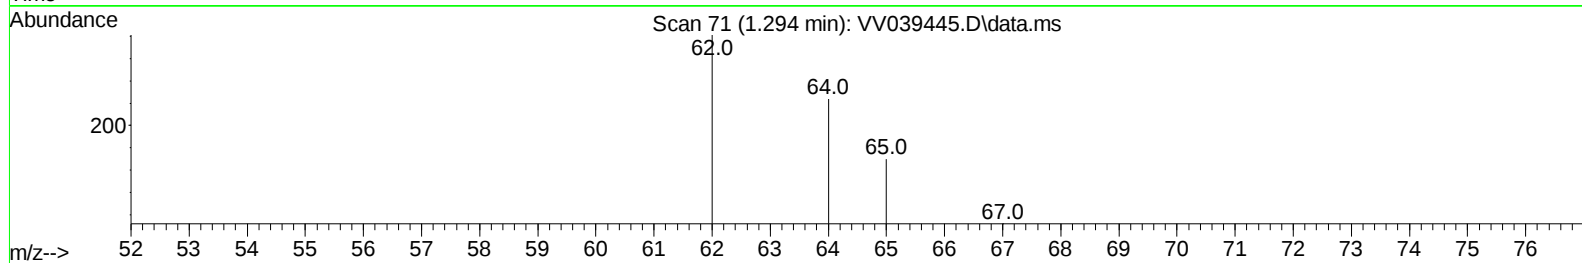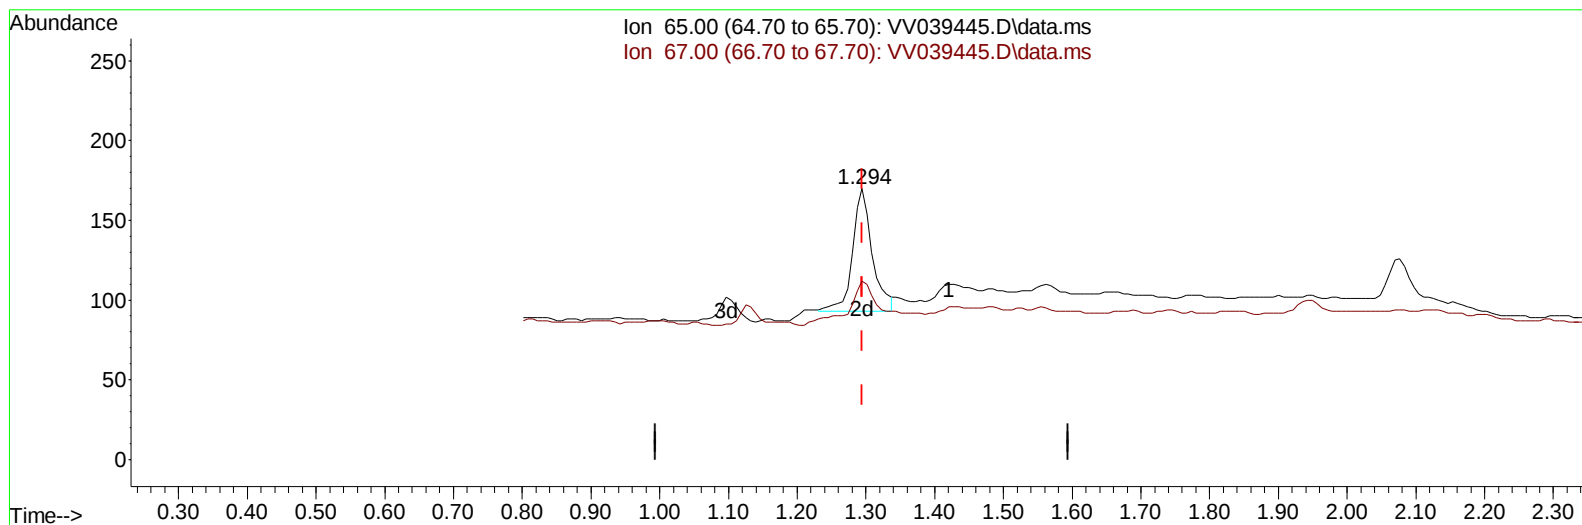

TIC: VV039445.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.02 ug/L m

response 154

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	9.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120325\
 Data File : VV039445.D
 Acq On : 03 Dec 2025 09:55
 Operator : SY/MD
 Sample : VSTD0.0269
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 04 00:43:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:43:25 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6846	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	6511	0.500	ug/L	0.00
12) 1,4-Dichlorobenzene-d4	11.197	152	3380	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	154m	0.022	ug/L	0.00
4) 1,2-Dichloroethane-d4	0.000	65	0d	0.000	ug/L	
7) 1,2-Dichloropropane-d6	0.000	67	0d	0.000	ug/L	
8) Toluene-d8	0.000	98	0d	0.000	ug/L	
10) 1,1,2,2-Tetrachloroeth...	0.000	84	0d	0.000	ug/L	
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.294	62	401	0.027	ug/L #	24
6) Trichloroethene	5.876	95	179	0.023	ug/L #	89
9) 1,2-Dibromoethane	8.321	107	139	0.026	ug/L #	84
11) 1,1,2,2-Tetrachloroethane	10.177	83	153	0.023	ug/L #	95
13) 1,2,3-Trichloropropane	10.199	75	81	0.023	ug/L	89
14) 1,2-Dibromo-3-chloropr...	12.351	75	16	0.022	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120325\
Data File : VV039445.D
Acq On : 03 Dec 2025 09:55
Operator : SY/MD
Sample : VSTD0.0269
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 04 00:43:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:43:25 2025
Response via : Initial Calibration

