


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120419\
 Data File : VV013900.D
 Acq On : 04 Dec 2019 12:12
 Operator : SY/MD
 Sample : BFB75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
 Title : VOC Analysis
 Last Update : Thu Dec 05 01:28:56 2019

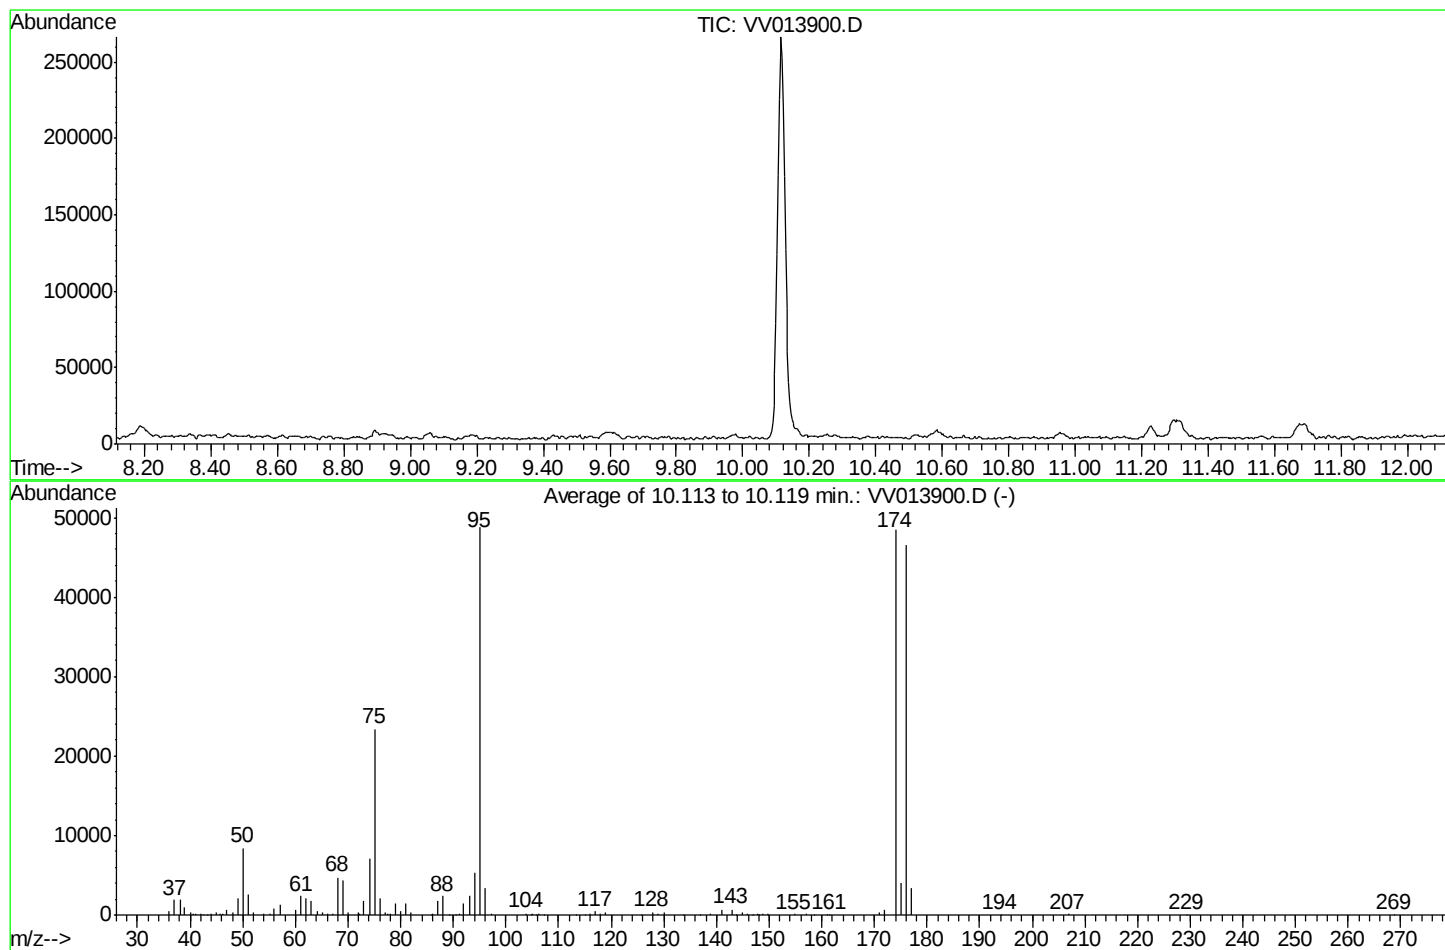

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	8393	PASS
75	95	30	80	48.0	23389	PASS
95	95	100	100	100.0	48768	PASS
96	95	5	9	7.0	3391	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	99.4	48496	PASS
175	174	5	9	8.2	3980	PASS
176	174	95	101	96.1	46586	PASS
177	176	5	9	7.2	3355	PASS

Scan 2806 (10.113 min): VV013900.D
BFB75

m/z	Abundance
36.00	613.0
37.00	1955.0
38.10	1989.0
39.00	966.0
40.00	988.0
41.10	111.0
41.90	118.0
43.30	158.0
44.00	1070.0
45.00	424.0
45.80	109.0
46.30	142.0
47.00	643.0
48.00	274.0
49.00	2096.0
50.00	8388.0
51.00	2735.0
51.90	328.0
54.00	152.0
55.20	182.0
56.00	838.0
57.10	1290.0
58.00	121.0
60.00	690.0
61.10	2319.0
62.00	2163.0
63.00	2100.0
64.20	400.0
64.90	481.0
65.90	176.0
67.00	259.0
68.10	4677.0
69.00	4652.0
70.00	396.0
71.90	326.0
73.00	1880.0
74.10	7172.0
75.00	23784.0
76.10	2201.0
77.00	342.0
78.10	141.0
79.00	1547.0
80.00	561.0
80.90	1500.0
81.90	389.0
85.70	183.0
86.90	1970.0
87.90	2560.0
91.00	171.0
92.00	1506.0
93.10	2397.0
94.00	5310.0
95.10	48808.0
96.10	3552.0
97.10	169.0
103.90	184.0
104.80	148.0
105.80	247.0
115.90	179.0
117.10	430.0
117.90	138.0
118.90	332.0
125.60	105.0
127.90	351.0
128.80	141.0
130.10	240.0
130.80	107.0
133.60	125.0
136.80	108.0
138.90	150.0
141.00	554.0
142.90	682.0
143.80	123.0
144.90	376.0
145.80	152.0
147.70	109.0
148.80	110.0
149.80	103.0
154.80	161.0
157.00	108.0
158.60	104.0
160.90	109.0
161.50	107.0
170.80	272.0
171.90	629.0
174.00	47008.0
175.00	3935.0
176.00	45760.0
177.00	3396.0
194.00	110.0
268.70	100.0

Scan 2807 (10.116 min): VV013900.D
BFB75

m/z	Abundance
36.00	573.0
37.00	2110.0
38.10	1870.0
39.00	1095.0
40.00	1052.0
40.70	112.0
41.20	142.0
42.00	187.0
42.50	123.0
43.30	150.0
44.00	988.0
44.90	431.0
45.80	174.0
46.20	127.0
47.00	669.0
48.00	375.0
49.00	2147.0
50.00	8645.0
51.00	2735.0
51.90	268.0
53.90	124.0
55.10	184.0
56.00	840.0
57.00	1314.0
58.00	136.0
60.00	681.0
61.10	2479.0
62.00	2225.0
63.00	2074.0
64.20	440.0
65.10	472.0
66.00	165.0
67.10	220.0
68.10	4827.0
69.00	4615.0
70.00	388.0
71.90	346.0
72.20	322.0
73.00	1914.0
74.10	7187.0
75.00	24192.0
76.10	2131.0
77.00	414.0
77.60	173.0
78.10	192.0
79.00	1584.0
80.00	538.0
80.90	1446.0
82.00	398.0
85.90	173.0
86.90	1903.0
87.90	2401.0
91.00	186.0
92.00	1463.0
93.10	2497.0
94.00	5378.0
95.10	50024.0
96.10	3535.0
97.10	156.0
103.90	198.0
105.00	148.0
106.20	196.0
113.30	102.0
115.80	193.0
117.10	517.0
117.90	138.0
119.00	376.0
127.80	352.0
128.80	196.0
130.10	369.0
138.90	150.0
141.00	658.0
143.00	699.0
144.90	371.0
145.90	138.0
146.90	108.0
147.70	139.0
148.10	104.0
148.80	119.0
149.80	132.0
154.80	146.0
157.00	127.0
170.80	324.0
171.90	697.0
174.00	49976.0
175.00	4189.0
176.00	48072.0
177.00	3477.0
194.00	106.0
206.90	143.0

m/z	Abundance
36.00	579.0
37.00	2030.0
38.00	1741.0
39.00	1201.0
40.00	1026.0
40.70	195.0
41.20	127.0
42.00	286.0
42.50	126.0
43.20	168.0
44.00	923.0
44.90	376.0
45.80	175.0
46.30	148.0
47.00	703.0
48.00	415.0
49.00	2005.0
50.10	8147.0
51.00	2513.0
51.90	172.0
55.00	245.0
56.00	772.0
57.00	1248.0
58.00	103.0
60.00	543.0
61.10	2245.0
62.00	2075.0
63.00	1837.0
64.00	418.0
65.00	422.0
66.10	115.0
68.00	4642.0
69.00	4256.0
70.00	337.0
71.90	312.0
72.20	351.0
73.00	1970.0
74.10	6890.0
75.10	22192.0
76.00	1917.0
77.00	395.0
77.70	213.0
78.00	241.0
79.00	1442.0
79.90	499.0
80.90	1201.0
82.10	418.0
83.00	143.0
86.00	208.0
87.00	1572.0
87.90	2213.0
89.20	115.0
90.40	101.0
91.10	197.0
92.00	1383.0
93.10	2287.0
94.00	5287.0
95.00	47472.0
96.10	3088.0
97.20	167.0
103.90	242.0
105.00	152.0
106.20	193.0
107.20	104.0
114.90	105.0
115.90	217.0
117.00	502.0
117.90	138.0
119.00	379.0
127.80	308.0
128.80	182.0
130.10	372.0
138.80	120.0
141.00	598.0
143.00	755.0
144.90	402.0
146.00	157.0
147.00	126.0
147.70	122.0
148.70	111.0
149.80	155.0
154.80	133.0
156.90	129.0
170.80	366.0
172.00	703.0
174.00	48504.0
175.00	3818.0
176.00	45928.0
177.00	3193.0
206.90	149.0
229.30	105.0

Scan 2795 (10.077 min): VV013900.D
BFB75

m/z	Abundance
36.20	107.0
36.80	137.0
37.70	110.0
38.90	116.0
40.00	761.0
41.40	141.0
42.10	104.0
43.10	123.0
44.00	746.0
45.10	113.0
48.60	100.0
50.90	129.0
57.90	120.0
59.30	135.0
63.20	159.0
64.90	177.0
67.40	123.0
69.00	120.0
72.90	113.0
76.90	103.0
82.80	118.0
101.10	118.0
119.80	123.0
130.90	105.0