

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120420\
 Data File : VV019476.D
 Acq On : 04 Dec 2020 14:11
 Operator : SY/MD
 Sample : VV1204MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA-V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	237699	239575	15.11%	2.175%
2	1.576	144	151	161	rVB	183254	207799	13.11%	1.887%
3	2.119	311	320	343	rVB	395999	598961	37.79%	5.439%
4	2.470	427	429	434	rBV4	592	540	0.03%	0.005%
5	2.634	476	480	483	rBV4	1056	965	0.06%	0.009%
6	2.688	493	497	503	rBV7	937	1098	0.07%	0.010%
7	2.778	523	525	531	rBV6	1075	857	0.05%	0.008%
8	2.833	541	542	544	rBV	631	345	0.02%	0.003%
9	2.904	561	564	566	rBV3	696	465	0.03%	0.004%
10	3.122	630	632	636	rVB2	590	284	0.02%	0.003%
11	3.148	636	640	641	rBV3	1170	791	0.05%	0.007%
12	3.303	685	688	691	rBV3	507	304	0.02%	0.003%
13	3.331	695	697	700	rBV4	507	201	0.01%	0.002%
14	3.360	704	706	712	rBV6	478	461	0.03%	0.004%
15	3.450	730	734	739	rVB6	658	637	0.04%	0.006%
16	3.528	755	758	759	rBV3	524	372	0.02%	0.003%
17	3.582	772	775	776	rBV2	563	293	0.02%	0.003%
18	3.627	786	789	790	rBV2	584	285	0.02%	0.003%
19	3.701	808	812	814	rBV4	664	606	0.04%	0.006%
20	3.743	823	825	827	rVB2	588	267	0.02%	0.002%
21	3.759	827	830	831	rBV	699	371	0.02%	0.003%
22	3.769	831	833	837	rVV3	427	244	0.02%	0.002%
23	3.788	837	839	843	rVB4	729	476	0.03%	0.004%
24	3.811	843	846	848	rBV3	395	183	0.01%	0.002%
25	3.839	853	855	858	rBV2	518	223	0.01%	0.002%
26	3.897	863	873	910	rBV	106000	300139	18.93%	2.725%
27	4.303	993	999	1000	rBV4	874	900	0.06%	0.008%
28	4.373	1006	1021	1050	rBV	254914	625508	39.46%	5.680%
29	4.659	1109	1110	1111	rBV	687	248	0.02%	0.002%
30	4.711	1124	1126	1128	rBV2	762	384	0.02%	0.003%
31	4.807	1153	1156	1158	rBV2	727	486	0.03%	0.004%
32	4.833	1162	1164	1165	rBV	661	204	0.01%	0.002%
33	4.878	1176	1178	1181	rVB3	785	307	0.02%	0.003%
34	4.942	1196	1198	1201	rBV3	748	476	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120420\
 Data File : VV019476.D
 Acq On : 04 Dec 2020 14:11
 Operator : SY/MD
 Sample : VV1204MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA-V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	4.962	1201	1204	1208	rVB3	912	700	0.04%	0.006%
36	4.981	1208	1210	1214	rBV3	1163	671	0.04%	0.006%
37	5.068	1221	1237	1269	rBV2	613392	1585175	100.00%	14.394%
38	5.463	1357	1360	1363	rBV4	703	562	0.04%	0.005%
39	5.483	1363	1366	1368	rVV3	789	464	0.03%	0.004%
40	5.640	1403	1415	1438	rBV	369887	749401	47.28%	6.805%
41	5.926	1494	1504	1522	rVB	42530	83674	5.28%	0.760%
42	6.090	1541	1555	1584	rBV	360987	742793	46.86%	6.745%
43	6.505	1680	1684	1688	rBV6	995	879	0.06%	0.008%
44	6.524	1688	1690	1692	rVV4	563	287	0.02%	0.003%
45	6.614	1715	1718	1721	rVB3	732	417	0.03%	0.004%
46	6.630	1721	1723	1725	rBV2	1030	553	0.03%	0.005%
47	6.711	1746	1748	1751	rVV2	738	371	0.02%	0.003%
48	6.753	1757	1761	1763	rBV5	1267	947	0.06%	0.009%
49	6.823	1780	1783	1784	rBV2	571	343	0.02%	0.003%
50	6.839	1785	1788	1792	rVB3	971	734	0.05%	0.007%
51	6.855	1792	1793	1795	rBV2	468	243	0.02%	0.002%
52	6.897	1802	1806	1809	rVV4	650	404	0.03%	0.004%
53	6.926	1811	1815	1818	rBV3	972	763	0.05%	0.007%
54	7.007	1828	1840	1859	rBV	188082	342958	21.64%	3.114%
55	7.290	1926	1928	1930	rBV3	626	387	0.02%	0.004%
56	7.335	1930	1942	1961	rBV	678606	1170278	73.83%	10.627%
57	7.640	2028	2037	2053	rBV	138319	238092	15.02%	2.162%
58	7.910	2119	2121	2124	rBV	673	378	0.02%	0.003%
59	8.106	2172	2182	2219	rBV2	306183	623954	39.36%	5.666%
60	8.624	2341	2343	2347	rBV4	1391	850	0.05%	0.008%
61	8.871	2409	2420	2445	rBV	585020	958974	60.50%	8.708%
62	9.228	2529	2531	2532	rBV	548	230	0.01%	0.002%
63	9.293	2549	2551	2554	rVB3	1193	637	0.04%	0.006%
64	9.318	2554	2559	2562	rBV4	1002	916	0.06%	0.008%
65	9.360	2570	2572	2576	rVB5	781	409	0.03%	0.004%
66	9.511	2617	2619	2624	rVB3	889	542	0.03%	0.005%
67	9.704	2676	2679	2682	rBV3	835	653	0.04%	0.006%
68	9.749	2691	2693	2695	rBV2	547	282	0.02%	0.003%
69	9.769	2697	2699	2700	rBV	678	266	0.02%	0.002%
70	9.887	2733	2736	2743	rVB4	1176	959	0.06%	0.009%
71	9.920	2743	2746	2748	rVB3	753	400	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120420\
 Data File : VV019476.D
 Acq On : 04 Dec 2020 14:11
 Operator : SY/MD
 Sample : VV1204MBL01
 Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA-V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

72	10.064	2787	2791	2793	rBV3	516	318	0.02%	0.003%
73	10.125	2807	2810	2816	rVB6	978	679	0.04%	0.006%
74	10.177	2823	2826	2827	rBV3	750	436	0.03%	0.004%
75	10.235	2831	2844	2865	rVV	391039	615867	38.85%	5.592%
76	10.383	2886	2890	2895	rBV5	1119	853	0.05%	0.008%
77	10.408	2897	2898	2900	rBV2	809	312	0.02%	0.003%
78	10.453	2909	2912	2914	rVB4	886	478	0.03%	0.004%
79	10.553	2940	2943	2945	rBV4	791	501	0.03%	0.005%
80	10.601	2955	2958	2961	rBV4	978	679	0.04%	0.006%
81	10.653	2971	2974	2976	rBV2	803	358	0.02%	0.003%
82	10.765	3006	3009	3011	rBV2	574	302	0.02%	0.003%
83	10.897	3045	3050	3054	rBV5	828	1016	0.06%	0.009%
84	10.916	3054	3056	3058	rBV4	477	236	0.01%	0.002%
85	10.974	3071	3074	3077	rBV4	693	362	0.02%	0.003%
86	11.151	3127	3129	3130	rBV	407	221	0.01%	0.002%
87	11.209	3142	3147	3150	rBV6	1098	1128	0.07%	0.010%
88	11.270	3154	3166	3192	rVV	559513	876880	55.32%	7.963%
89	11.643	3270	3282	3301	rBV	635467	1010498	63.75%	9.176%
90	11.839	3341	3343	3348	rVB3	1024	629	0.04%	0.006%
91	12.334	3493	3497	3499	rBV3	1187	872	0.06%	0.008%
92	12.489	3543	3545	3546	rBV2	726	226	0.01%	0.002%
93	12.518	3552	3554	3559	rVB4	691	482	0.03%	0.004%
94	12.801	3640	3642	3645	rBV3	523	247	0.02%	0.002%
95	12.920	3677	3679	3681	rBV2	798	374	0.02%	0.003%
96	13.238	3776	3778	3782	rVB4	785	415	0.03%	0.004%
97	13.595	3886	3889	3893	rBV4	838	694	0.04%	0.006%
98	13.743	3933	3935	3937	rBV	799	432	0.03%	0.004%
99	14.267	4094	4098	4100	rBV5	841	705	0.04%	0.006%
100	14.685	4226	4228	4232	rBV4	905	596	0.04%	0.005%


Sum of corrected areas: 11012597

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120420\
Data File : VV019476.D
Acq On : 04 Dec 2020 14:11
Operator : SY/MD
Sample : VV1204MBL01
Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA-V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK94

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

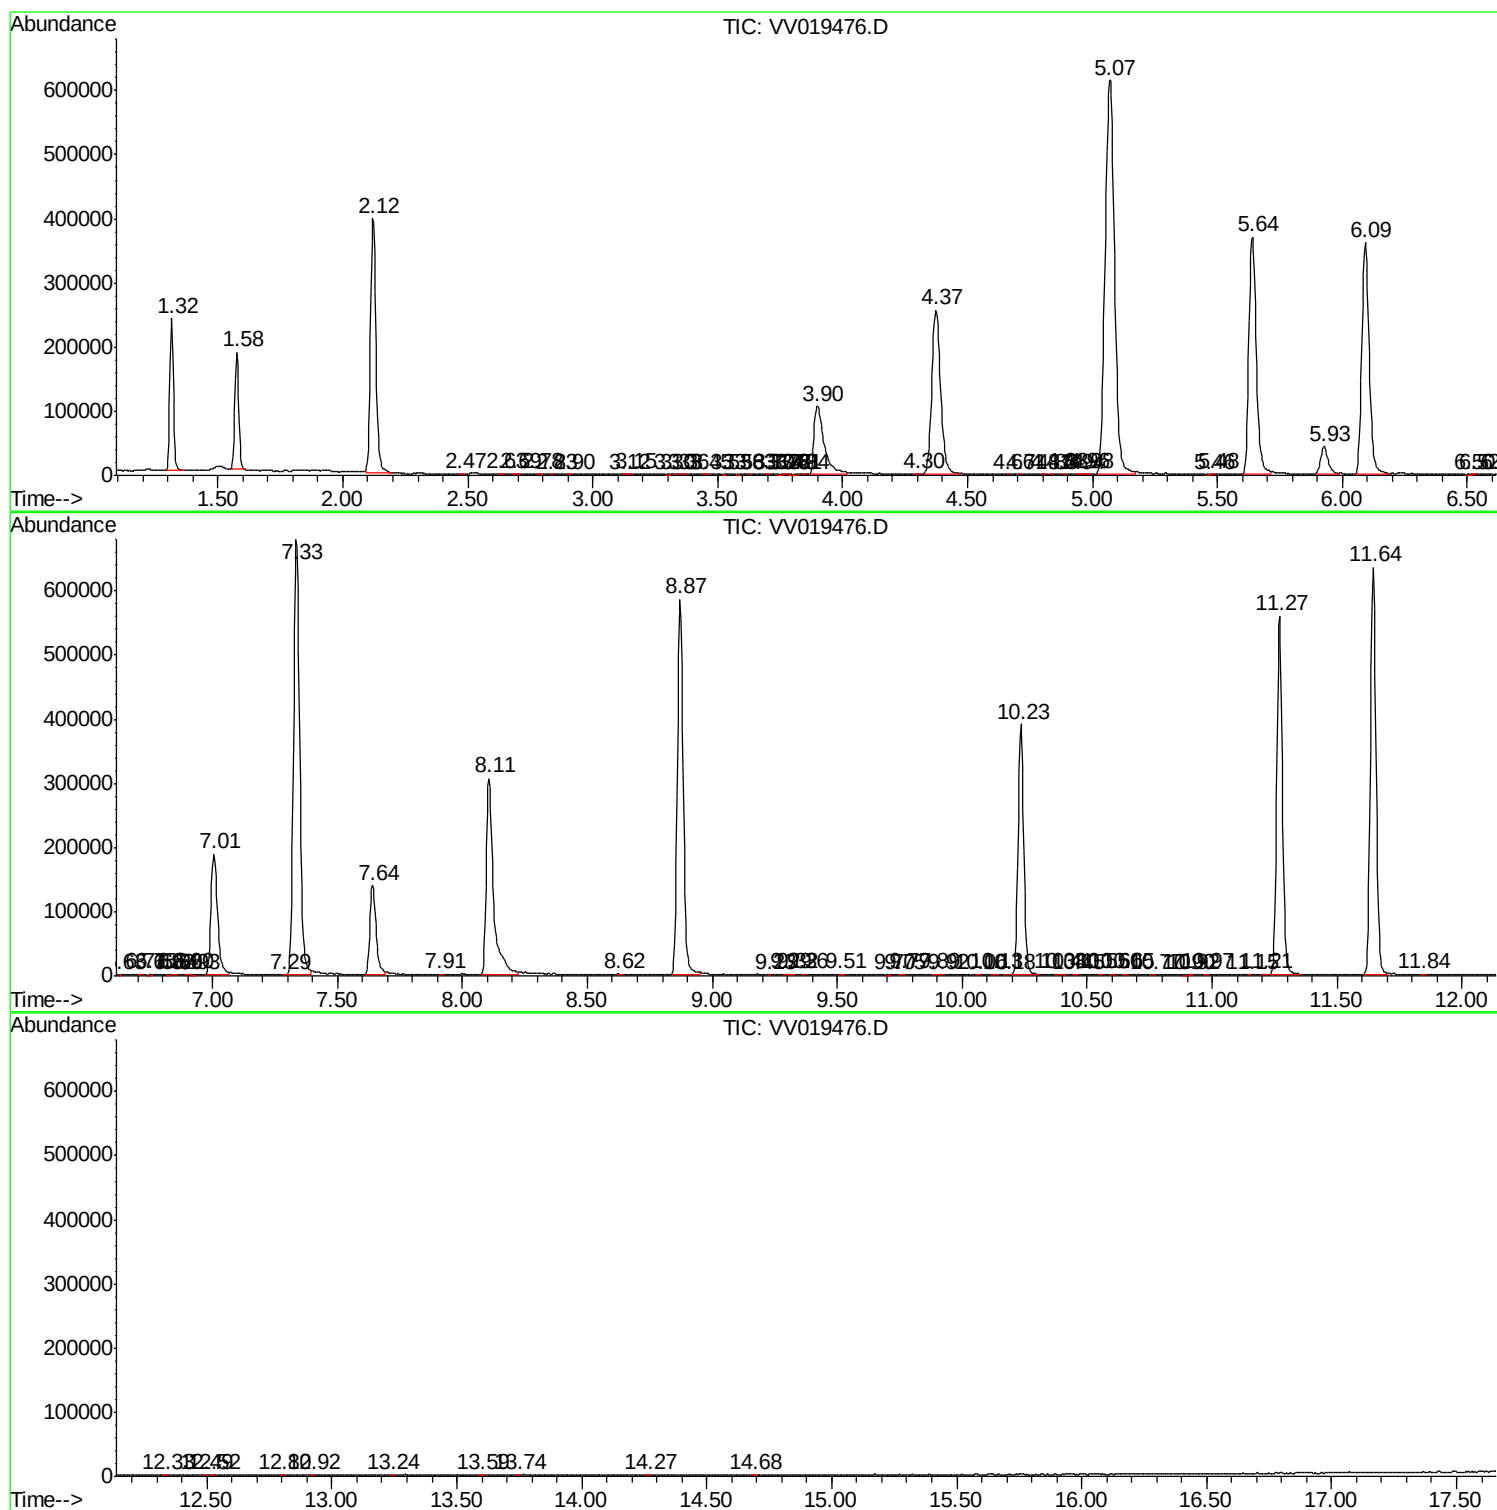

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120420\
Data File : VV019476.D
Acq On : 04 Dec 2020 14:11
Operator : SY/MD
Sample : VV1204MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA-V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK94

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120420\
Data File : VV019476.D
Acq On : 04 Dec 2020 14:11
Operator : SY/MD
Sample : VV1204MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A-V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK94

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc