


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120420\
Data File : VV019473.D
Acq On : 04 Dec 2020 10:51
Operator : SY/MD
Sample : BFB61
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Title : VOC Analysis
Last Update : Mon Dec 07 09:35:42 2020

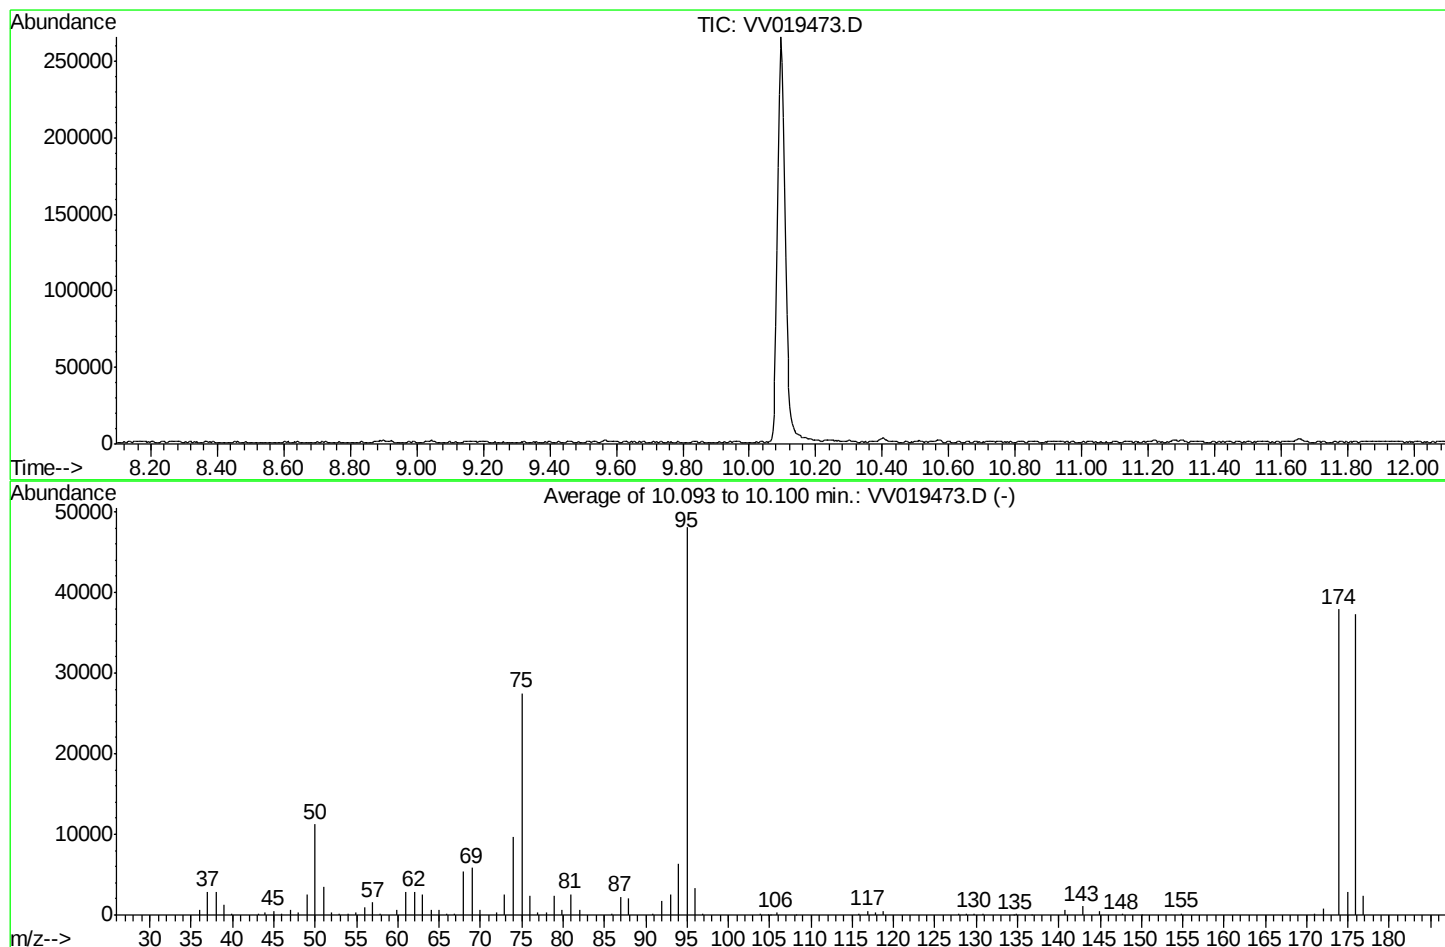

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	11254	PASS
75	95	30	80	57.2	27506	PASS
95	95	100	100	100.0	48085	PASS
96	95	5	9	6.9	3335	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.8	37914	PASS
175	174	5	9	7.6	2869	PASS
176	174	95	101	98.4	37306	PASS
177	176	5	9	6.5	2434	PASS

m/z	Abundance
35.90	603.0
37.00	2929.0
38.00	2965.0
39.00	1246.0
40.00	375.0
43.20	115.0
43.90	948.0
45.00	555.0
46.00	242.0
47.00	621.0
47.90	428.0
49.00	2645.0
50.00	11332.0
51.00	3491.0
52.00	249.0
52.90	188.0
54.00	111.0
54.90	281.0
56.00	954.0
57.00	1601.0
57.90	199.0
59.90	660.0
61.00	3029.0
62.00	3013.0
63.00	2588.0
64.00	646.0
65.00	735.0
65.90	196.0
66.90	252.0
68.00	5609.0
69.00	5915.0
70.00	715.0
72.00	375.0
73.00	2676.0
74.00	10048.0
75.00	27648.0
76.00	2413.0
76.90	320.0
78.00	220.0
78.90	2498.0
79.90	741.0
80.90	2593.0
82.00	581.0
86.00	210.0
87.00	2263.0
87.90	2103.0
90.90	245.0
92.00	1697.0
93.00	2524.0
94.00	6607.0
95.00	48616.0
96.00	3528.0
96.90	148.0
103.80	236.0
105.10	105.0
105.80	287.0
115.90	235.0
116.90	488.0
117.80	248.0
118.80	442.0
127.90	217.0
128.70	186.0
129.80	226.0
130.80	106.0
134.60	111.0
140.80	591.0
142.80	1043.0
144.90	495.0
147.80	123.0
154.80	164.0
170.90	210.0
172.00	695.0
173.90	36904.0
174.90	2833.0
175.90	36752.0
176.90	2470.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	652.0
37.00	2956.0
38.00	3052.0
39.00	1300.0
39.90	319.0
43.20	126.0
43.90	903.0
45.00	553.0
46.00	228.0
47.10	604.0
47.90	408.0
49.00	2714.0
50.00	11671.0
51.00	3592.0
52.00	264.0
52.90	178.0
54.00	127.0
54.90	297.0
56.00	1015.0
57.00	1601.0
57.90	192.0
59.90	670.0
61.00	2985.0
62.00	2982.0
63.00	2665.0
64.00	639.0
65.00	696.0
65.90	196.0
66.90	246.0
68.00	5610.0
69.00	5982.0
70.00	676.0
72.00	345.0
72.90	2580.0
74.00	9983.0
75.00	28360.0
76.00	2459.0
76.90	330.0
77.90	255.0
78.90	2530.0
79.90	731.0
80.90	2643.0
81.90	585.0
85.90	159.0
86.90	2280.0
87.90	2054.0
90.80	211.0
91.90	1832.0
93.00	2678.0
94.00	6662.0
95.00	49568.0
96.00	3469.0
96.90	150.0
103.80	238.0
104.80	112.0
105.80	264.0
108.20	101.0
115.90	211.0
116.90	512.0
117.80	296.0
118.80	444.0
127.80	221.0
128.70	164.0
129.80	257.0
130.90	144.0
134.80	132.0
136.70	118.0
140.80	662.0
142.90	1082.0
144.90	519.0
147.70	122.0
149.90	104.0
154.90	180.0
170.90	233.0
171.90	805.0
173.90	39064.0
174.90	2948.0
175.90	38512.0
176.90	2549.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	720.0
37.00	2750.0
38.00	2782.0
39.00	1214.0
39.90	301.0
40.10	293.0
43.20	116.0
43.90	881.0
45.00	540.0
46.00	155.0
47.10	549.0
47.90	347.0
49.00	2457.0
50.00	10759.0
51.00	3400.0
51.90	258.0
53.00	151.0
54.10	114.0
55.00	276.0
56.00	930.0
57.00	1531.0
57.90	134.0
59.90	628.0
61.00	2777.0
62.00	2827.0
63.00	2529.0
64.00	570.0
65.00	684.0
65.90	201.0
66.90	223.0
68.00	5053.0
69.00	5509.0
70.00	548.0
72.00	302.0
73.00	2245.0
74.00	8916.0
75.00	26512.0
76.00	2168.0
76.90	304.0
77.90	290.0
78.90	2354.0
79.90	683.0
80.90	2437.0
81.90	541.0
85.90	124.0
86.90	2170.0
87.90	1976.0
90.90	186.0
91.90	1765.0
93.00	2465.0
94.00	6020.0
95.00	46072.0
96.00	3008.0
96.90	141.0
103.80	220.0
104.80	135.0
105.90	229.0
108.10	101.0
115.80	219.0
116.90	461.0
117.80	285.0
118.80	398.0
127.80	225.0
128.80	119.0
129.80	230.0
130.90	142.0
134.80	156.0
136.70	131.0
140.80	629.0
142.90	1029.0
144.80	497.0
147.60	138.0
150.00	115.0
154.90	168.0
170.90	213.0
171.90	842.0
173.90	37776.0
174.90	2828.0
175.90	36656.0
176.90	2285.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Scan 2789 (10.058 min): VV019473.D
BFB61

m/z	Abundance
38.00	140.0
40.00	262.0
40.70	107.0
43.90	536.0
79.00	101.0
80.10	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61