

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
 Data File : VV033090.D
 Acq On : 04 Dec 2023 10:31
 Operator : SY/MD
 Sample : VV1204WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 05 03:21:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 05 03:20:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	342241	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	341559	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	184824	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	84409	41.257	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.520%
7) Chloroethane-d5	1.532	69	61070	42.840	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.680%
11) 1,1-Dichloroethene-d2	2.059	65	33384	42.893	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.780%
21) 2-Butanone-d5	3.780	46	97175	95.629	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.630%
24) Chloroform-d	4.249	84	189986	43.757	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.520%
26) 1,2-Dichloroethane-d4	4.940	65	124353	46.066	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.140%
32) Benzene-d6	4.960	84	362104	45.329	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.660%
36) 1,2-Dichloropropane-d6	5.989	67	100664	46.867	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.740%
41) Toluene-d8	7.243	98	332701	43.659	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.320%
43) trans-1,3-Dichloroprop...	7.551	79	57317	42.201	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.400%
47) 2-Hexanone-d5	8.024	63	80193	92.938	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.940%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	137094	44.901	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	159014	48.355	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.720%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.548	75	2813	0.765	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033090.D
Acq On : 04 Dec 2023 10:31
Operator : SY/MD
Sample : VV1204WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 05 03:21:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 05 03:20:48 2023
Response via : Initial Calibration

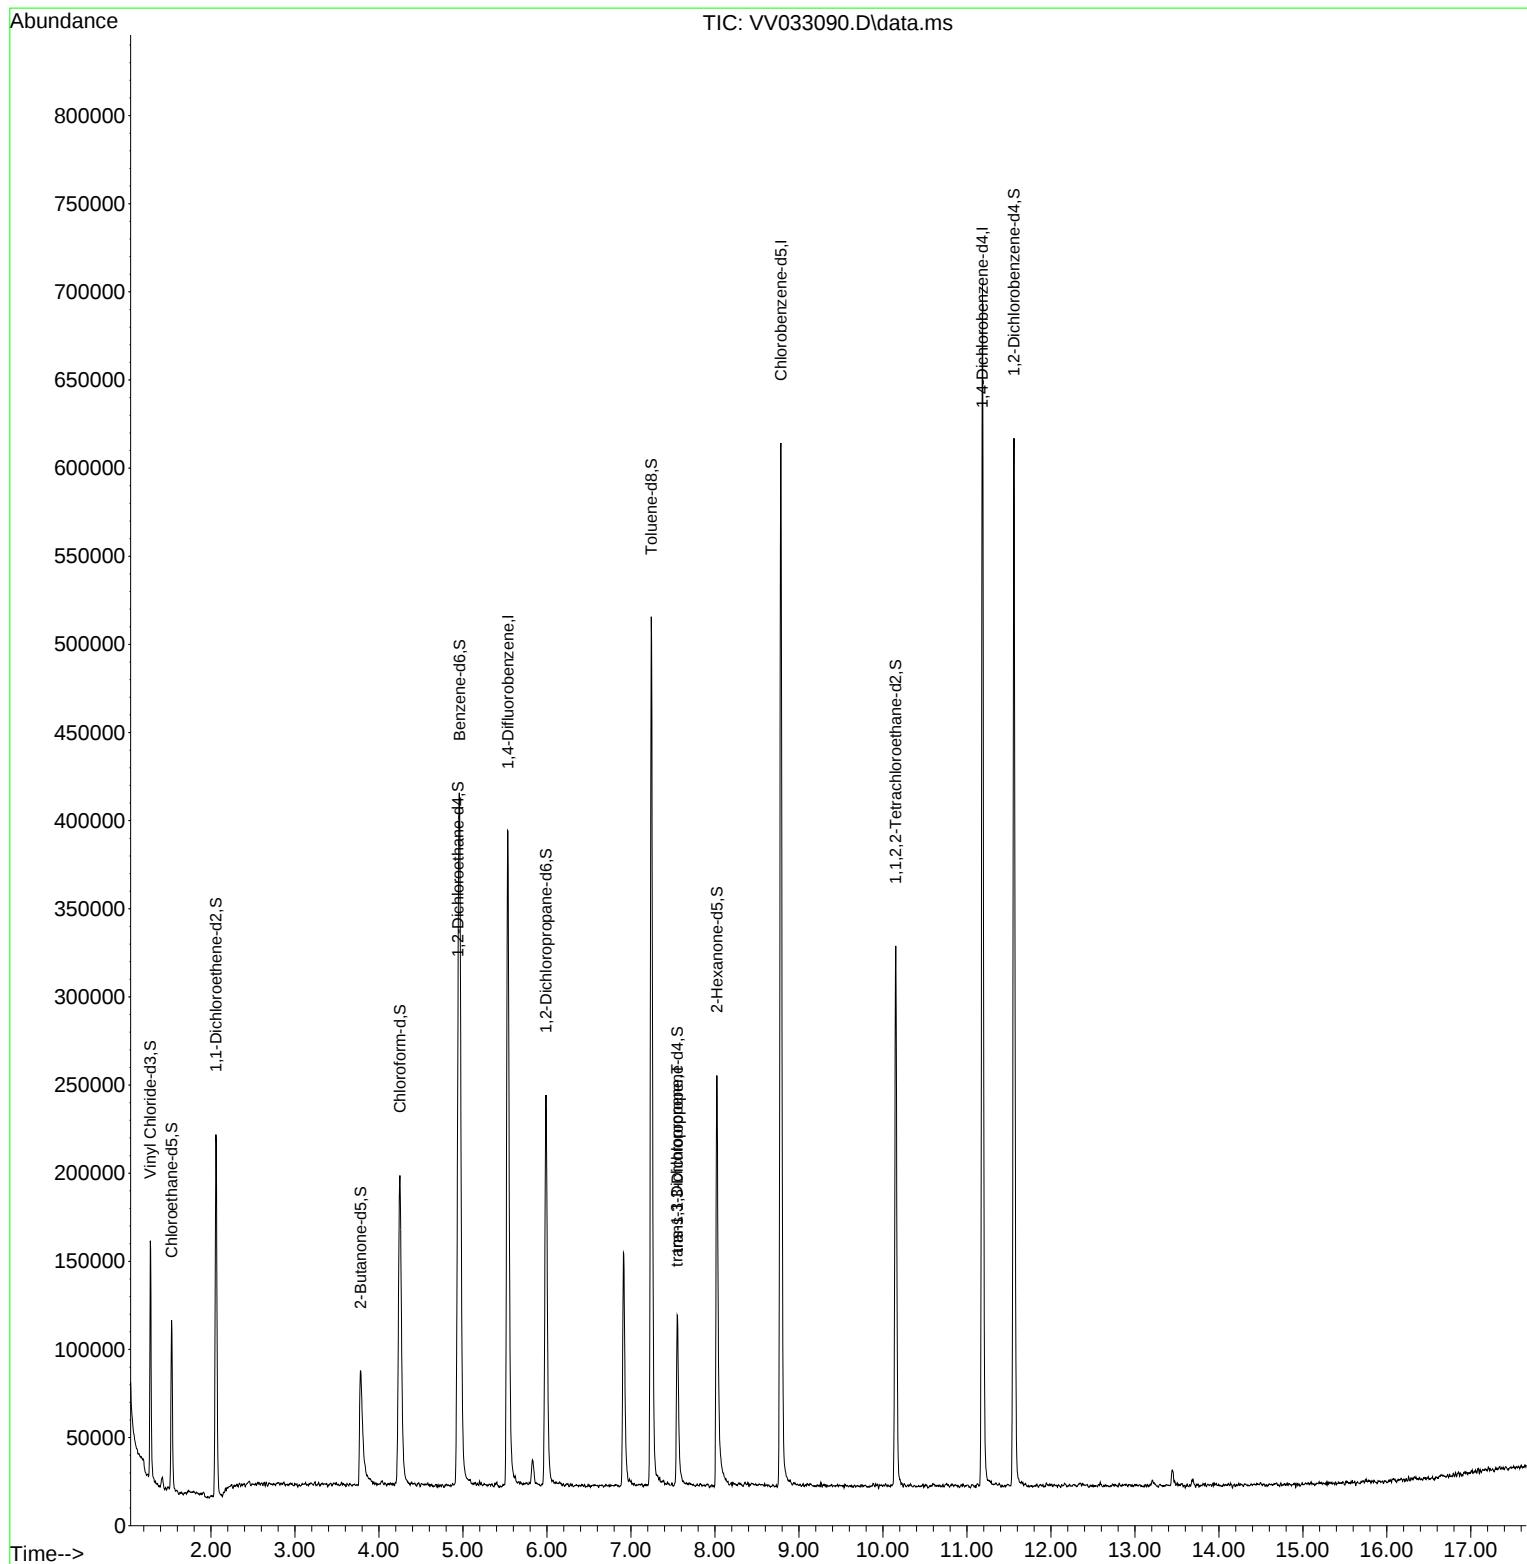

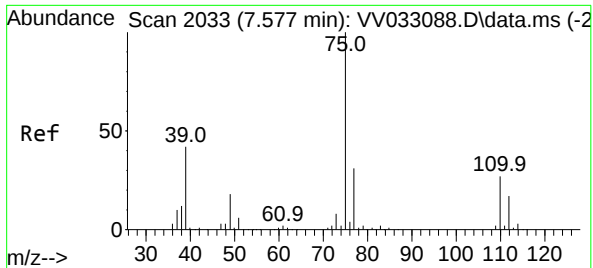

#44
 trans-1,3-Dichloropropene
 Concen: 0.765 ug/L
 RT: 7.548 min Scan# 20
 Delta R.T. -0.029 min
 Lab File: VV033090.D
 Acq: 04 Dec 2023 10:31

Instrument :
 MSVOA_V
 ClientSampleId :

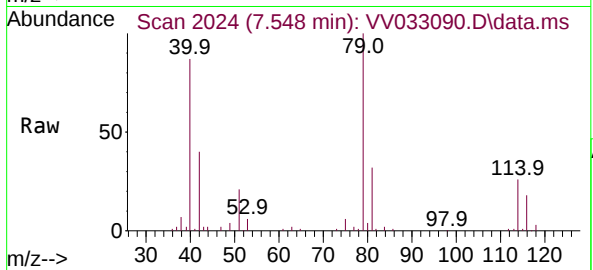

Tgt Ion: 75 Resp: 2813
 Ion Ratio Lower Upper
 75 100
 77 40.8 22.0 41.0

