

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
 Data File : VV033089.D
 Acq On : 04 Dec 2023 10:08
 Operator : SY/MD
 Sample : VV1204MBL01
 Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	157664	170731	15.01%	1.829%
2	1.423	111	119	126	rVB2	7185	9767	0.86%	0.105%
3	1.532	145	153	174	rVB	109618	138352	12.16%	1.482%
4	1.667	192	195	198	rBV2	1216	718	0.06%	0.008%
5	1.693	198	203	206	rBV2	2320	2025	0.18%	0.022%
6	1.712	206	209	210	rBV	1172	567	0.05%	0.006%
7	1.770	223	227	228	rBV3	1405	1066	0.09%	0.011%
8	1.873	256	259	261	rBV	1280	869	0.08%	0.009%
9	1.912	267	271	277	rVB3	2506	3057	0.27%	0.033%
10	1.937	277	279	284	rVB	1868	1474	0.13%	0.016%
11	1.963	284	287	292	rBV2	651	644	0.06%	0.007%
12	2.002	295	299	302	rBV	544	487	0.04%	0.005%
13	2.060	306	317	331	rBV	228862	332553	29.23%	3.562%
14	2.127	335	338	341	rBV4	886	814	0.07%	0.009%
15	2.150	341	345	348	rBV	2955	2464	0.22%	0.026%
16	2.195	348	359	362	rBV	3608	6437	0.57%	0.069%
17	2.317	395	397	400	rBV	1283	799	0.07%	0.009%
18	2.957	593	596	599	rBV	1710	1250	0.11%	0.013%
19	3.101	638	641	646	rVB	1424	1087	0.10%	0.012%
20	3.127	647	649	652	rVB	1499	802	0.07%	0.009%
21	3.777	843	851	885	rBV	69877	191427	16.83%	2.050%
22	4.246	980	997	1020	rBV2	185021	474591	41.71%	5.083%
23	4.568	1094	1097	1098	rBV2	1497	907	0.08%	0.010%
24	4.725	1143	1146	1149	rBV	1790	1290	0.11%	0.014%
25	4.844	1180	1183	1184	rBV	1371	882	0.08%	0.009%
26	4.953	1200	1217	1245	rBV2	426810	1137742	100.00%	12.186%
27	5.285	1316	1320	1325	rBV	2377	2320	0.20%	0.025%
28	5.529	1385	1396	1422	rBV	389359	795798	69.95%	8.524%
29	5.825	1478	1488	1502	rBV5	15150	33676	2.96%	0.361%
30	5.918	1514	1517	1520	rBV	1544	987	0.09%	0.011%
31	5.985	1526	1538	1564	rVB	236648	485203	42.65%	5.197%
32	6.362	1652	1655	1662	rVB	1754	1426	0.13%	0.015%
33	6.748	1772	1775	1777	rBV2	1156	665	0.06%	0.007%
34	6.764	1777	1780	1782	rVB2	1629	791	0.07%	0.008%
35	6.812	1792	1795	1798	rBV	1920	1167	0.10%	0.012%
36	6.912	1816	1826	1844	rBV	143230	258420	22.71%	2.768%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
 Data File : VV033089.D
 Acq On : 04 Dec 2023 10:08
 Operator : SY/MD
 Sample : VV1204MBL01
 Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.011	1854	1857	1861	rBV	1659	1286	0.11%	0.014%
38	7.243	1914	1929	1952	rBV	533300	938290	82.47%	10.050%
39	7.551	2015	2025	2046	rBV	105305	188679	16.58%	2.021%
40	7.712	2070	2075	2077	rBV	1874	1951	0.17%	0.021%
41	7.860	2119	2121	2124	rVB	1493	823	0.07%	0.009%
42	8.021	2162	2171	2194	rBV2	231875	429278	37.73%	4.598%
43	8.387	2282	2285	2289	rVB	1840	1259	0.11%	0.013%
44	8.429	2295	2298	2302	rBV	1477	1285	0.11%	0.014%
45	8.481	2312	2314	2316	rBV	1237	526	0.05%	0.006%
46	8.558	2334	2338	2341	rBV	1811	1497	0.13%	0.016%
47	8.783	2397	2408	2435	rBV	616708	1006941	88.50%	10.785%
48	9.008	2473	2478	2481	rBV	1919	1909	0.17%	0.020%
49	9.358	2581	2587	2589	rBV	2792	2809	0.25%	0.030%
50	9.439	2609	2612	2615	rBV	1693	1110	0.10%	0.012%
51	9.493	2627	2629	2635	rVB2	1770	1128	0.10%	0.012%
52	9.648	2675	2677	2682	rBV	1596	1355	0.12%	0.015%
53	9.747	2705	2708	2711	rBV	1803	1461	0.13%	0.016%
54	9.776	2715	2717	2724	rVV	1297	1186	0.10%	0.013%
55	9.979	2777	2780	2784	rBV	1675	1525	0.13%	0.016%
56	10.153	2823	2834	2848	rBV	329454	514835	45.25%	5.514%
57	10.265	2866	2869	2874	rVB	1626	1250	0.11%	0.013%
58	10.480	2933	2936	2939	rBV2	1922	1575	0.14%	0.017%
59	10.561	2958	2961	2963	rBV3	929	676	0.06%	0.007%
60	10.635	2981	2984	2988	rVB	1504	1194	0.10%	0.013%
61	10.747	3016	3019	3020	rBV	1482	934	0.08%	0.010%
62	10.802	3032	3036	3039	rBV	2108	1699	0.15%	0.018%
63	10.831	3043	3045	3048	rVV2	1438	930	0.08%	0.010%
64	10.863	3052	3055	3060	rVB3	1522	1671	0.15%	0.018%
65	11.101	3126	3129	3132	rBV2	1398	1335	0.12%	0.014%
66	11.185	3144	3155	3175	rBV	701392	1069203	93.98%	11.452%
67	11.561	3261	3272	3290	rBV	614345	973960	85.60%	10.432%
68	11.950	3389	3393	3395	rBV2	1313	1223	0.11%	0.013%
69	12.230	3477	3480	3481	rBV	1221	674	0.06%	0.007%
70	12.281	3491	3496	3499	rBV	2443	2282	0.20%	0.024%
71	12.304	3500	3503	3507	rVV2	1293	1022	0.09%	0.011%
72	12.448	3546	3548	3551	rVB	1493	719	0.06%	0.008%
73	12.570	3583	3586	3587	rBV	2495	1567	0.14%	0.017%
74	12.587	3588	3591	3599	rVB7	4396	5487	0.48%	0.059%
75	12.857	3673	3675	3679	rVB	1967	1225	0.11%	0.013%
76	12.992	3714	3717	3721	rBV	1220	1001	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
 Data File : VV033089.D
 Acq On : 04 Dec 2023 10:08
 Operator : SY/MD
 Sample : VV1204MBL01
 Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.204	3775	3783	3792	rBV5	9345	14762	1.30%	0.158%
78	13.268	3800	3803	3807	rBV	1648	1186	0.10%	0.013%
79	13.313	3813	3817	3821	rBV3	1540	1712	0.15%	0.018%
80	13.377	3831	3837	3840	rBV2	2071	2227	0.20%	0.024%
81	13.397	3840	3843	3845	rBV	1199	679	0.06%	0.007%
82	13.442	3850	3857	3872	rVB	28231	46671	4.10%	0.500%
83	13.551	3888	3891	3894	rBV	1439	1221	0.11%	0.013%
84	13.631	3913	3916	3921	rBV	2259	2362	0.21%	0.025%
85	13.683	3927	3932	3943	rVB4	9574	14157	1.24%	0.152%
86	13.725	3943	3945	3949	rBV3	1114	999	0.09%	0.011%
87	13.812	3969	3972	3974	rBV	1605	1097	0.10%	0.012%
88	13.959	4015	4018	4020	rBV	1363	972	0.09%	0.010%
89	14.181	4084	4087	4091	rVB	1650	1008	0.09%	0.011%
90	14.355	4138	4141	4145	rVB	2138	1314	0.12%	0.014%
91	14.657	4232	4235	4237	rBV2	1137	821	0.07%	0.009%
92	14.850	4292	4295	4298	rBV	1525	1231	0.11%	0.013%
93	14.911	4312	4314	4318	rVB	2336	1309	0.12%	0.014%
94	15.130	4377	4382	4385	rBV	2119	2117	0.19%	0.023%
95	15.188	4397	4400	4404	rBV2	1611	1188	0.10%	0.013%
96	15.210	4405	4407	4411	rBV2	1237	957	0.08%	0.010%
97	15.602	4527	4529	4532	rBV2	1339	801	0.07%	0.009%
98	15.795	4586	4589	4591	rBV2	1762	1156	0.10%	0.012%
99	16.509	4808	4811	4815	rBV4	2213	2266	0.20%	0.024%
100	16.689	4865	4867	4872	rBV	2514	1881	0.17%	0.020%


Sum of corrected areas: 9336109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033089.D
Acq On : 04 Dec 2023 10:08
Operator : SY/MD
Sample : VV1204MBL01
Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

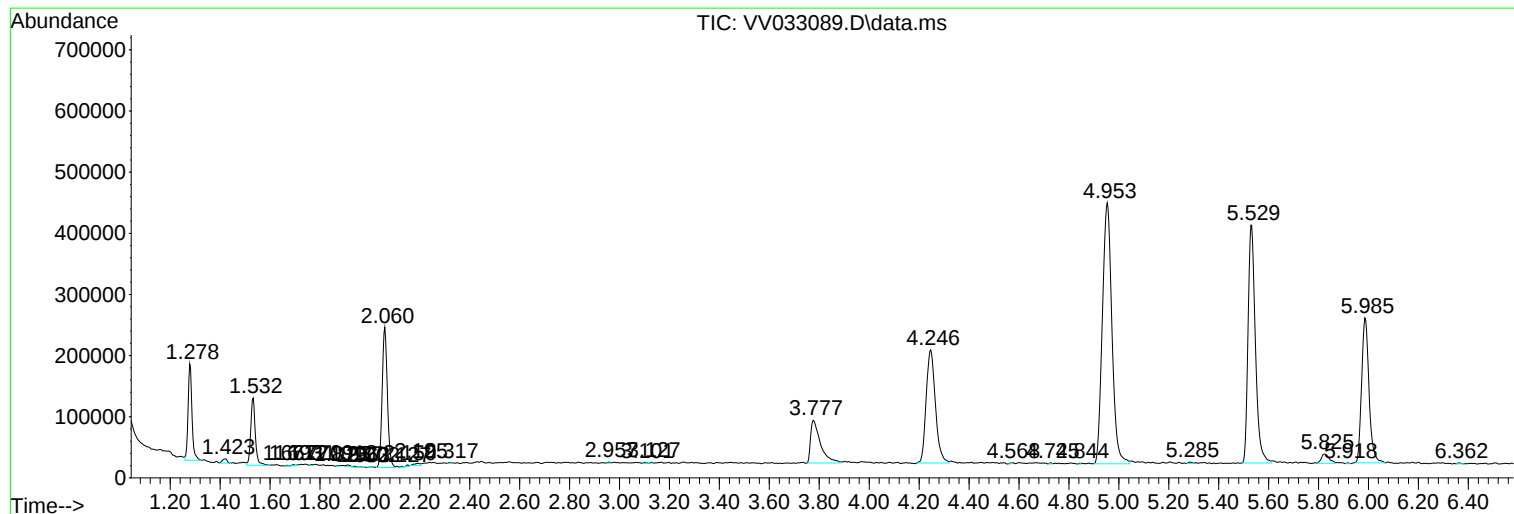

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033089.D
Acq On : 04 Dec 2023 10:08
Operator : SY/MD
Sample : VV1204MBL01
Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033089.D
Acq On : 04 Dec 2023 10:08
Operator : SY/MD
Sample : VV1204MBL01
Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------