

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
 Data File : VV033090.D
 Acq On : 04 Dec 2023 10:31
 Operator : SY/MD
 Sample : VV1204WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	137058	150121	14.33%	1.716%
2	1.423	112	119	127	rVB3	7191	11459	1.09%	0.131%
3	1.487	134	139	144	rBV5	2070	2677	0.26%	0.031%
4	1.532	145	153	168	rVB	97048	120837	11.53%	1.381%
5	1.632	180	184	187	rBV2	1258	1099	0.10%	0.013%
6	1.648	187	189	190	rBV2	617	233	0.02%	0.003%
7	1.683	196	200	201	rBV2	1261	811	0.08%	0.009%
8	1.699	201	205	208	rVB3	943	830	0.08%	0.009%
9	1.722	208	212	213	rBV2	1577	1011	0.10%	0.012%
10	1.796	233	235	242	rVB2	1476	1346	0.13%	0.015%
11	1.828	242	245	252	rVV3	1473	2000	0.19%	0.023%
12	1.873	256	259	261	rVV2	1409	947	0.09%	0.011%
13	1.886	261	263	265	rVV	1628	921	0.09%	0.011%
14	1.912	265	271	277	rVB2	2743	4103	0.39%	0.047%
15	1.960	284	286	291	rVB2	824	732	0.07%	0.008%
16	2.002	291	299	301	rBV2	1292	1466	0.14%	0.017%
17	2.014	301	303	307	rVB3	558	221	0.02%	0.003%
18	2.059	307	317	336	rBV	205531	303166	28.93%	3.465%
19	2.127	336	338	341	rVB3	1364	652	0.06%	0.007%
20	2.153	341	346	348	rBV	2654	2635	0.25%	0.030%
21	2.172	348	352	354	rBV	2342	1632	0.16%	0.019%
22	2.191	354	358	361	rBV	1964	1840	0.18%	0.021%
23	2.275	381	384	387	rBV	1511	1198	0.11%	0.014%
24	2.339	399	404	409	rBV	2138	2544	0.24%	0.029%
25	2.658	499	503	508	rVB	2248	1956	0.19%	0.022%
26	3.619	799	802	808	rBV	1689	1837	0.18%	0.021%
27	3.783	843	853	875	rBV	65083	173682	16.57%	1.985%
28	4.194	978	981	983	rBV	1786	1313	0.13%	0.015%
29	4.249	984	998	1026	rVV	175023	444728	42.44%	5.083%
30	4.458	1061	1063	1065	rBV	1471	942	0.09%	0.011%
31	4.702	1136	1139	1143	rBV	1581	1139	0.11%	0.013%
32	4.956	1202	1218	1247	rBV2	391844	1047886	100.00%	11.977%
33	5.198	1290	1293	1296	rBV	2568	1716	0.16%	0.020%
34	5.381	1347	1350	1352	rBV	1816	1145	0.11%	0.013%
35	5.532	1386	1397	1421	rBV	371117	764111	72.92%	8.734%
36	5.828	1481	1489	1500	rVB3	13359	24727	2.36%	0.283%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
 Data File : VV033090.D
 Acq On : 04 Dec 2023 10:31
 Operator : SY/MD
 Sample : VV1204WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK231

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.989	1527	1539	1561	rBV	220635	454221	43.35%	5.192%
38	6.911	1817	1826	1844	rBV2	131715	243487	23.24%	2.783%
39	7.243	1918	1929	1949	rBV	492232	858902	81.97%	9.817%
40	7.551	2017	2025	2046	rBV	95296	167268	15.96%	1.912%
41	8.024	2163	2172	2203	rBV	233281	434430	41.46%	4.965%
42	8.214	2228	2231	2235	rBV	2021	1724	0.16%	0.020%
43	8.413	2291	2293	2296	rBV2	1271	839	0.08%	0.010%
44	8.593	2347	2349	2352	rBV2	1535	684	0.07%	0.008%
45	8.786	2398	2409	2436	rBV	591004	977644	93.30%	11.174%
46	9.262	2554	2557	2562	rVB2	2702	1860	0.18%	0.021%
47	9.548	2643	2646	2651	rBV2	2178	2137	0.20%	0.024%
48	9.914	2757	2760	2765	rBV	1713	1412	0.13%	0.016%
49	9.963	2771	2775	2778	rBV	2294	2274	0.22%	0.026%
50	10.098	2814	2817	2820	rBV	1335	1006	0.10%	0.011%
51	10.152	2824	2834	2854	rVB	306084	496567	47.39%	5.676%
52	10.255	2862	2866	2873	rBV	1993	2269	0.22%	0.026%
53	10.596	2969	2972	2974	rBV	1474	1016	0.10%	0.012%
54	11.127	3131	3137	3142	rBV7	2246	3382	0.32%	0.039%
55	11.185	3144	3155	3174	rBV	682204	1040358	99.28%	11.891%
56	11.419	3225	3228	3231	rBV	1254	794	0.08%	0.009%
57	11.561	3260	3272	3297	rBV	594402	927136	88.48%	10.597%
58	11.947	3388	3392	3396	rBV	2172	2210	0.21%	0.025%
59	12.088	3433	3436	3445	rVB	1539	2034	0.19%	0.023%
60	12.130	3446	3449	3451	rBV	1327	935	0.09%	0.011%
61	12.586	3589	3591	3594	rBV3	1587	817	0.08%	0.009%
62	12.811	3658	3661	3666	rBV	1801	1735	0.17%	0.020%
63	12.924	3694	3696	3698	rBV	1216	756	0.07%	0.009%
64	13.149	3763	3766	3770	rBV3	1523	1194	0.11%	0.014%
65	13.207	3780	3784	3788	rBV4	2620	2825	0.27%	0.032%
66	13.445	3852	3858	3865	rBV3	8481	13674	1.30%	0.156%
67	13.606	3906	3908	3910	rBV	1219	775	0.07%	0.009%
68	13.680	3928	3931	3932	rBV3	2224	1301	0.12%	0.015%
69	13.731	3945	3947	3950	rBV	1811	1323	0.13%	0.015%
70	13.946	4011	4014	4016	rBV	1717	1041	0.10%	0.012%
71	14.139	4072	4074	4081	rVB	2824	2846	0.27%	0.033%
72	14.184	4081	4088	4091	rBV	2196	2791	0.27%	0.032%
73	14.737	4256	4260	4263	rBV	1970	1648	0.16%	0.019%
74	14.930	4315	4320	4323	rBV	2617	2631	0.25%	0.030%
75	15.287	4428	4431	4434	rBV	2023	1264	0.12%	0.014%
76	15.390	4460	4463	4466	rBV	1648	1142	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033090.D
Acq On : 04 Dec 2023 10:31
Operator : SY/MD
Sample : VV1204WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis

77	15.512	4498	4501	4503	rBV2	2017	1330	0.13%	0.015%
78	15.651	4538	4544	4549	rBV3	1999	3098	0.30%	0.035%
79	16.062	4670	4672	4673	rBV2	1737	833	0.08%	0.010%
80	16.258	4731	4733	4739	rVB	2538	1747	0.17%	0.020%




Sum of corrected areas: 8749023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033090.D
Acq On : 04 Dec 2023 10:31
Operator : SY/MD
Sample : VV1204WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

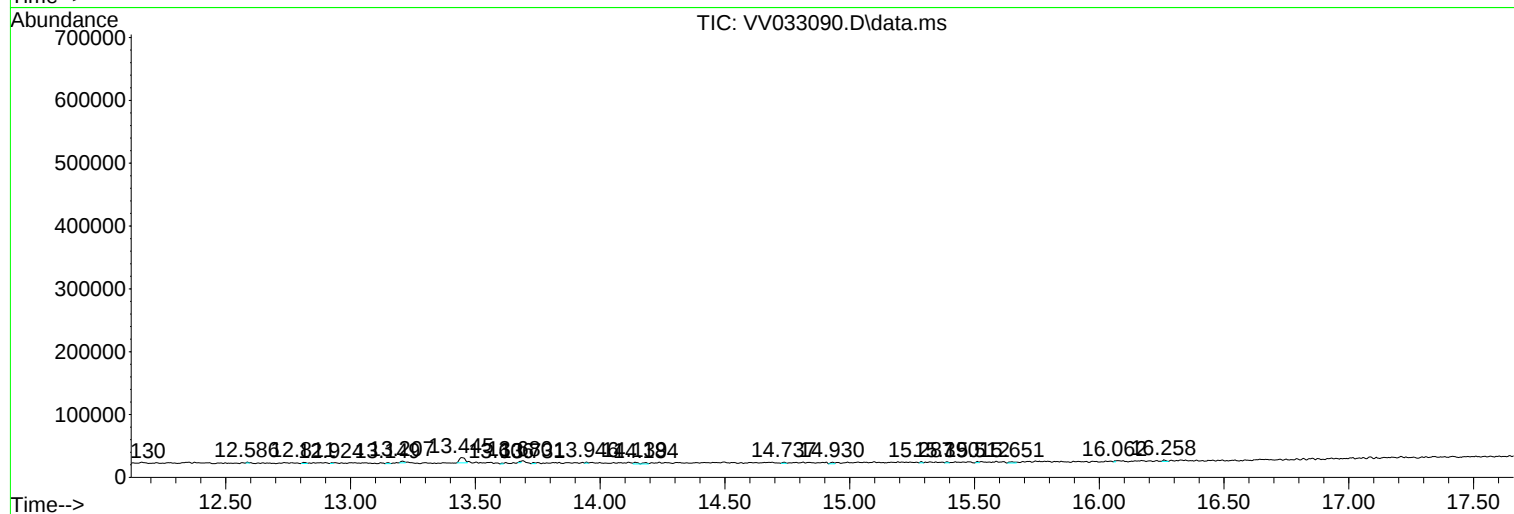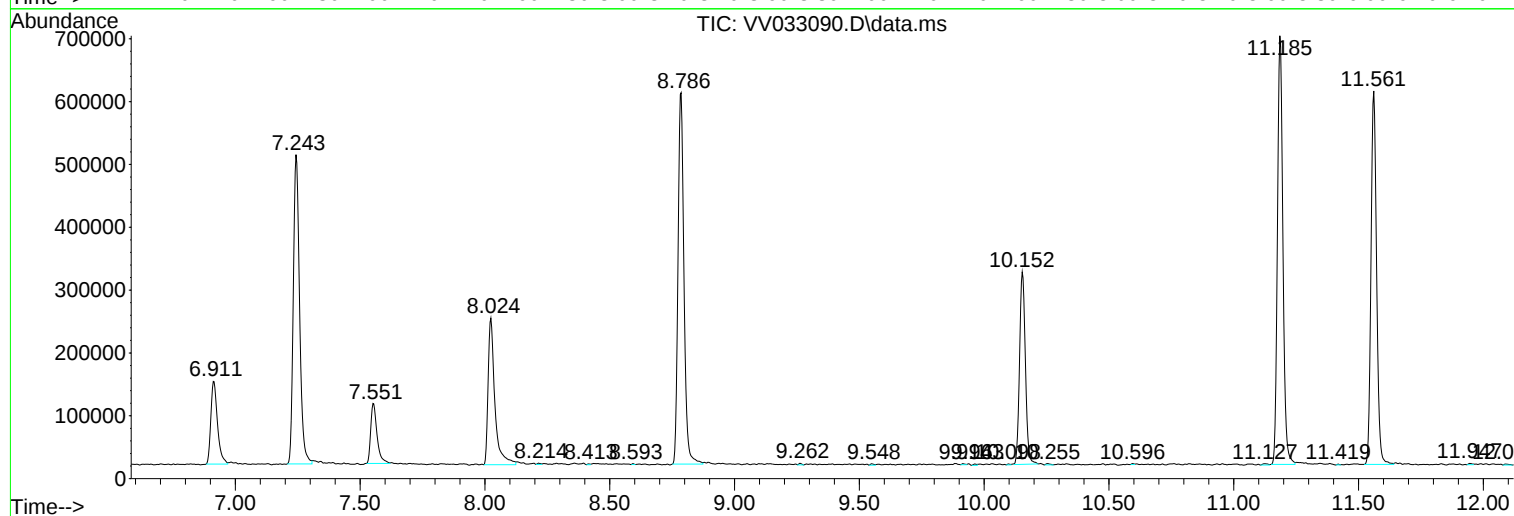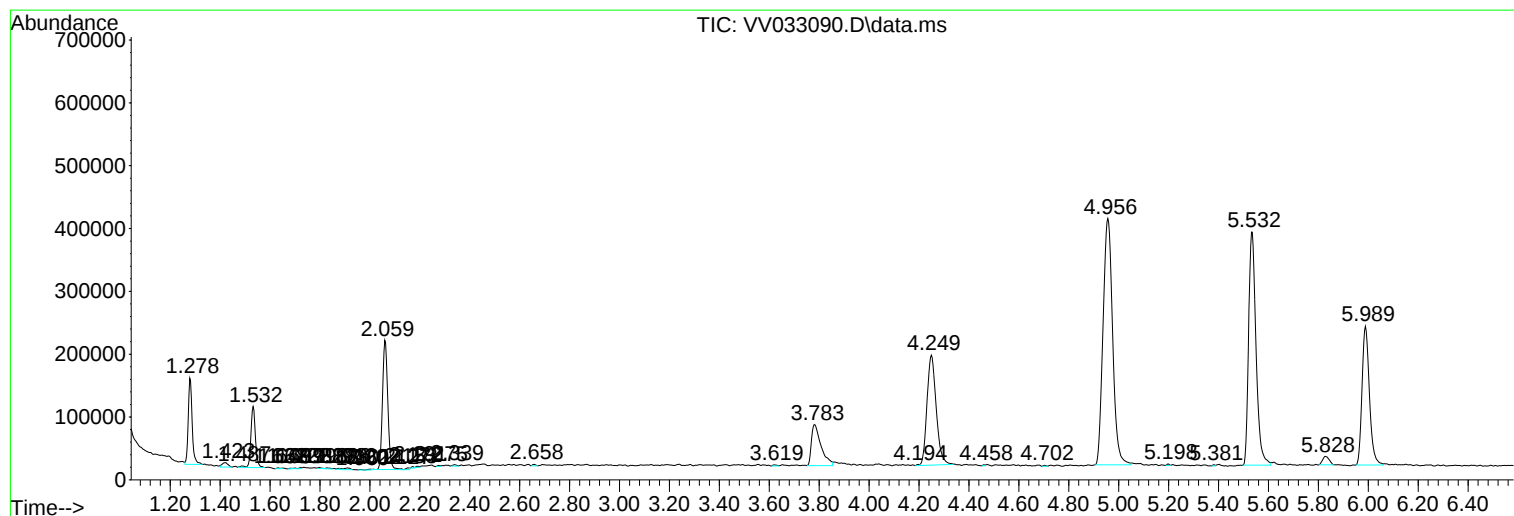

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033090.D
Acq On : 04 Dec 2023 10:31
Operator : SY/MD
Sample : VV1204WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033090.D
Acq On : 04 Dec 2023 10:31
Operator : SY/MD
Sample : VV1204WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK231

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------