

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120423\
 Data File : VW033091.D
 Acq On : 04 Dec 2023 10:57
 Operator : SY/MD
 Sample : 04929-08MEDL 4X
 Misc : 3.82G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	154360	172625	5.71%	1.354%
2	1.429	109	121	122	rBV4	14812	20354	0.67%	0.160%
3	1.513	141	147	165	rVB	99428	133072	4.40%	1.044%
4	1.645	185	188	190	rBV2	589	365	0.01%	0.003%
5	1.667	192	195	198	rVV	826	575	0.02%	0.005%
6	1.700	202	205	206	rBV2	1232	802	0.03%	0.006%
7	1.806	235	238	244	rBV2	1341	1302	0.04%	0.010%
8	1.947	280	282	291	rVB	1707	1976	0.07%	0.015%
9	1.986	291	294	299	rBV3	1299	1345	0.04%	0.011%
10	2.015	299	303	305	rBV2	1014	713	0.02%	0.006%
11	2.053	305	315	331	rBV	221947	322981	10.68%	2.533%
12	2.114	331	334	340	rVB4	1060	924	0.03%	0.007%
13	2.166	340	350	352	rBV	3792	5698	0.19%	0.045%
14	2.211	361	364	365	rBV2	1517	981	0.03%	0.008%
15	2.558	466	472	480	rVB3	5907	9240	0.31%	0.072%
16	3.307	700	705	707	rBV	2048	2131	0.07%	0.017%
17	3.783	845	853	883	rBV	53498	147993	4.89%	1.161%
18	4.246	982	997	1029	rVB2	181953	463312	15.32%	3.633%
19	4.555	1090	1093	1096	rBV	1854	1436	0.05%	0.011%
20	4.953	1201	1217	1242	rBV2	424662	1113465	36.81%	8.732%
21	5.336	1333	1336	1341	rBV2	1599	1646	0.05%	0.013%
22	5.532	1386	1397	1425	rBV	370076	760056	25.13%	5.960%
23	5.831	1482	1490	1500	rVB6	9242	17877	0.59%	0.140%
24	5.986	1526	1538	1565	rBV2	232405	482114	15.94%	3.781%
25	6.365	1653	1656	1658	rBV	1581	1088	0.04%	0.009%
26	6.420	1671	1673	1679	rBV	1394	1021	0.03%	0.008%
27	6.912	1816	1826	1842	rBV	149636	267332	8.84%	2.096%
28	7.243	1917	1929	1954	rBV	526200	939821	31.07%	7.370%
29	7.551	2016	2025	2039	rBV	107272	184370	6.10%	1.446%
30	8.024	2163	2172	2191	rBV	223345	408306	13.50%	3.202%
31	8.371	2276	2280	2287	rVB2	2021	2844	0.09%	0.022%
32	8.783	2398	2408	2437	rBV	601350	1110874	36.73%	8.711%
33	9.297	2565	2568	2571	rBV	1722	1286	0.04%	0.010%
34	10.030	2792	2796	2802	rBV2	1817	2803	0.09%	0.022%
35	10.153	2823	2834	2851	rBV	342975	543394	17.97%	4.261%
36	10.374	2897	2903	2908	rBV	2927	3563	0.12%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
 Data File : VV033091.D
 Acq On : 04 Dec 2023 10:57
 Operator : SY/MD
 Sample : 04929-08MEDL 4X
 Misc : 3.82G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	10.509	2942	2945	2946	rBV	1467	918	0.03%	0.007%
38	10.593	2968	2971	2977	rBV	1587	2061	0.07%	0.016%
39	11.059	3113	3116	3118	rBV	1719	933	0.03%	0.007%
40	11.117	3124	3134	3145	rBV	260800	402222	13.30%	3.154%
41	11.188	3145	3156	3159	rBV	821655	1181518	39.06%	9.265%
42	11.577	3261	3277	3298	rBV2	1394911	3024547	100.00%	23.718%
43	12.130	3446	3449	3454	rBV	1542	1474	0.05%	0.012%
44	12.435	3542	3544	3548	rVB	1718	967	0.03%	0.008%
45	12.587	3584	3591	3600	rBV4	8505	13376	0.44%	0.105%
46	13.075	3738	3743	3746	rBV	2019	2160	0.07%	0.017%
47	13.201	3770	3782	3801	rBV	620545	966038	31.94%	7.575%
48	13.448	3854	3859	3869	rVB3	5845	7629	0.25%	0.060%
49	13.686	3923	3933	3941	rBV3	4909	9369	0.31%	0.073%
50	14.763	4265	4268	4277	rVB5	5559	6424	0.21%	0.050%
51	14.831	4286	4289	4293	rVB	2292	1804	0.06%	0.014%
52	15.583	4521	4523	4526	rVB2	2202	1062	0.04%	0.008%

Sum of corrected areas: 12752187




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033091.D
Acq On : 04 Dec 2023 10:57
Operator : SY/MD
Sample : 04929-08MEDL 4X
Misc : 3.82G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

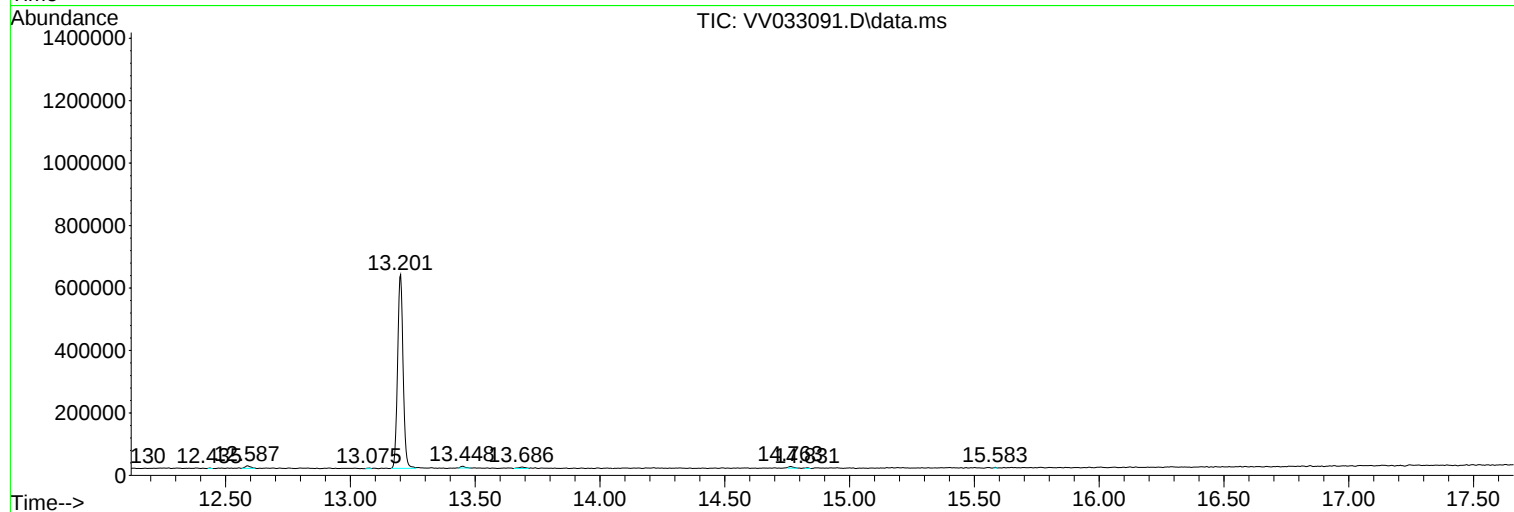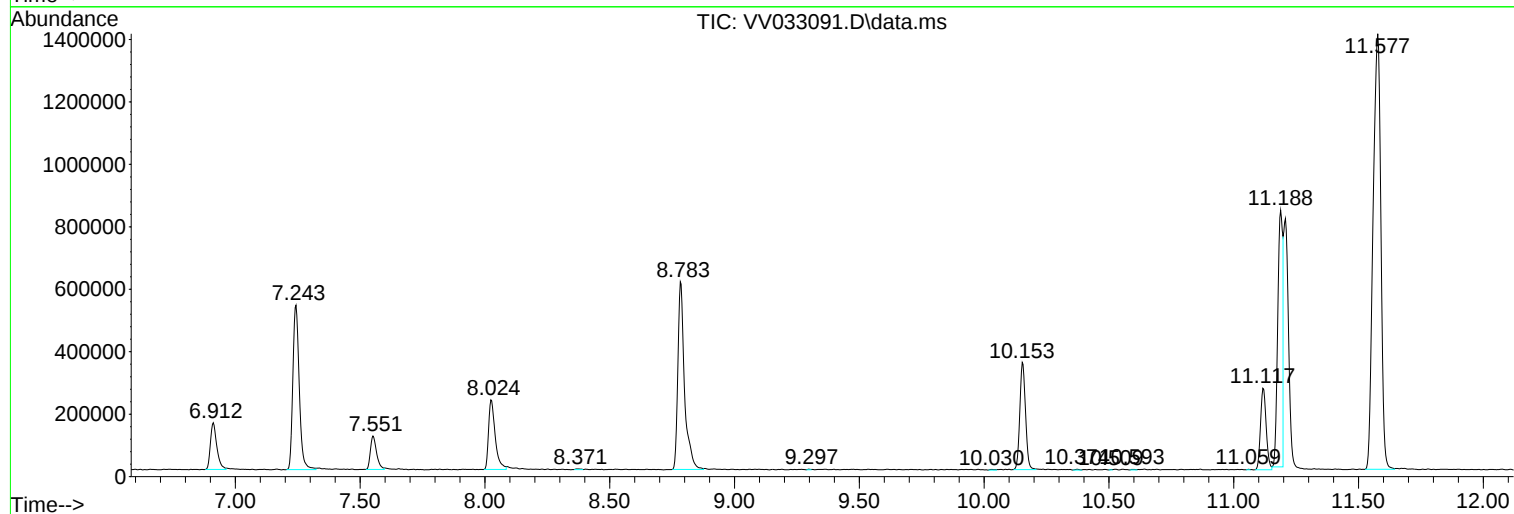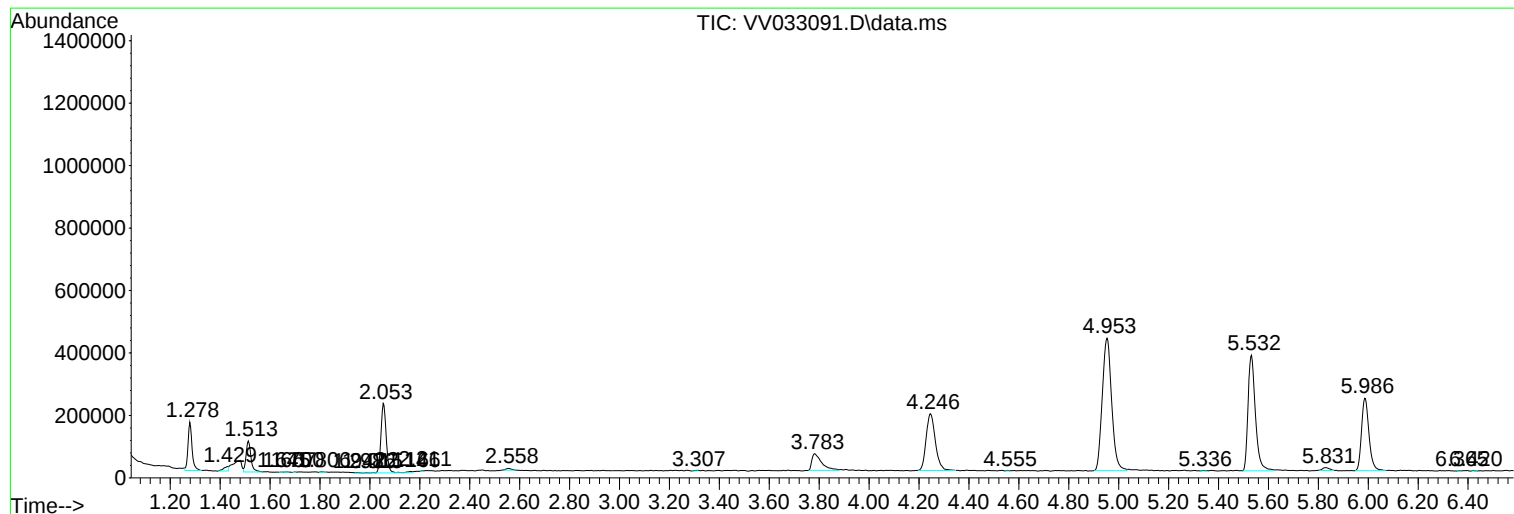

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033091.D
Acq On : 04 Dec 2023 10:57
Operator : SY/MD
Sample : 04929-08MEDL 4X
Misc : 3.82G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033091.D
Acq On : 04 Dec 2023 10:57
Operator : SY/MD
Sample : 04929-08MEDL 4X
Misc : 3.82G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc