


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120423\
Data File : VV033087.D
Acq On : 04 Dec 2023 08:51
Operator : SY/MD
Sample : BFB239
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB239

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis
Last Update : Tue Dec 05 03:20:48 2023

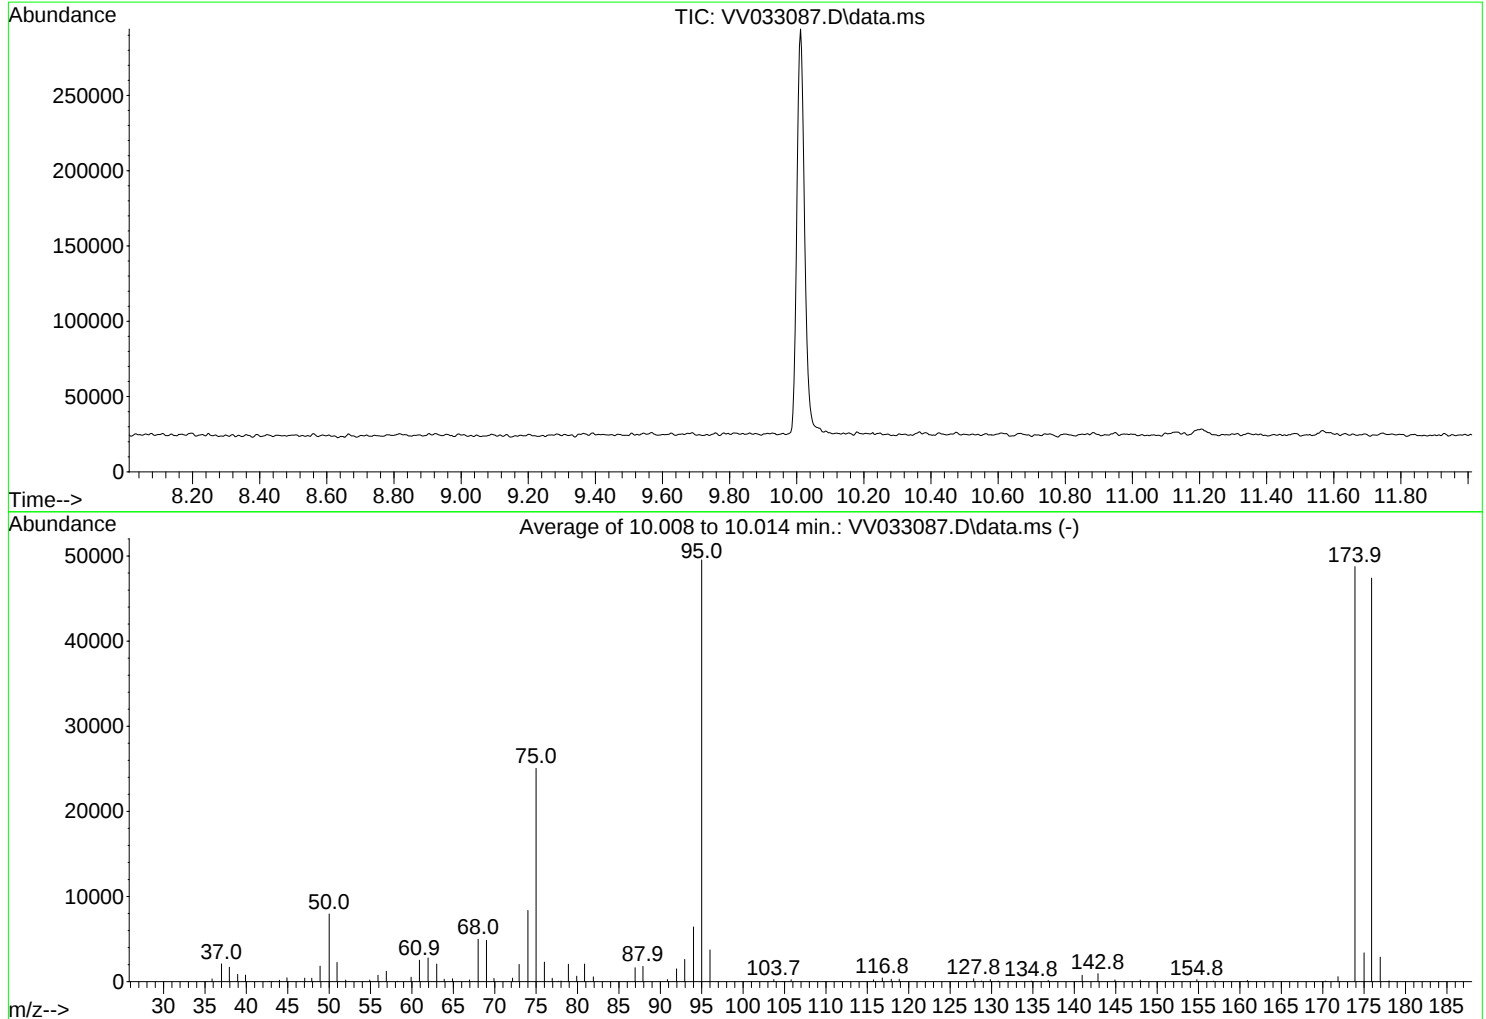

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	7946	PASS
75	95	30	80	50.6	25056	PASS
95	95	100	100	100.0	49547	PASS
96	95	5	9	7.5	3716	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.4	48757	PASS
175	174	5	9	6.9	3382	PASS
176	174	95	105	97.2	47408	PASS
177	176	5	10	6.0	2868	PASS

m/z	Abundance
35.90	766.0
37.80	335.0
39.10	124.0
39.90	23768.0
43.90	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
35.90	947.0
37.00	2128.0
38.00	2041.0
38.90	964.0
39.90	24592.0
43.10	106.0
44.00	313.0
44.90	441.0
47.00	435.0
47.90	429.0
48.90	1884.0
50.00	8035.0
51.00	2155.0
52.00	209.0
54.90	207.0
55.90	753.0
56.90	1227.0
58.30	118.0
59.90	451.0
60.90	2537.0
62.00	2741.0
63.00	2010.0
63.90	383.0
65.00	386.0
66.90	178.0
68.00	5128.0
69.00	4849.0
69.90	421.0
72.20	365.0
72.90	2028.0
74.00	8278.0
75.00	25400.0
76.00	2359.0
77.00	290.0
78.00	112.0
78.90	2000.0
79.90	668.0
80.80	2182.0
81.90	582.0
87.00	1747.0
87.90	1896.0
90.90	279.0
91.90	1469.0
93.00	2621.0
94.00	6301.0
95.00	48760.0
96.00	3758.0
103.70	258.0
104.80	106.0
105.80	167.0
115.70	197.0
116.80	460.0
117.90	252.0
118.90	288.0
127.80	370.0
128.80	117.0
129.80	238.0
134.80	133.0
136.80	148.0
140.90	765.0
142.90	907.0
144.90	187.0
148.00	202.0
154.80	237.0
156.80	138.0
160.90	123.0
171.90	543.0
173.90	47248.0
175.00	3227.0
175.90	46024.0
177.00	2754.0
178.00	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
35.90	1118.0
37.00	2132.0
38.00	2080.0
39.00	1019.0
39.90	24752.0
44.10	302.0
44.90	478.0
47.00	431.0
47.90	412.0
48.90	1859.0
50.00	8173.0
50.90	2313.0
52.00	184.0
54.90	197.0
55.90	770.0
56.90	1254.0
59.90	561.0
60.90	2560.0
62.00	2919.0
63.00	2161.0
63.90	288.0
64.90	352.0
66.90	226.0
68.00	5150.0
69.00	4953.0
69.90	387.0
72.10	461.0
73.00	2071.0
74.00	8575.0
75.00	25848.0
76.00	2355.0
77.00	320.0
78.00	117.0
78.90	2097.0
79.90	665.0
80.90	2115.0
81.90	586.0
87.00	1688.0
87.90	1803.0
90.90	246.0
91.90	1533.0
93.00	2712.0
94.00	6582.0
95.00	51112.0
96.00	3848.0
103.70	260.0
105.80	216.0
115.70	215.0
116.80	445.0
117.90	285.0
118.90	301.0
127.80	338.0
128.80	109.0
129.90	263.0
130.80	102.0
134.80	109.0
136.80	168.0
141.00	815.0
142.80	1020.0
144.90	216.0
148.00	199.0
154.80	261.0
156.80	107.0
160.90	179.0
170.30	105.0
171.80	636.0
173.90	50344.0
175.00	3480.0
175.90	49080.0
176.90	2957.0
178.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239

m/z	Abundance
35.90	1201.0
37.00	1976.0
38.00	1970.0
39.00	937.0
39.90	24264.0
42.80	109.0
44.10	329.0
44.90	437.0
47.10	398.0
47.90	322.0
48.90	1705.0
50.00	7631.0
50.90	2296.0
52.00	181.0
54.90	176.0
55.90	718.0
56.90	1183.0
59.90	558.0
60.90	2476.0
61.90	2678.0
63.00	2018.0
63.90	196.0
64.80	307.0
67.00	204.0
68.00	4662.0
69.00	4774.0
69.90	313.0
72.10	412.0
73.00	1997.0
74.00	8264.0
75.00	23920.0
76.00	2171.0
76.80	279.0
77.00	279.0
77.70	163.0
78.90	2027.0
79.90	581.0
80.90	1903.0
81.90	534.0
86.90	1478.0
87.90	1663.0
90.80	211.0
92.00	1501.0
92.90	2493.0
94.00	6397.0
95.00	48768.0
96.00	3543.0
103.70	234.0
105.80	270.0
115.80	244.0
116.80	399.0
117.90	294.0
118.80	282.0
127.90	283.0
129.90	242.0
130.80	102.0
136.90	160.0
141.00	695.0
142.80	909.0
144.90	221.0
147.80	160.0
154.80	220.0
160.90	181.0
170.40	140.0
171.80	572.0
173.90	48680.0
175.00	3438.0
175.90	47120.0
176.90	2893.0

Instrument :
MSVOA_V
ClientSampleId :
BFB239