




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039465.D
Acq On : 04 Dec 2025 13:03
Operator : SY/MD
Sample : Q3756-08
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-13B-47.5-120225-SIM

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:09:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

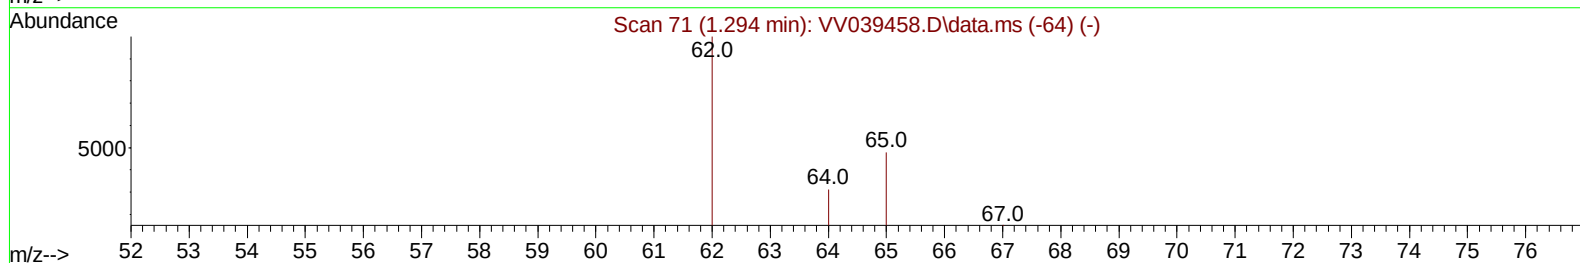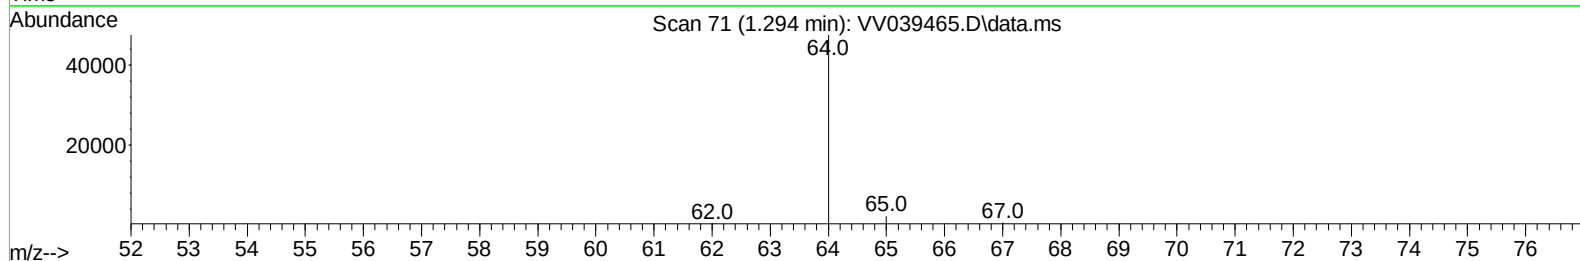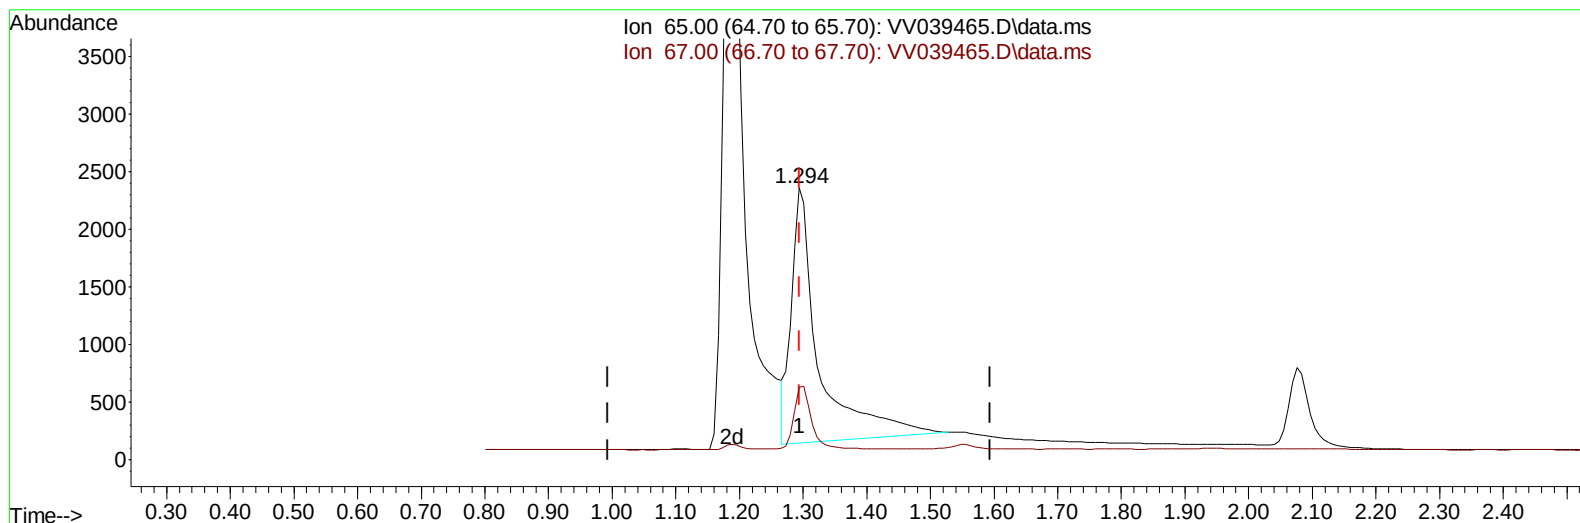

TIC: VV039465.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 1.04 ug/L

response 6703

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	15.71#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039465.D
Acq On : 04 Dec 2025 13:03
Operator : SY/MD
Sample : Q3756-08
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-13B-47.5-120225-SIM

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:09:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

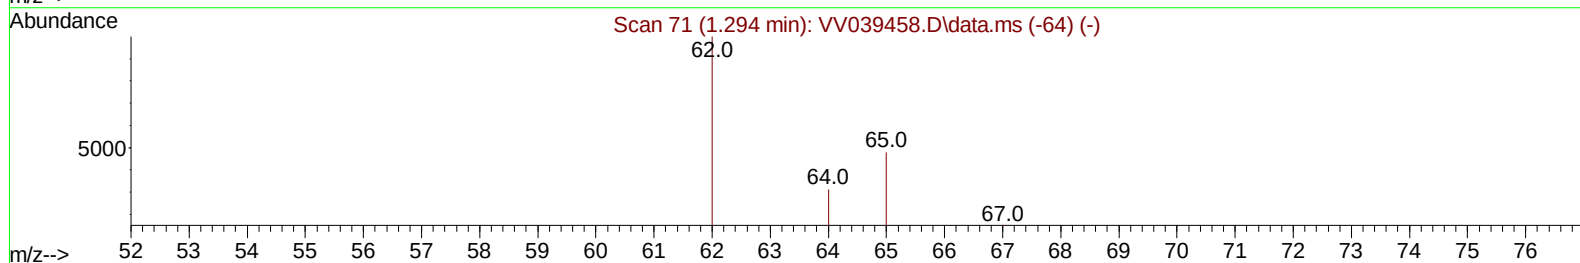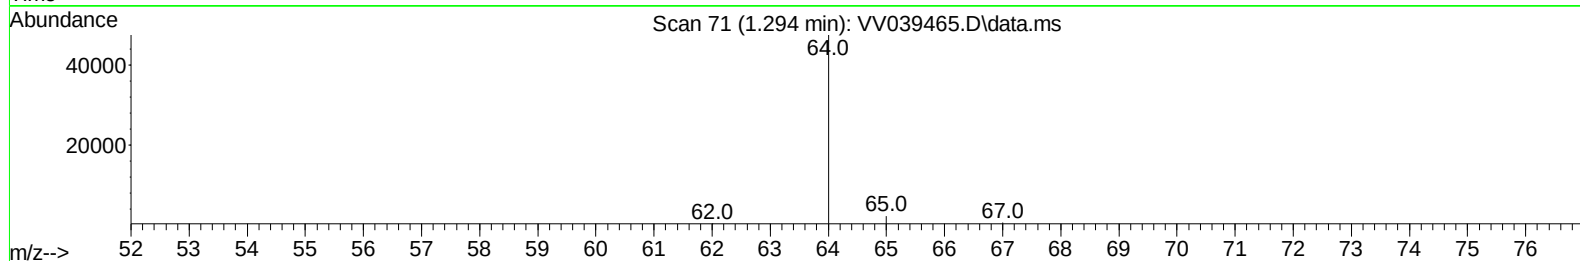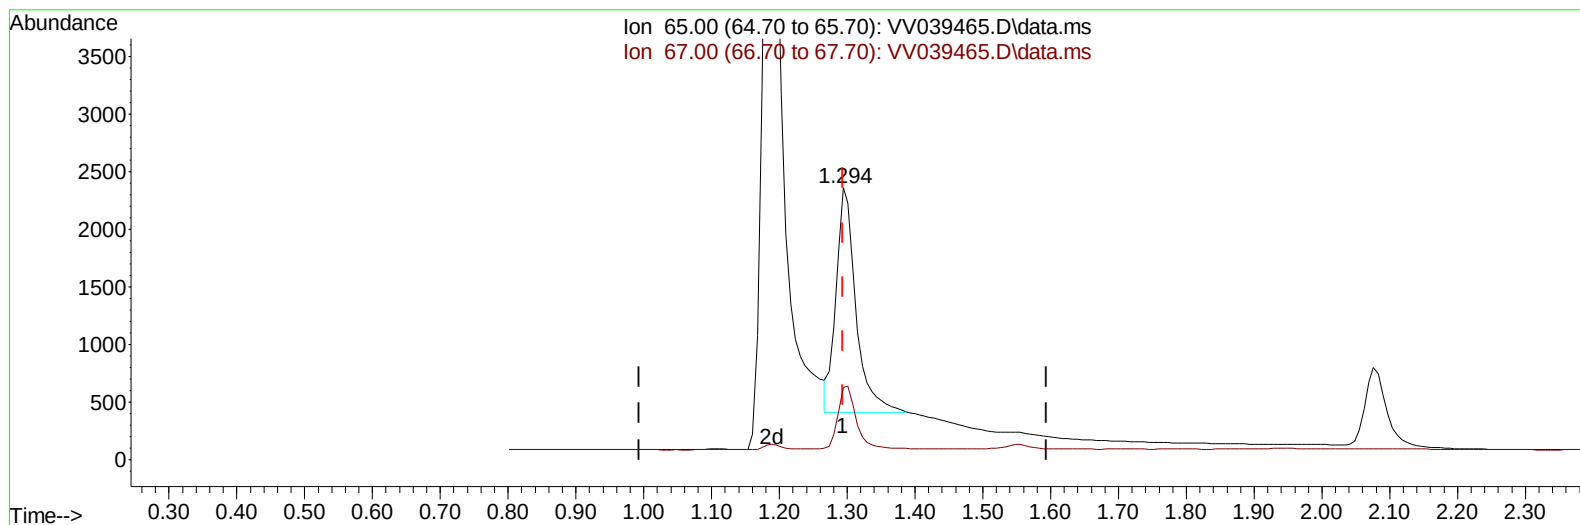

TIC: VV039465.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.62 ug/L m

response 3995

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	26.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
 Data File : VV039465.D
 Acq On : 04 Dec 2025 13:03
 Operator : SY/MD
 Sample : Q3756-08
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-13B-47.5-120225-SIM

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
 Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:09:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6414	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6408	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	3306	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3995m	0.619	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	=	124.000%	
4) 1,2-Dichloroethane-d4	4.993	65	1926	0.451	ug/L	0.02
Spiked Amount	0.500	Range 70 - 130	Recovery	=	90.000%	
7) 1,2-Dichloropropane-d6	5.995	67	2269	0.420	ug/L	-0.02
Spiked Amount	0.500	Range 60 - 140	Recovery	=	84.000%	
8) Toluene-d8	7.253	98	4165	0.457	ug/L	0.02
Spiked Amount	0.500	Range 70 - 130	Recovery	=	92.000%	
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1632	0.536	ug/L	0.00
Spiked Amount	0.500	Range 65 - 120	Recovery	=	108.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039465.D
Acq On : 04 Dec 2025 13:03
Operator : SY/MD
Sample : Q3756-08
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-13B-47.5-120225-SIM

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:09:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

