




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039466.D
Acq On : 04 Dec 2025 13:40
Operator : SY/MD
Sample : VIBLK228
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK228

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:09:55 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

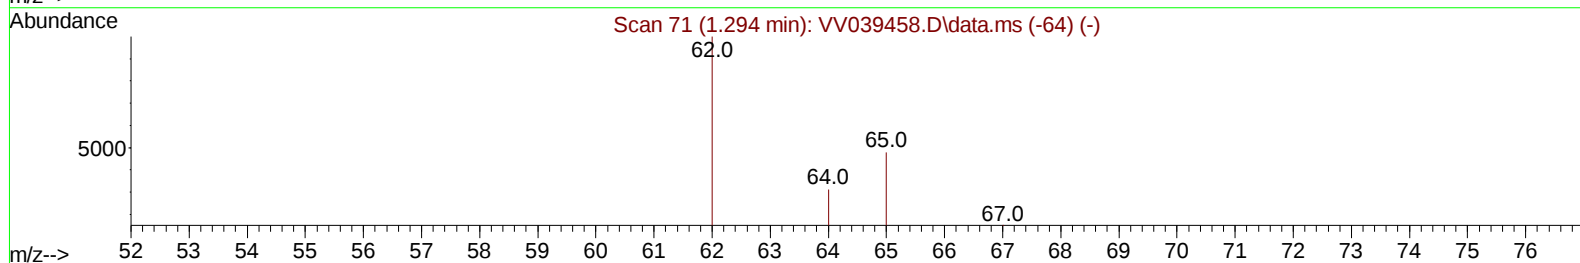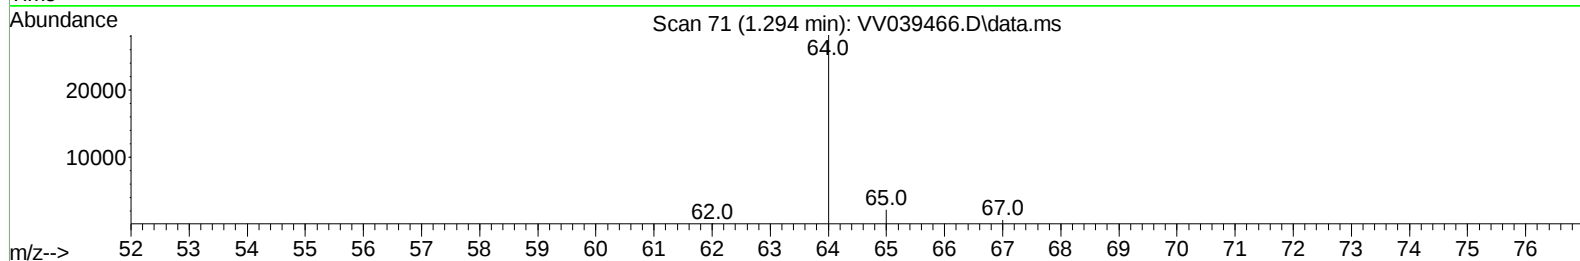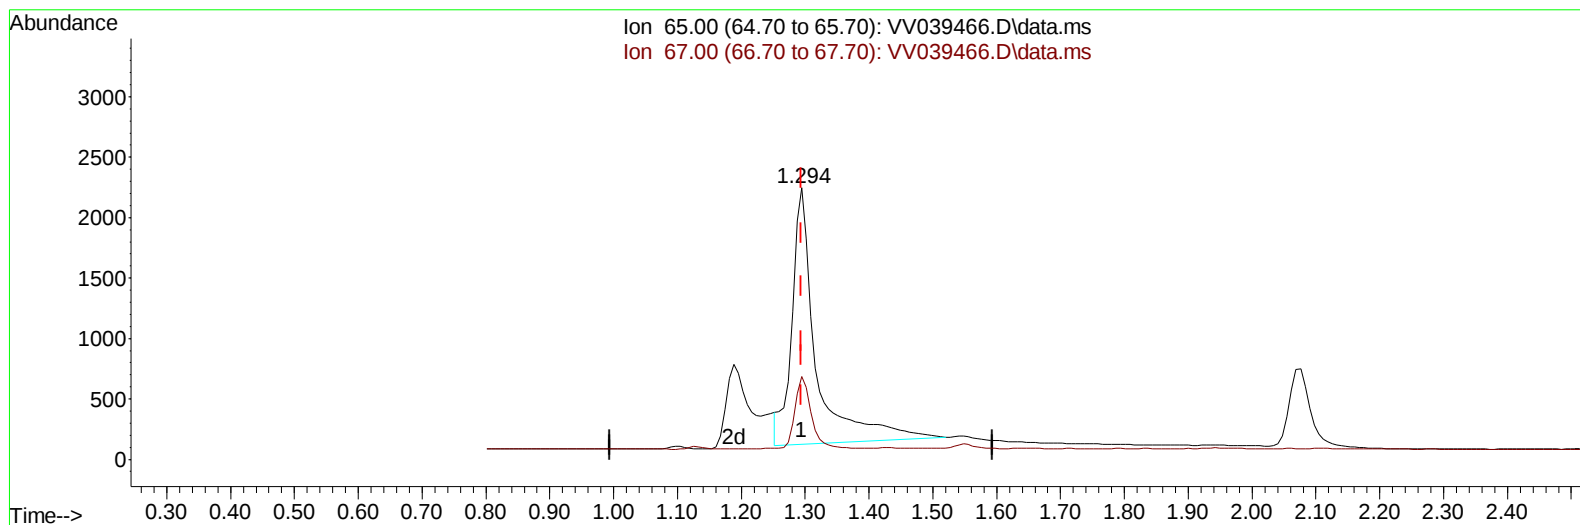

TIC: VV039466.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.90 ug/L

response 5639

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	19.22#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039466.D
Acq On : 04 Dec 2025 13:40
Operator : SY/MD
Sample : VIBLK228
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK228

Manual IntegrationsAPPROVED

Quant Time: Dec 05 00:09:55 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

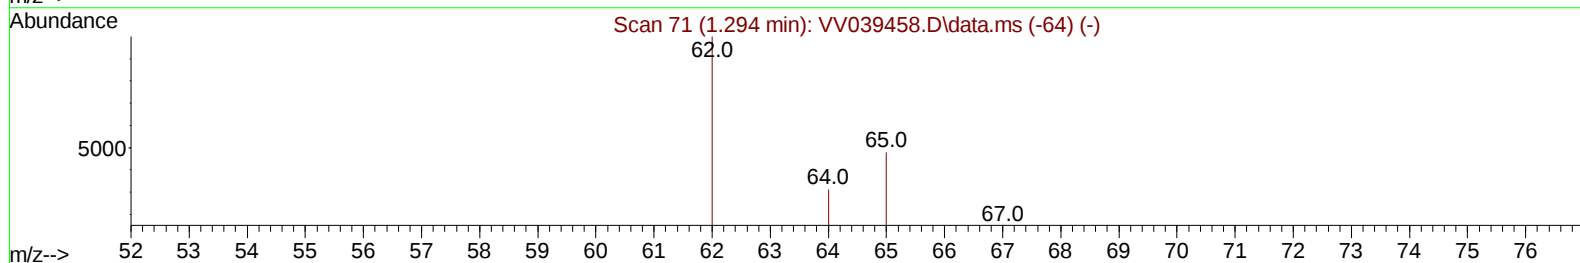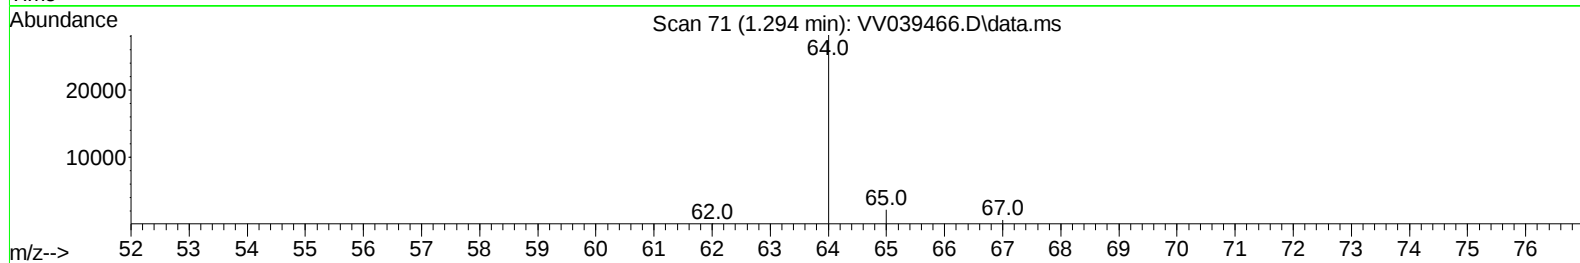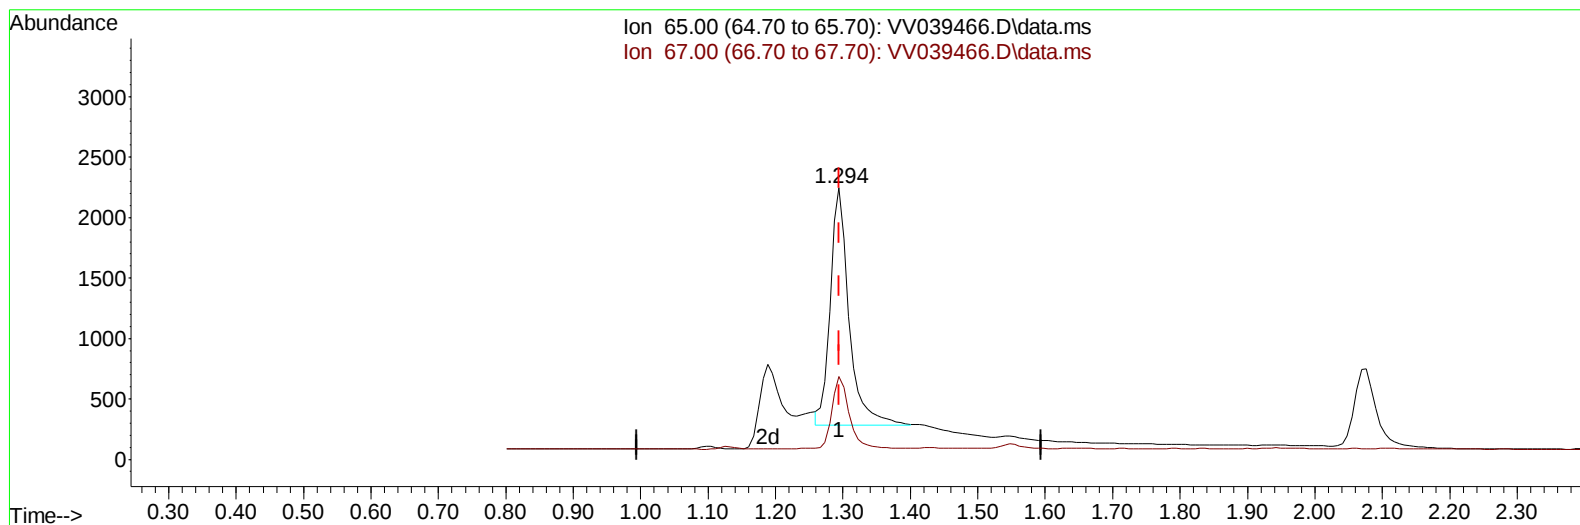

TIC: VV039466.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.61 ug/L m

response 3792

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	28.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
 Data File : VV039466.D
 Acq On : 04 Dec 2025 13:40
 Operator : SY/MD
 Sample : VIBLK228
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK228

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
 Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:09:55 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6215	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	5937	0.500	ug/L	0.00
12) 1,4-Dichlorobenzene-d4	11.197	152	3041	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3792m	0.607	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	=	122.000%	
4) 1,2-Dichloroethane-d4	4.969	65	1841	0.445	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	=	88.000%	
7) 1,2-Dichloropropane-d6	5.995	67	2093	0.418	ug/L	-0.02
Spiked Amount	0.500	Range 60 - 140	Recovery	=	84.000%	
8) Toluene-d8	7.253	98	4038	0.478	ug/L	0.02
Spiked Amount	0.500	Range 70 - 130	Recovery	=	96.000%	
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1594	0.565	ug/L	0.00
Spiked Amount	0.500	Range 65 - 120	Recovery	=	112.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039466.D
Acq On : 04 Dec 2025 13:40
Operator : SY/MD
Sample : VIBLK228
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK228

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:09:55 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

