




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039467.D
Acq On : 04 Dec 2025 14:01
Operator : SY/MD
Sample : Q3756-04DL 20X
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BR-01-190-120225-SIMDL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

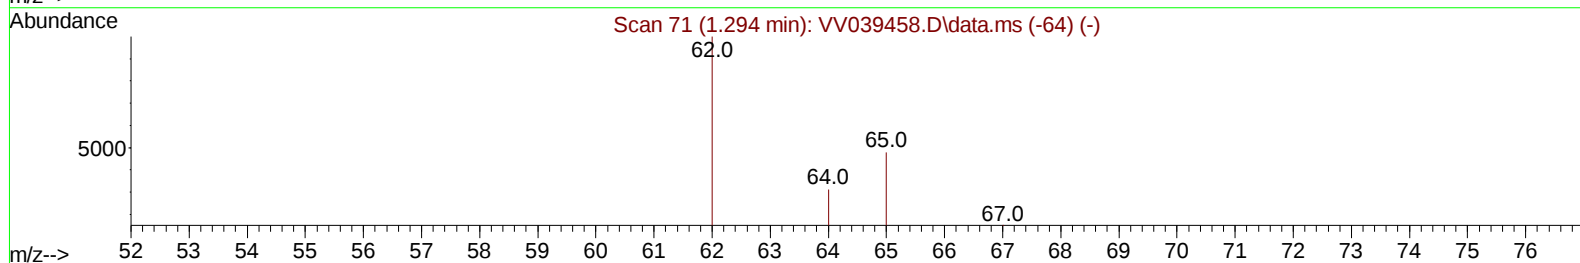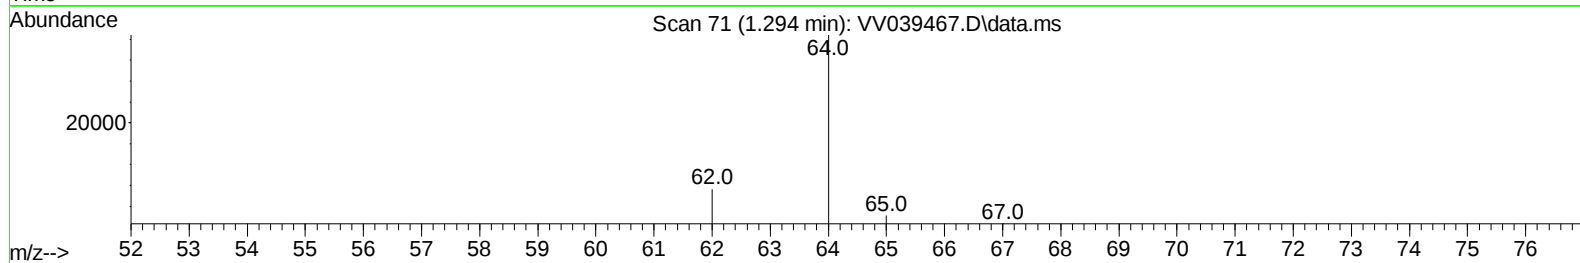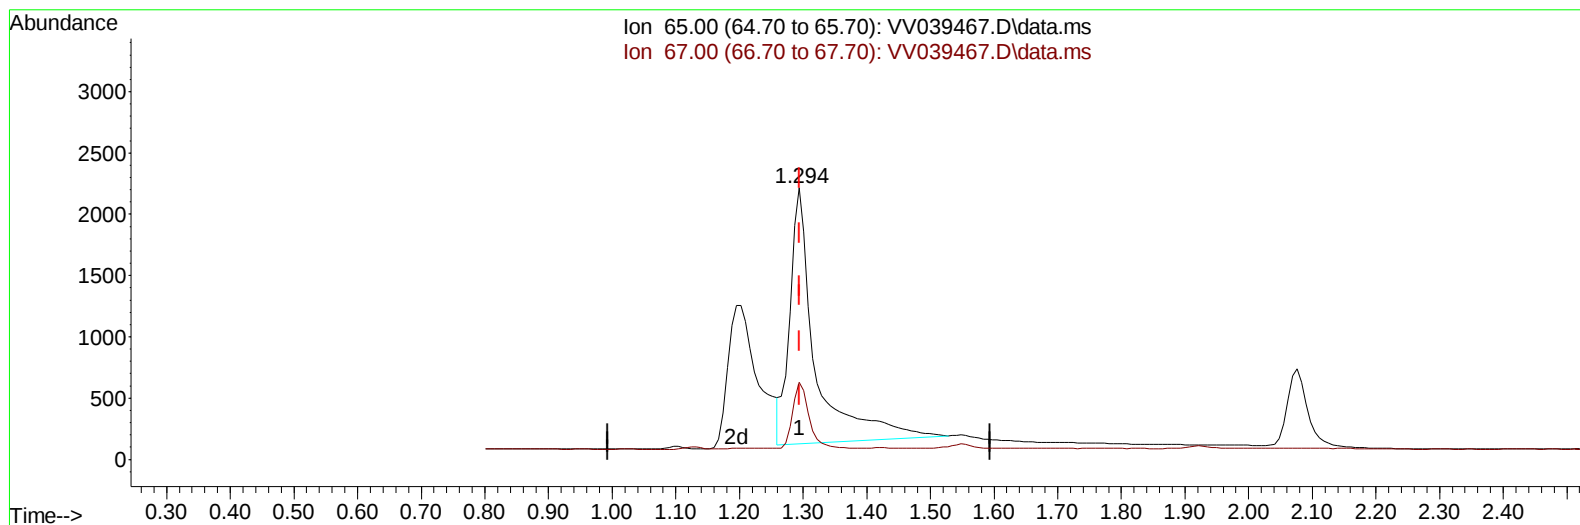

TIC: VV039467.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 1.03 ug/L

response 5880

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	16.65#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039467.D
Acq On : 04 Dec 2025 14:01
Operator : SY/MD
Sample : Q3756-04DL 20X
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BR-01-190-120225-SIMDL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

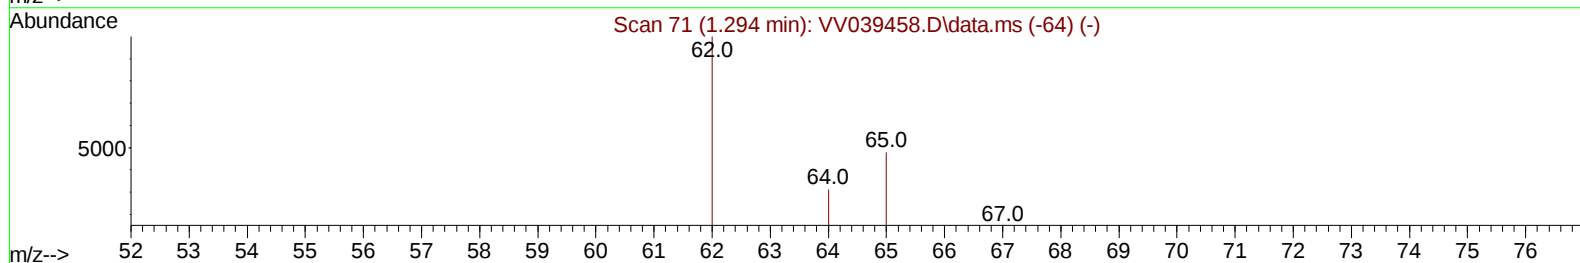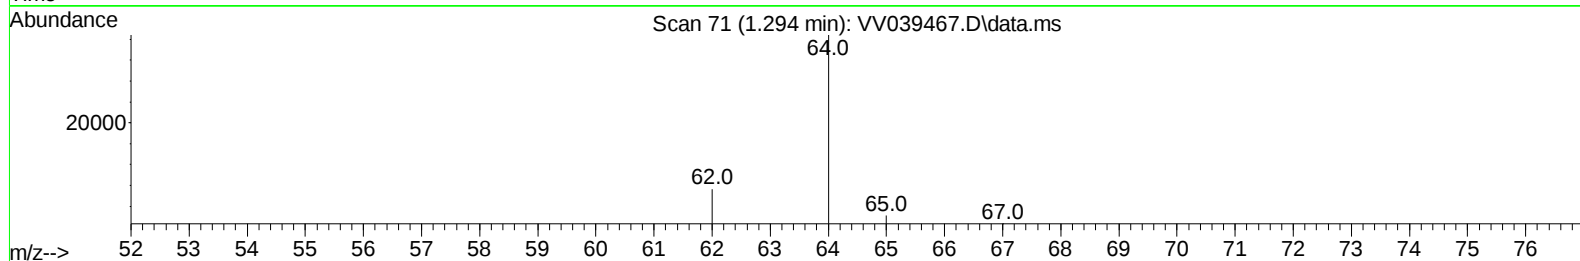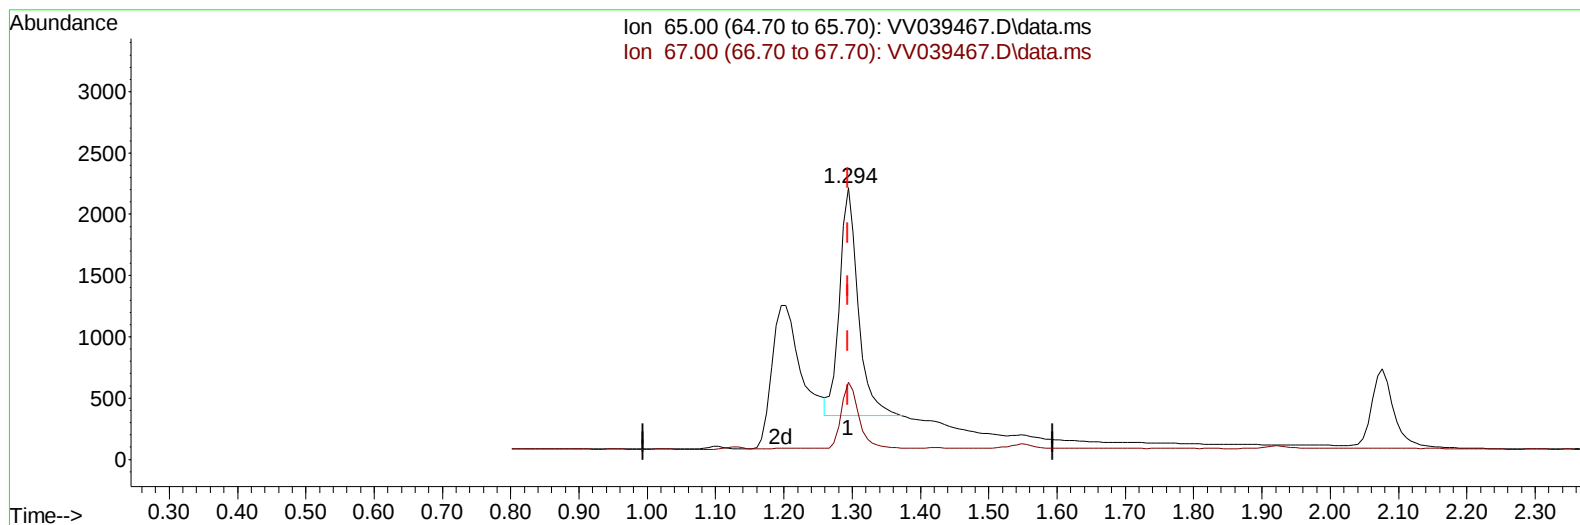

TIC: VV039467.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.62 ug/L m

response 3514

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	27.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
 Data File : VV039467.D
 Acq On : 04 Dec 2025 14:01
 Operator : SY/MD
 Sample : Q3756-04DL 20X
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BR-01-190-120225-SIMDL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
 Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:05 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5676	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5791	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	2925	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3514m	0.616	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	124.000%		
4) 1,2-Dichloroethane-d4	4.993	65	1757	0.465	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2049	0.419	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.253	98	3824	0.464	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1485	0.539	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	108.000%		
Target Compounds						
3) Vinyl chloride	1.294	62	12772	1.040	ug/L #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039467.D
Acq On : 04 Dec 2025 14:01
Operator : SY/MD
Sample : Q3756-04DL 20X
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BR-01-190-120225-SIMDL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

