




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039468.D
Acq On : 04 Dec 2025 15:03
Operator : SY/MD
Sample : Q3756-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-04B-26.5-120225-SIMRE

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

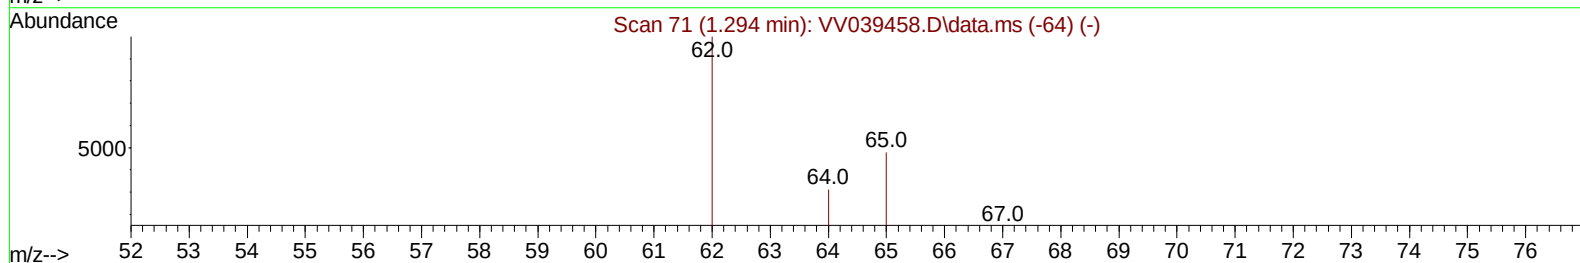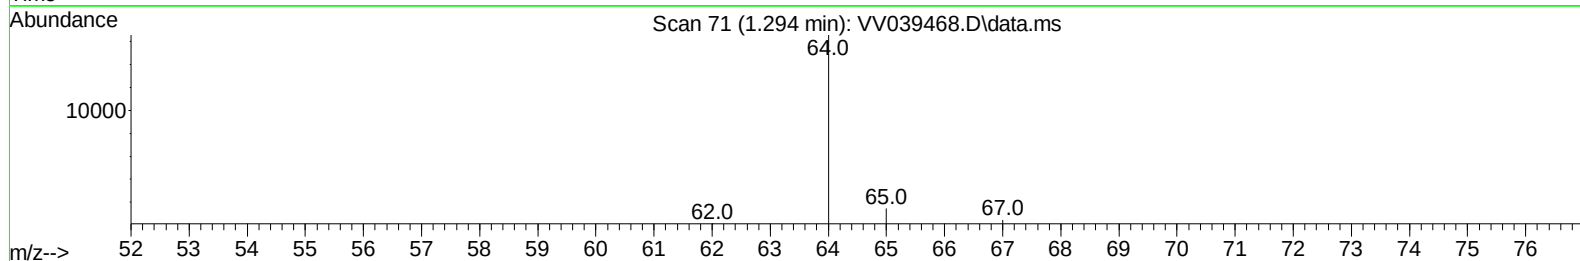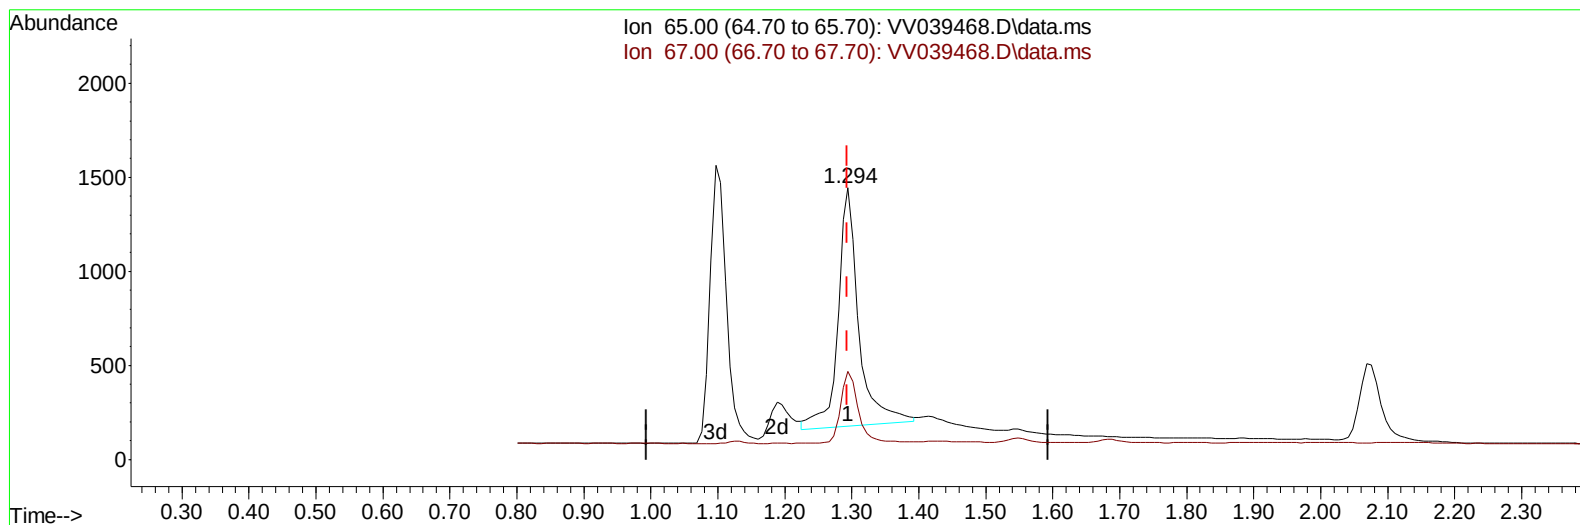

TIC: VV039468.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.71 ug/L

response 2733

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	26.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039468.D
Acq On : 04 Dec 2025 15:03
Operator : SY/MD
Sample : Q3756-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-04B-26.5-120225-SIMRE

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

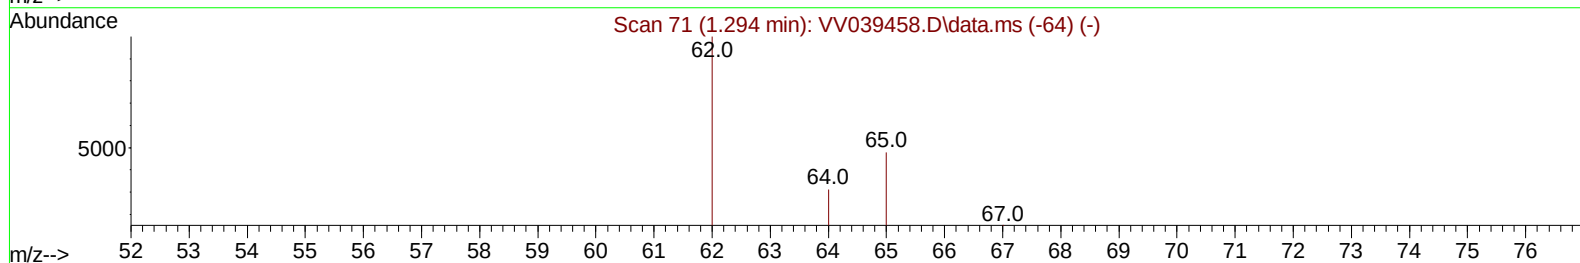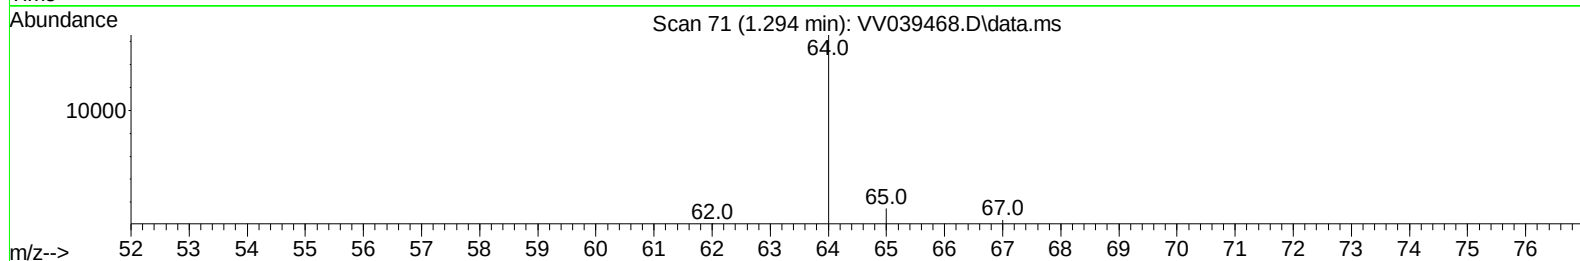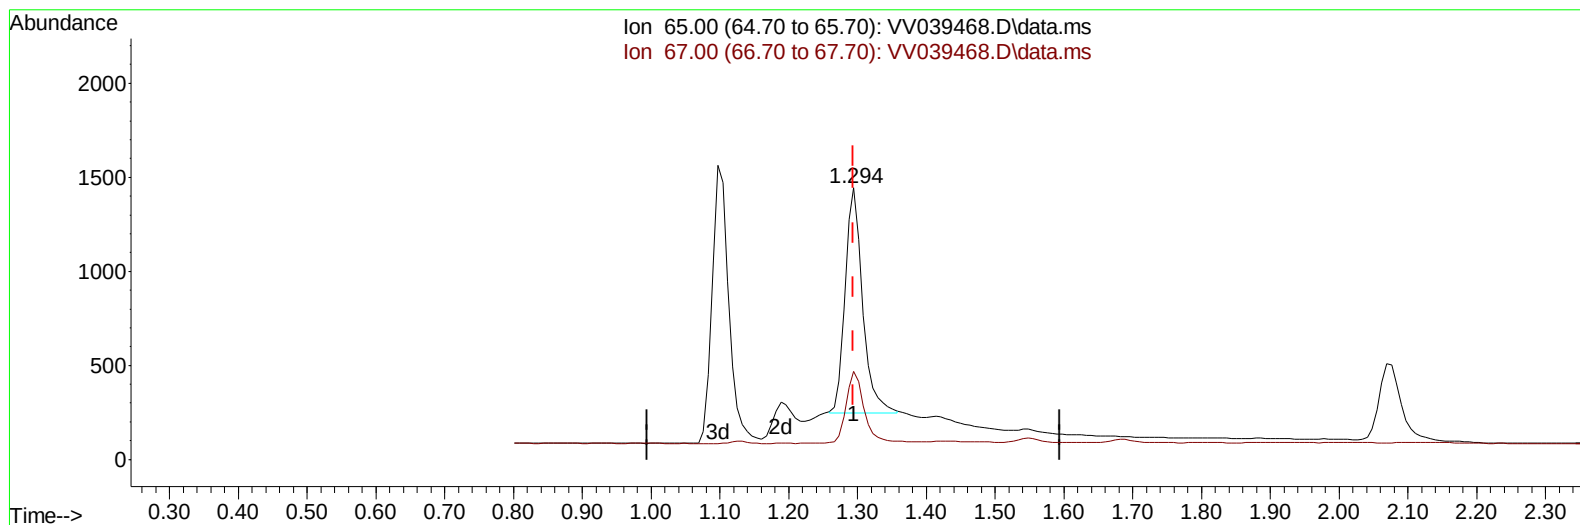

TIC: VV039468.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.294min (+ 0.000) 0.55 ug/L m

response 2107

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	34.46
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
 Data File : VV039468.D
 Acq On : 04 Dec 2025 15:03
 Operator : SY/MD
 Sample : Q3756-02
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 OW-04B-26.5-120225-SIMRE

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
 Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	3823	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	3906	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	2028	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	2107m	0.548	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	110.000%		
4) 1,2-Dichloroethane-d4	4.969	65	1499	0.589	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	118.000%		
7) 1,2-Dichloropropane-d6	5.995	67	1414	0.429	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	86.000%		
8) Toluene-d8	7.253	98	2475	0.445	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1480	0.797	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	160.000%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039468.D
Acq On : 04 Dec 2025 15:03
Operator : SY/MD
Sample : Q3756-02
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-04B-26.5-120225-SIMRE

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

