




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039470.D
Acq On : 04 Dec 2025 15:45
Operator : SY/MD
Sample : Q3756-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

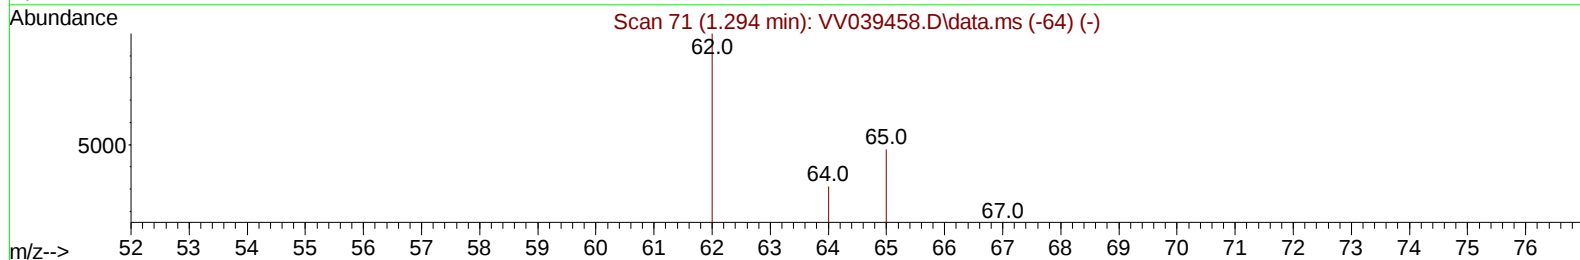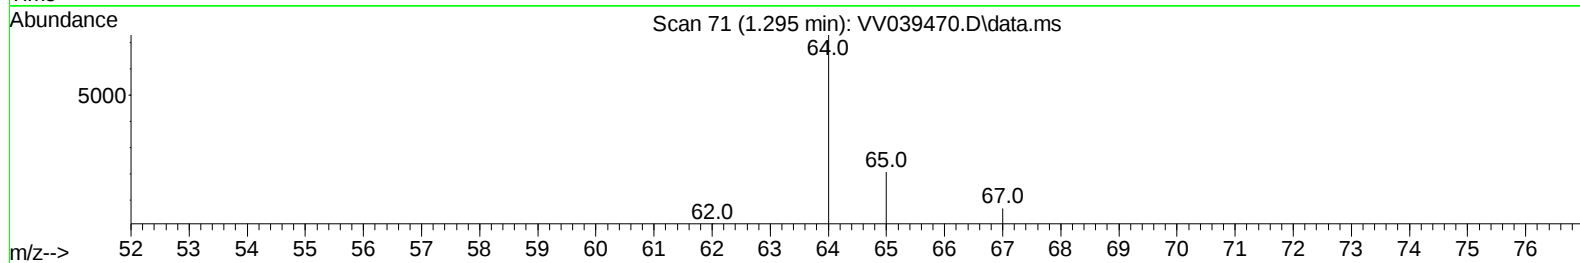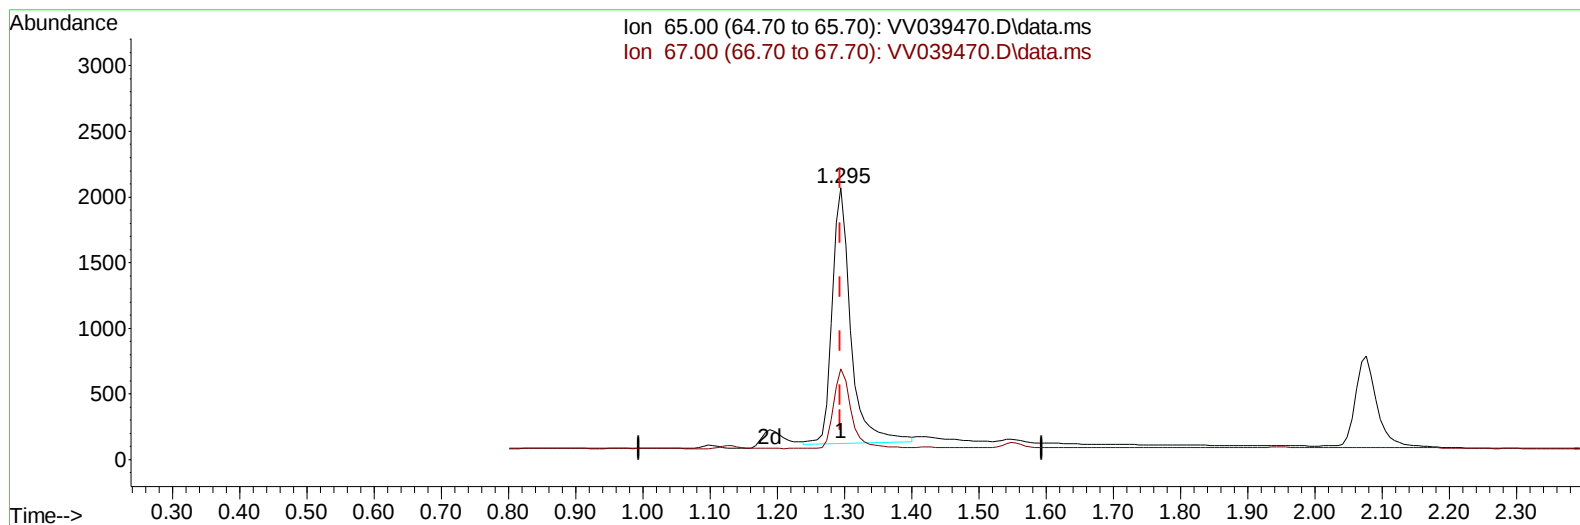

TIC: VV039470.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.71 ug/L

response 3753

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	30.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039470.D
Acq On : 04 Dec 2025 15:45
Operator : SY/MD
Sample : Q3756-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Dec 05 00:10:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

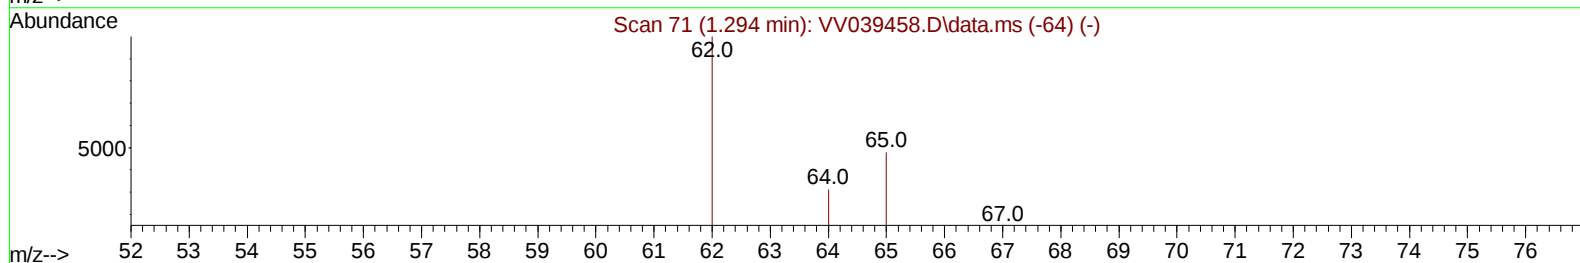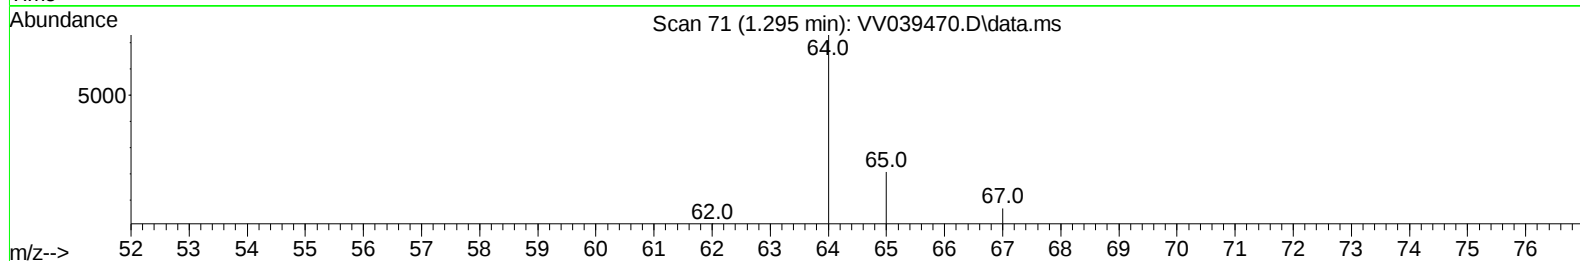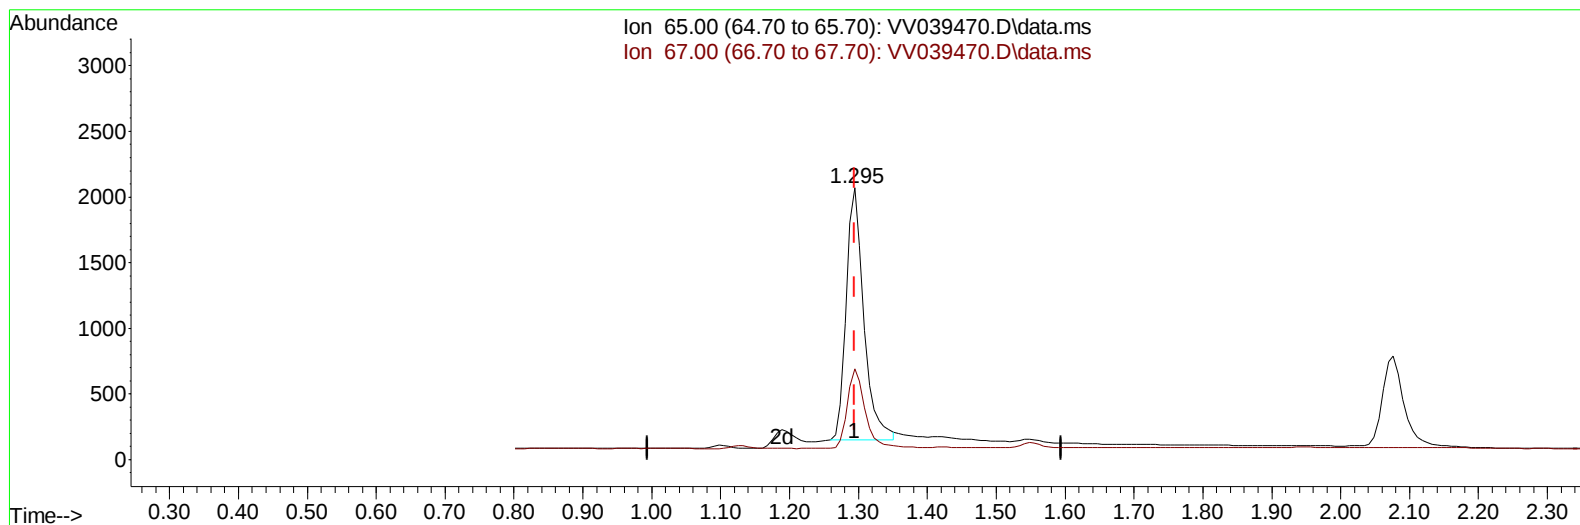

TIC: VV039470.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.65 ug/L m

response 3442

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	32.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
 Data File : VV039470.D
 Acq On : 04 Dec 2025 15:45
 Operator : SY/MD
 Sample : Q3756-12
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
 Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5258	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5346	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.198	152	2739	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.295	65	3442m	0.651	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	130.000%		
4) 1,2-Dichloroethane-d4	4.994	65	1878	0.536	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	108.000%		
7) 1,2-Dichloropropane-d6	5.996	67	2190	0.486	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	98.000%		
8) Toluene-d8	7.254	98	4157	0.546	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	110.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1600	0.629	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	126.000%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039470.D
Acq On : 04 Dec 2025 15:45
Operator : SY/MD
Sample : Q3756-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 12/10/2025
Supervised By : Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

