

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
 Data File : VV039469.D
 Acq On : 04 Dec 2025 15:24
 Operator : SY/MD
 Sample : VIBLK229
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK229

Manual Integrations
 APPROVED

Reviewed By : John Carlone 12/10/2025
 Supervised By : Mahesh Dadoda 12/10/2025

Quant Time: Dec 05 00:10:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	6254	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	6214	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	3212	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3477m	0.553	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	110.000%		
4) 1,2-Dichloroethane-d4	4.993	65	1933	0.464	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2215	0.422	ug/L	-0.02
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.253	98	4155	0.470	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1606	0.544	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	108.000%		

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120425\
Data File : VV039469.D
Acq On : 04 Dec 2025 15:24
Operator : SY/MD
Sample : VIBLK229
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

Quant Time: Dec 05 00:10:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : John Carlone 12/10/2025
Supervised By : Mahesh Dadoda 12/10/2025

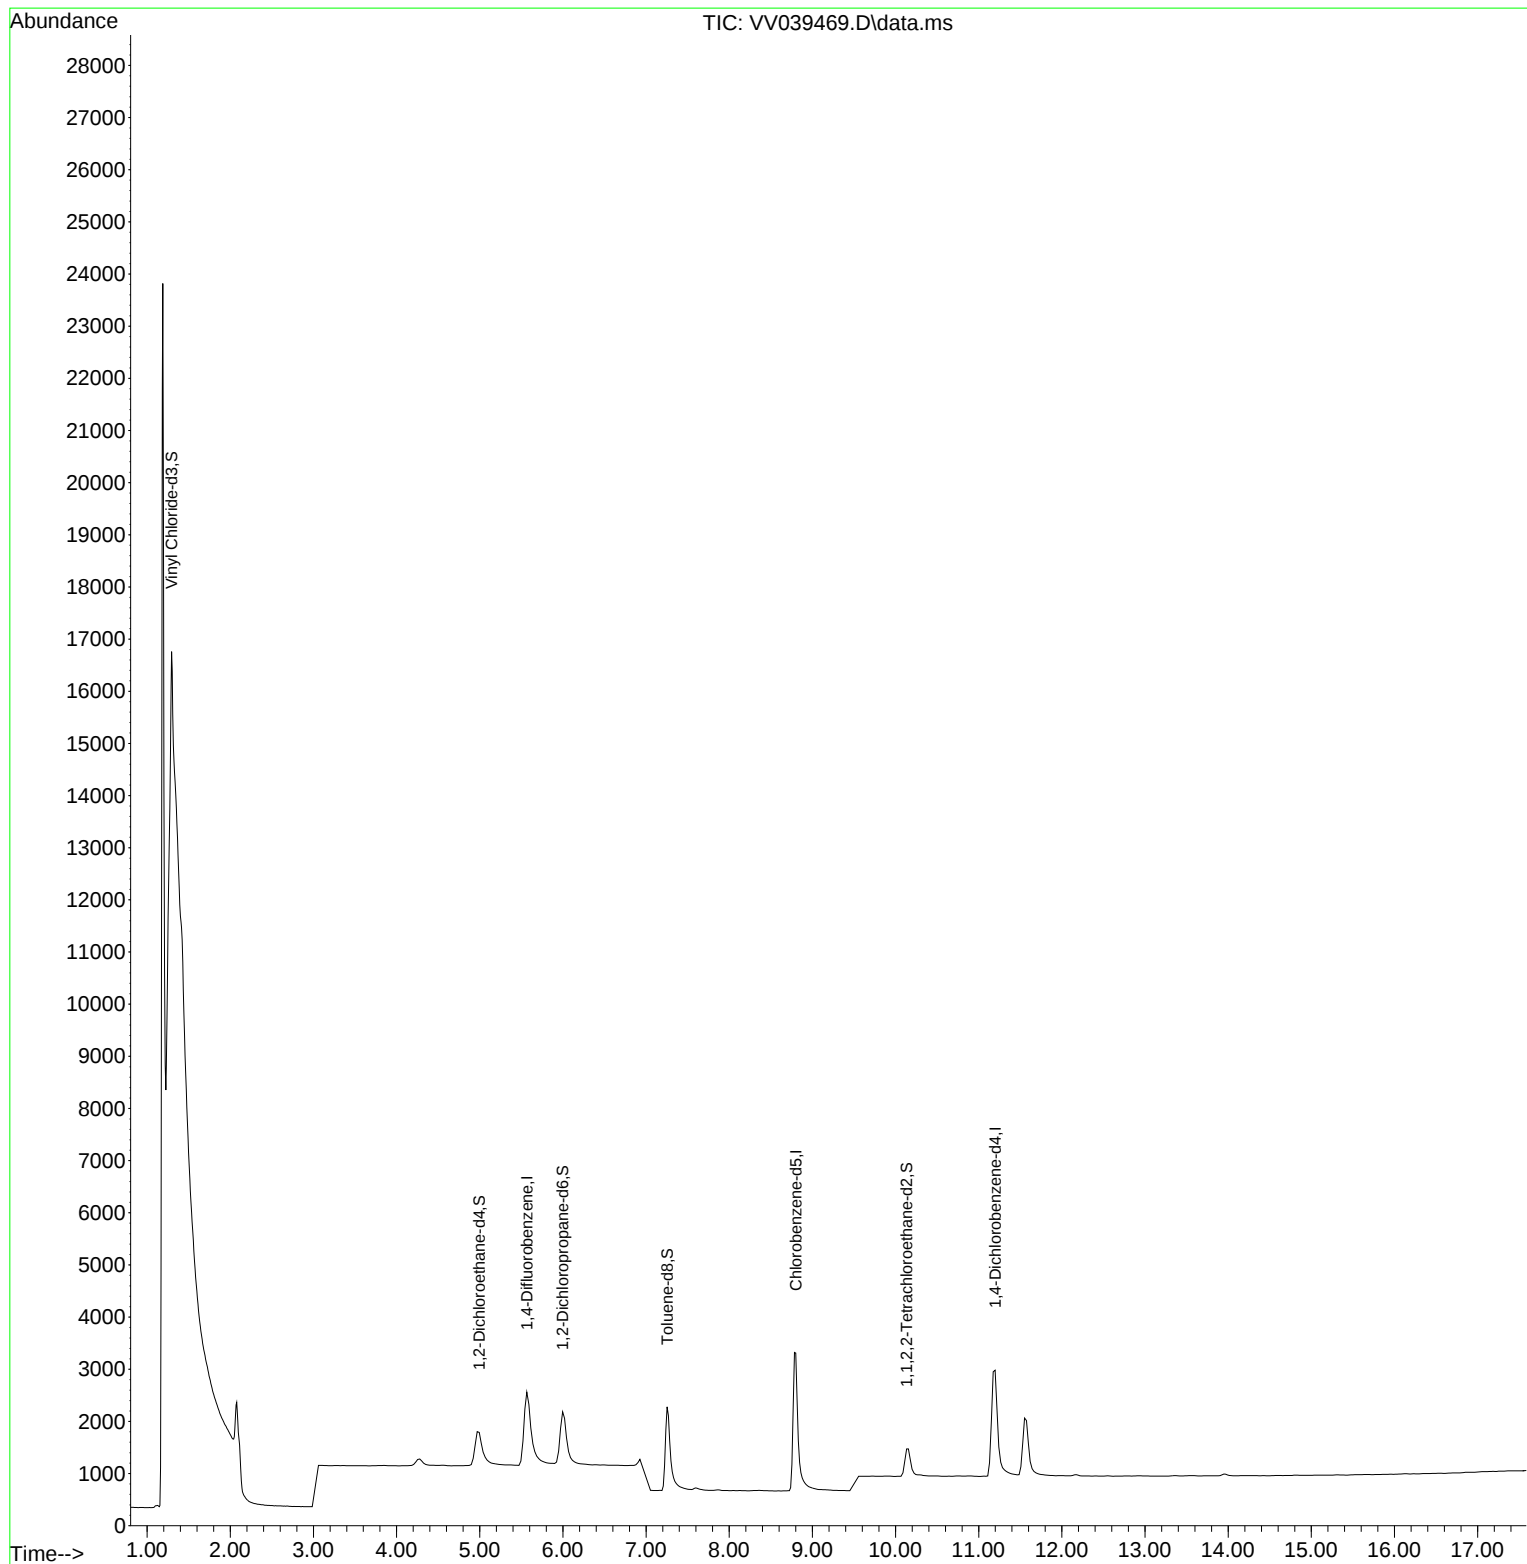

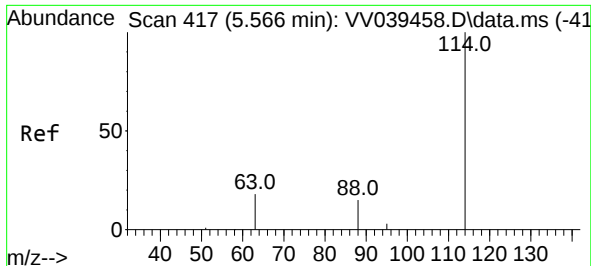





#1
1,4-Difluorobenzene
Concen: 0.500 ug/L
RT: 5.566 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24

Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

Tgt Ion:114 Resp: 6254
Ion Ratio Lower Upper
114 100
63 20.8 15.0 22.4
88 15.6 12.0 18.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

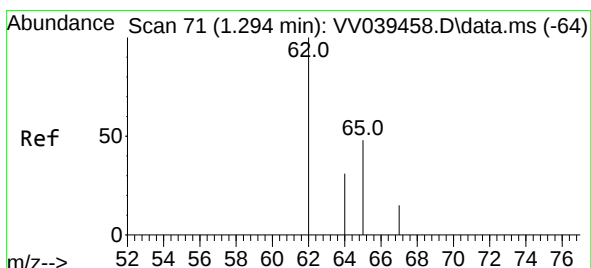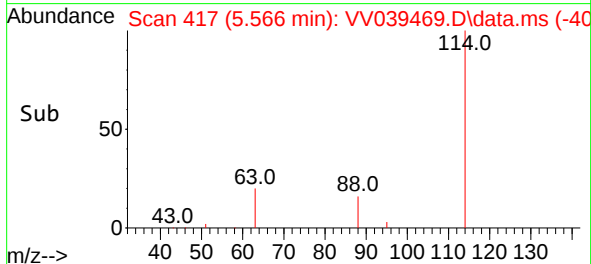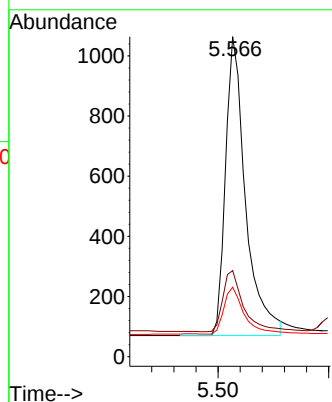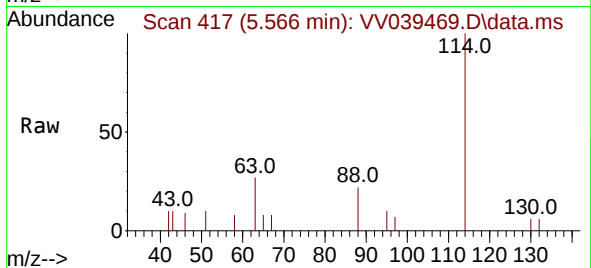

#2
Vinyl Chloride-d3
Concen: 0.553 ug/L m
RT: 1.294 min Scan# 71
Delta R.T. 0.000 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24

Tgt Ion: 65 Resp: 3477
Ion Ratio Lower Upper
65 100
67 31.1 22.3 41.5

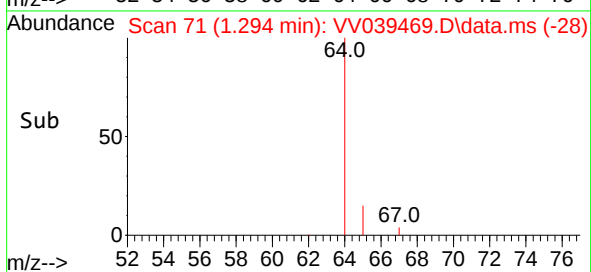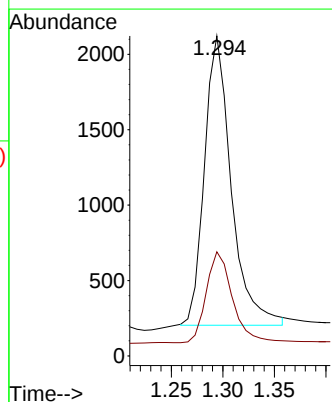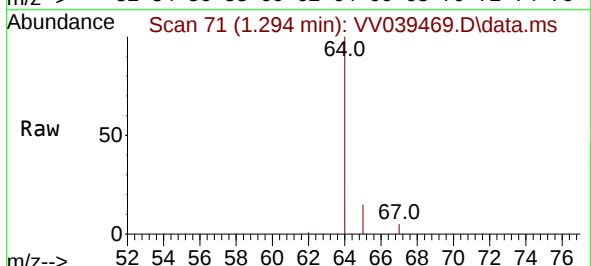

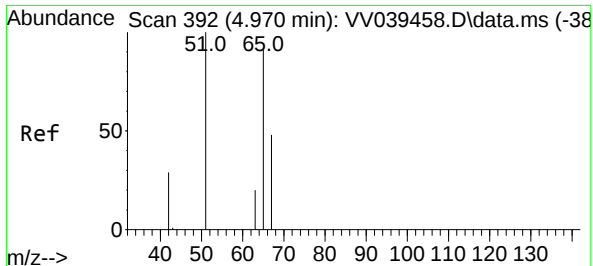





#4
1,2-Dichloroethane-d4
Concen: 0.464 ug/L
RT: 4.993 min Scan# 392
Delta R.T. 0.024 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24

Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

Tgt Ion: 65 Resp: 193
Ion Ratio Lower Upper
65 100
67 51.8 32.5 60.3
51 38.2 121.4 225.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

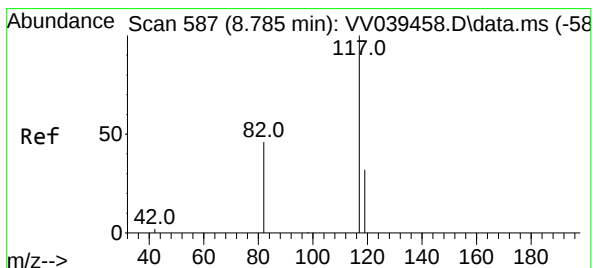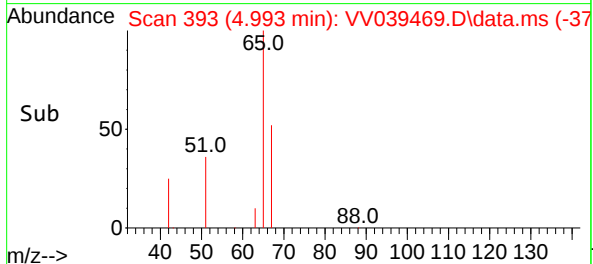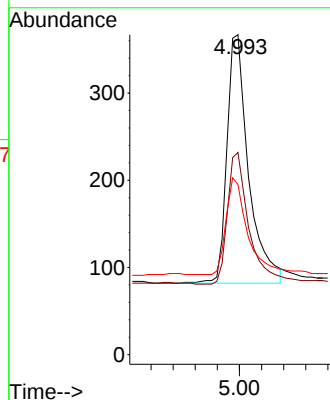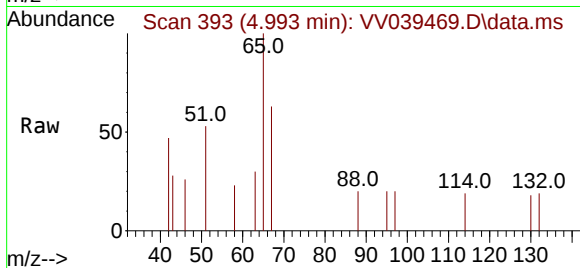

#5
Chlorobenzene-d5
Concen: 0.500 ug/L
RT: 8.800 min Scan# 588
Delta R.T. 0.015 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24


Tgt Ion:117 Resp: 6214
Ion Ratio Lower Upper
117 100
82 48.2 39.4 59.2
119 32.4 26.2 39.2

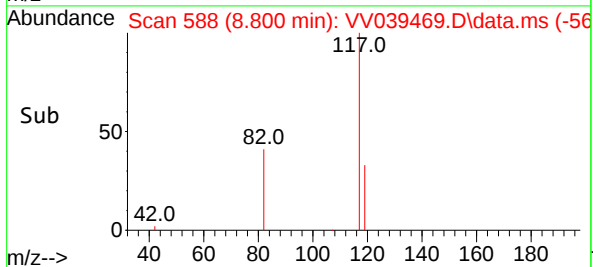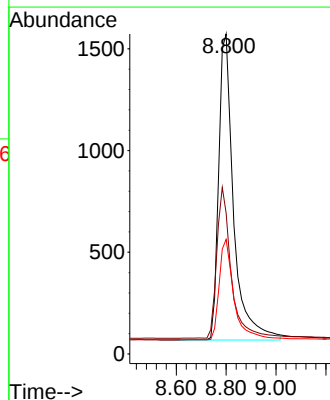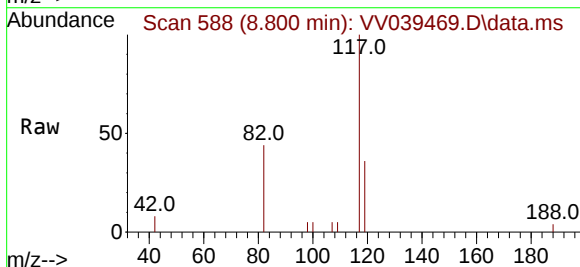

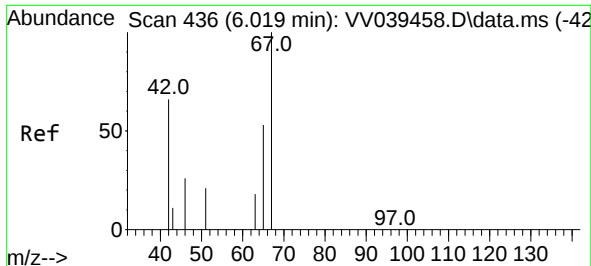

#7
1,2-Dichloropropane-d6
Concen: 0.422 ug/L
RT: 5.995 min Scan# 41
Delta R.T. -0.024 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24




Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

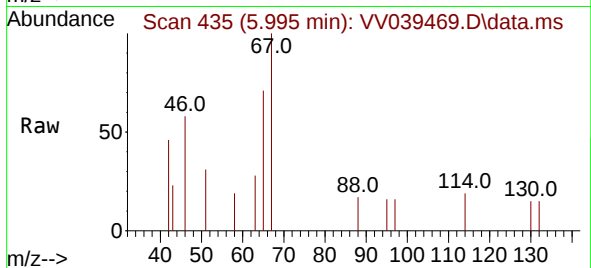

Tgt Ion:	67	Resp:	221
Ion	Ratio	Lower	Upper
67	100		
65	63.2	37.9	56.9
46	44.5	27.4	41.0
42	31.7	51.2	76.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

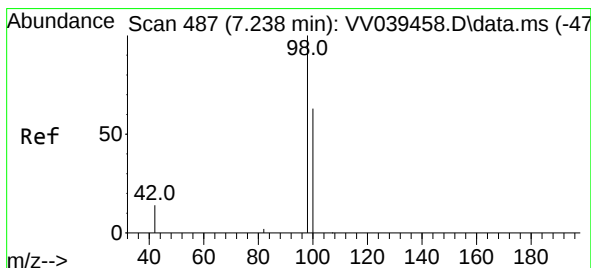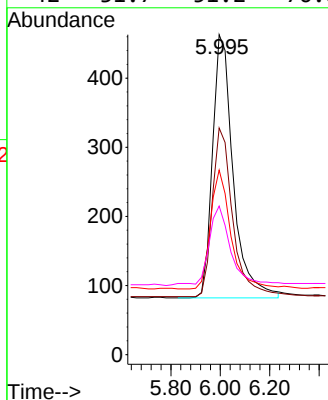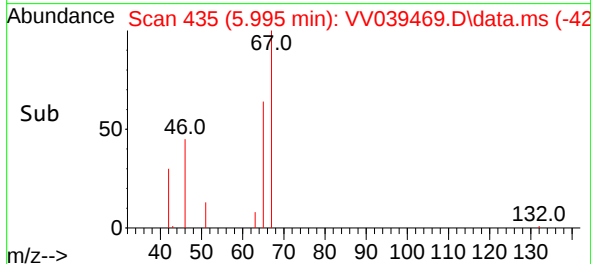

#8
Toluene-d8
Concen: 0.470 ug/L
RT: 7.253 min Scan# 488
Delta R.T. 0.015 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24


Tgt Ion:	98	Resp:	4155
Ion	Ratio	Lower	Upper
98	100		
100	61.0	44.5	82.7
42	10.2	10.1	18.7

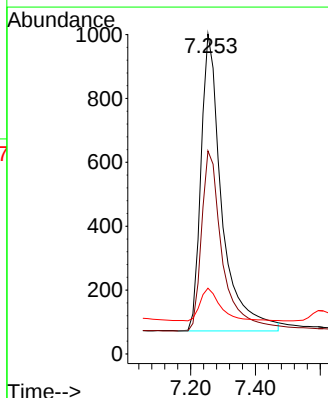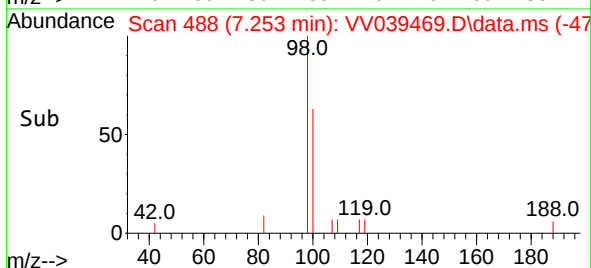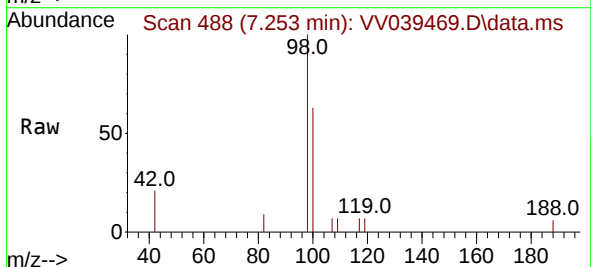

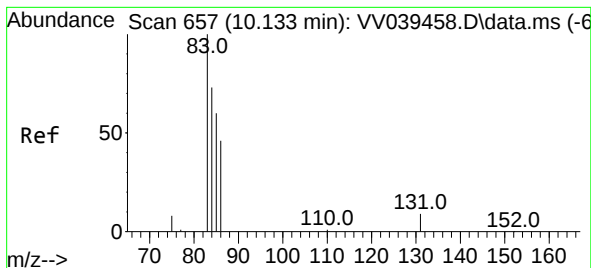

#10
1,1,2,2-Tetrachloroethane-d2
Concen: 0.544 ug/L
RT: 10.133 min Scan# 610
Delta R.T. -0.000 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24




Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

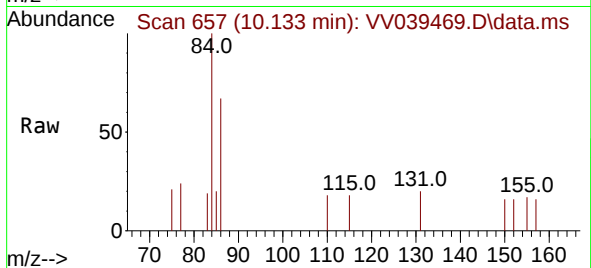


Tgt Ion: 84 Resp: 1600
Ion Ratio Lower Upper
84 100
86 62.4 44.4 82.5

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

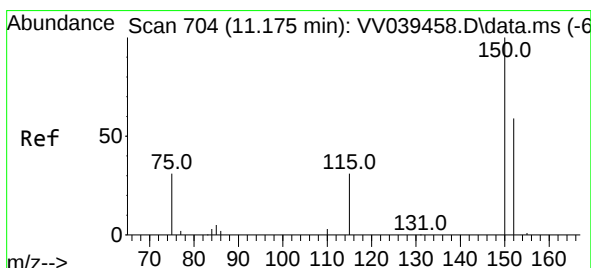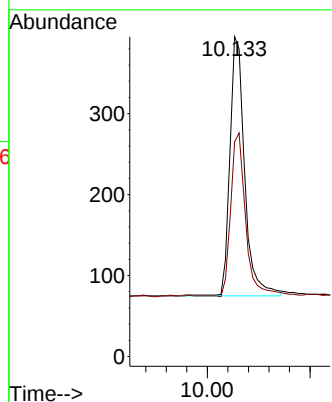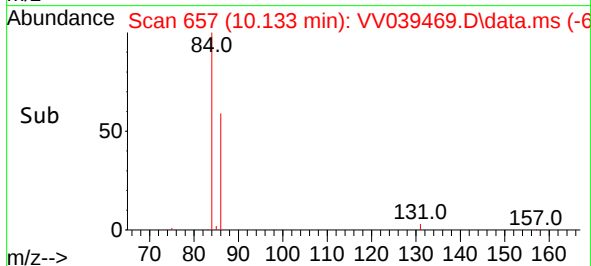

#12
1,4-Dichlorobenzene-d4
Concen: 0.500 ug/L
RT: 11.197 min Scan# 705
Delta R.T. 0.022 min
Lab File: VV039469.D
Acq: 04 Dec 2025 15:24

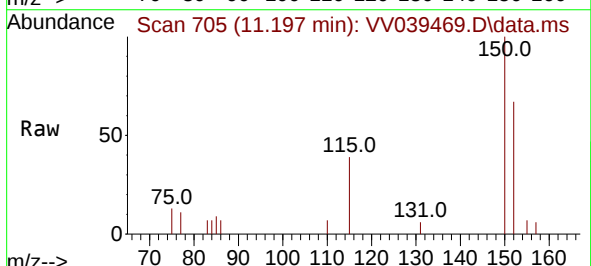

Tgt Ion:152 Resp: 3212
Ion Ratio Lower Upper
152 100
115 55.9 0.0 101.6
150 158.8 0.0 396.2

