

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120518\
 Data File : VV008845.D
 Acq On : 05 Dec 2018 17:26
 Operator : SY/MD
 Sample : J6155-16
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4150

Quant Time: Dec 06 07:18:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 06 04:51:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	112176	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	101058	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	45489	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	28742	4.81	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.20%
7) Chloroethane-d5	1.59	69	21308	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	2.14	63	41453	3.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.80%
20) 2-Butanone-d5	3.96	46	70611	47.79	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.58%
24) Chloroform-d	4.41	84	63284	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.09	65	31407	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
32) Benzene-d6	5.10	84	130929	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.12	67	37950	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.36	98	116087	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloropropene-	7.67	79	11801	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	8.14	63	49278	44.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	24969	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	42637	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Qvalue
13) Acetone	2.21	43	5526	6.719 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120518\
Data File : VV008845.D
Acq On : 05 Dec 2018 17:26
Operator : SY/MD
Sample : J6155-16
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4150

Quant Time: Dec 06 07:18:07 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 06 04:51:41 2018
Response via : Initial Calibration

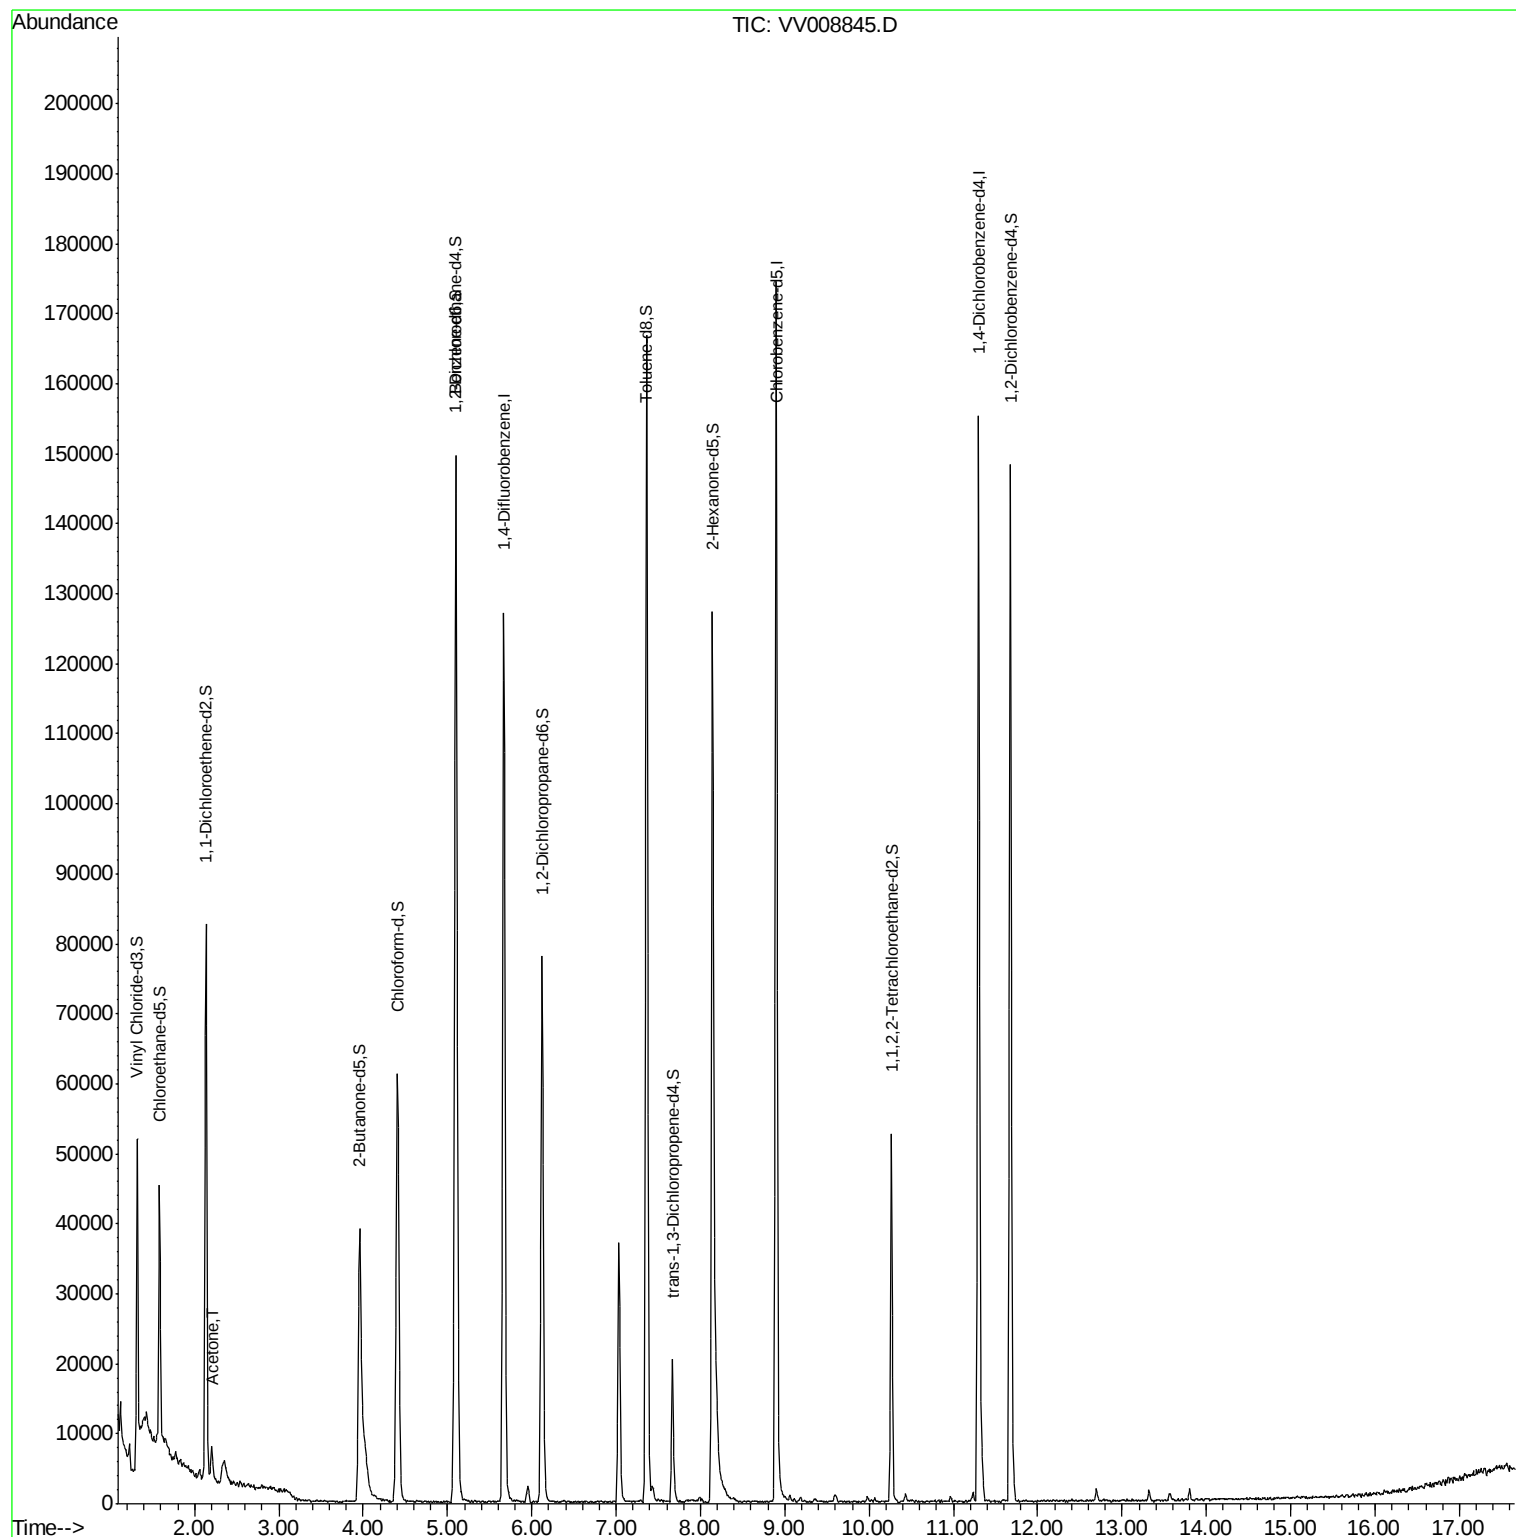

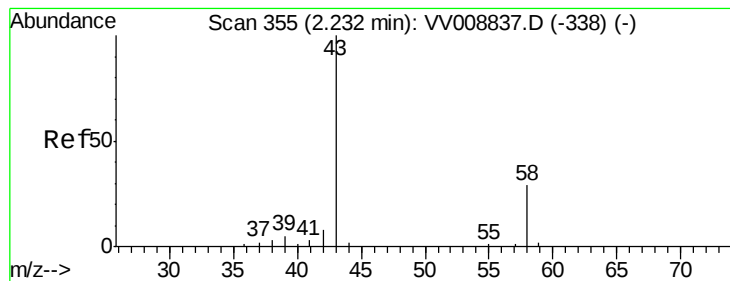

#13
 Acetone
 Concen: 6.719 ug/L
 RT: 2.21 min Scan# 347
 Delta R.T. -0.03 min
 Lab File: VV008845.D
 Acq: 05 Dec 2018 17:26

Instrument :
 MSVOA_V
 ClientSampleId :
 A4150

Tgt Ion: 43 Resp: 5526
 Ion Ratio Lower Upper
 43 100
 58 24.4 0.0 52.4

