

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120518\
 Data File : VV008846.D
 Acq On : 05 Dec 2018 17:51
 Operator : SY/MD
 Sample : J6155-17
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4152

Quant Time: Dec 06 07:21:20 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 06 04:51:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	109897	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	101749	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	45366	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	26899	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.59	69	20344	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.00%
11) 1,1-Dichloroethene-d2	2.14	63	40830	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	3.96	46	74595	51.54	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.08%
24) Chloroform-d	4.41	84	61921	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.09	65	31858	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.10	84	127300	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.12	67	38255	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.36	98	113132	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.67	79	12565	4.26	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.20%
46) 2-Hexanone-d5	8.14	63	51034	45.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.86%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	25327	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	41397	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Qvalue
13) Acetone	2.21	43	4953	6.147 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120518\
Data File : VV008846.D
Acq On : 05 Dec 2018 17:51
Operator : SY/MD
Sample : J6155-17
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4152

Quant Time: Dec 06 07:21:20 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 06 04:51:41 2018
Response via : Initial Calibration

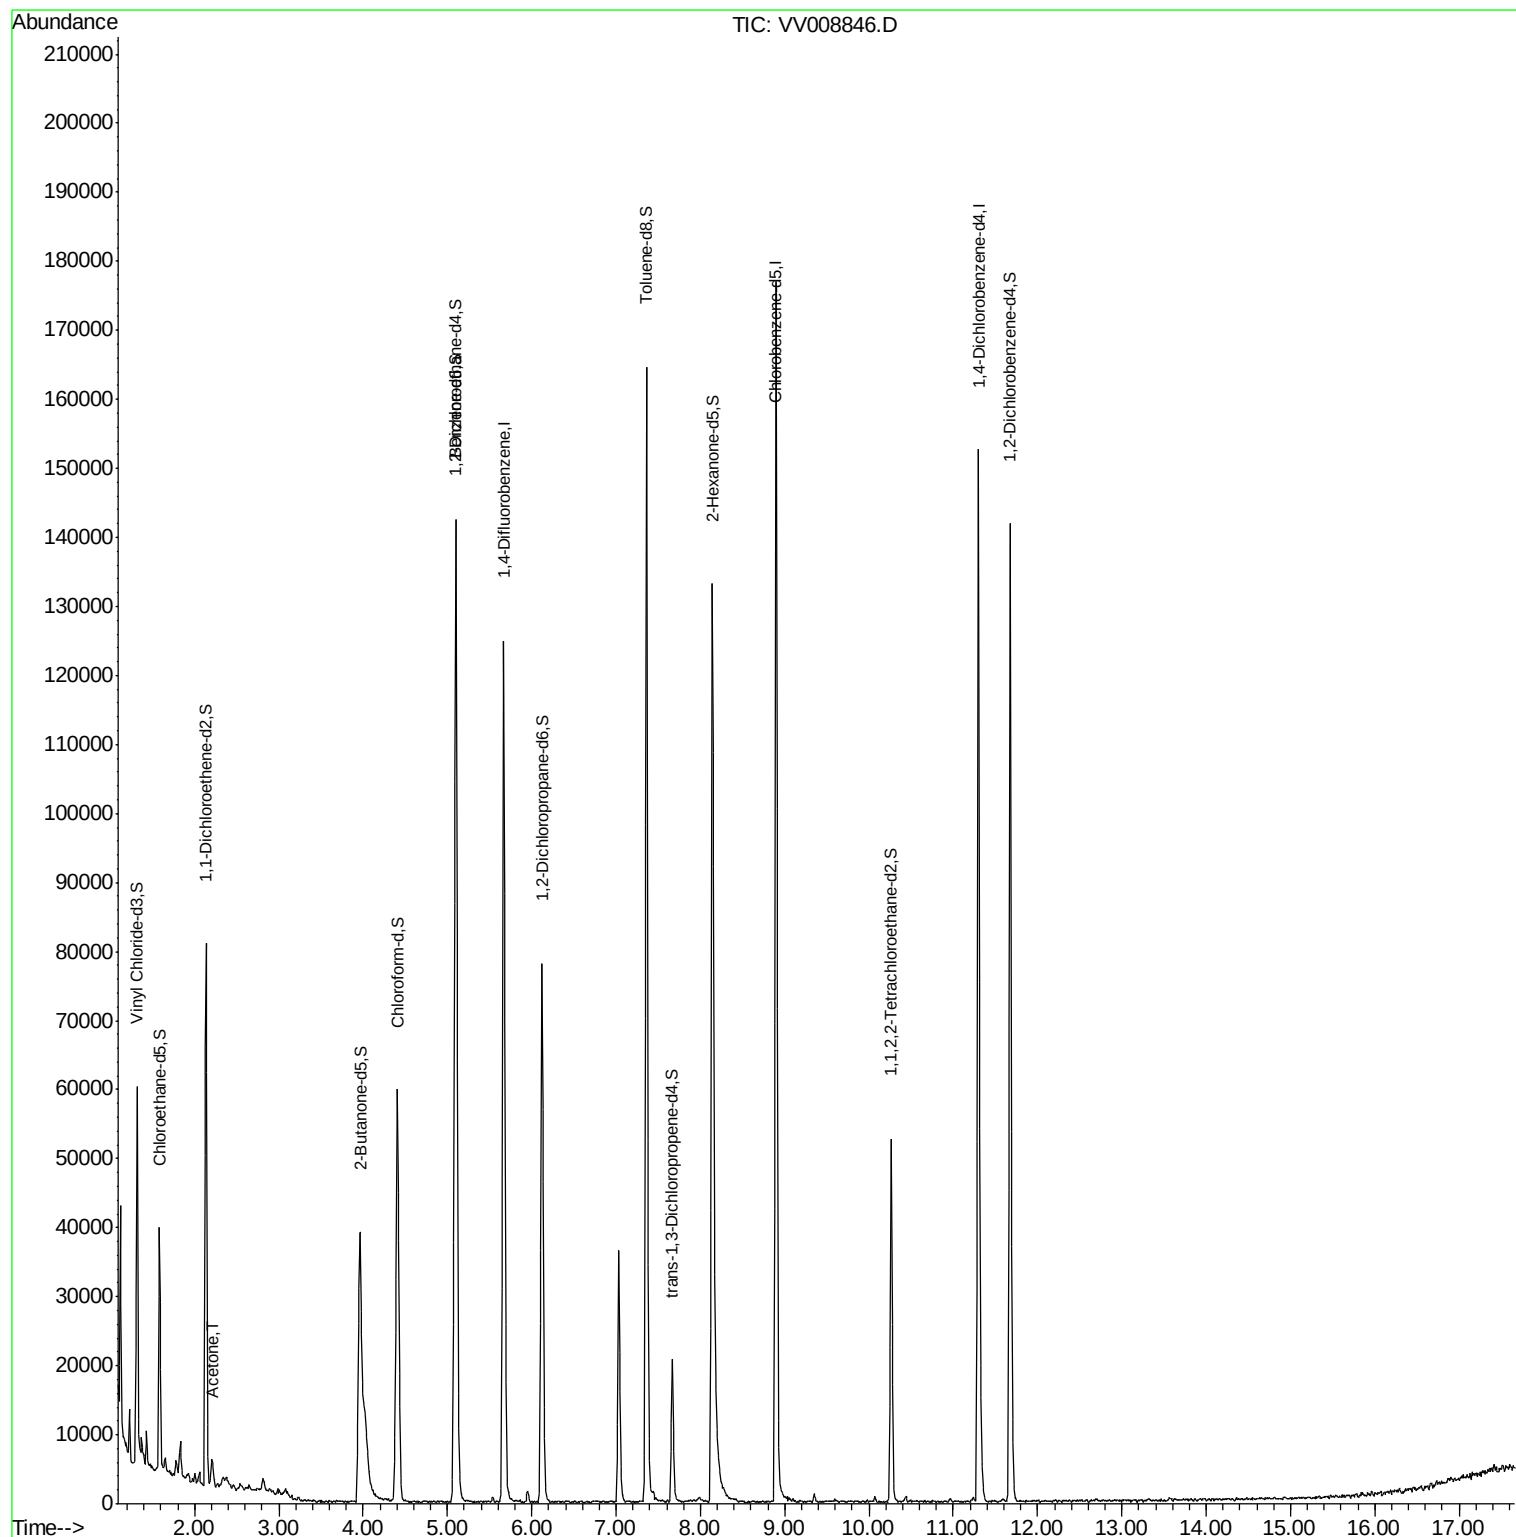

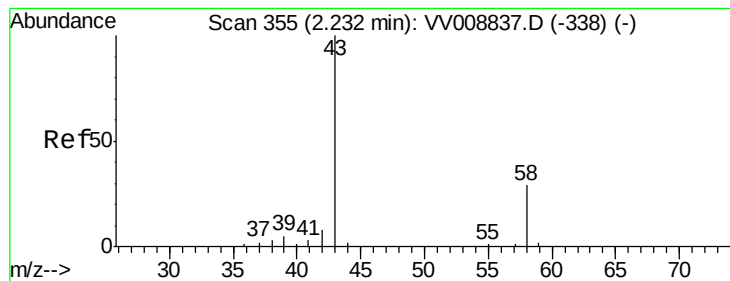

#13
 Acetone
 Concen: 6.147 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. -0.02 min
 Lab File: VV008846.D
 Acq: 05 Dec 2018 17:51

Instrument :
 MSVOA_V
 ClientSampleId :
 A4152

Tgt Ion: 43 Resp: 4953
 Ion Ratio Lower Upper
 43 100
 58 26.9 0.0 52.4

