

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120518\
 Data File : VV008848.D
 Acq On : 05 Dec 2018 18:42
 Operator : SY/MD
 Sample : J6155-19
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4168

Quant Time: Dec 06 07:32:58 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 06 04:51:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	105231	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	98792	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	44078	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27288	4.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.20%
7) Chloroethane-d5	1.59	69	20874	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.80%
11) 1,1-Dichloroethene-d2	2.14	63	40749	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.96	46	73948	53.35	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.70%
24) Chloroform-d	4.41	84	61326	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.09	65	31751	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
32) Benzene-d6	5.10	84	127253	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.12	67	37328	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	7.36	98	113014	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.67	79	13043	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
46) 2-Hexanone-d5	8.14	63	52268	47.92	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.84%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	25254	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	42017	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Qvalue
13) Acetone	2.21	43	4700	6.092 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120518\
Data File : VV008848.D
Acq On : 05 Dec 2018 18:42
Operator : SY/MD
Sample : J6155-19
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4168

Quant Time: Dec 06 07:32:58 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 06 04:51:41 2018
Response via : Initial Calibration

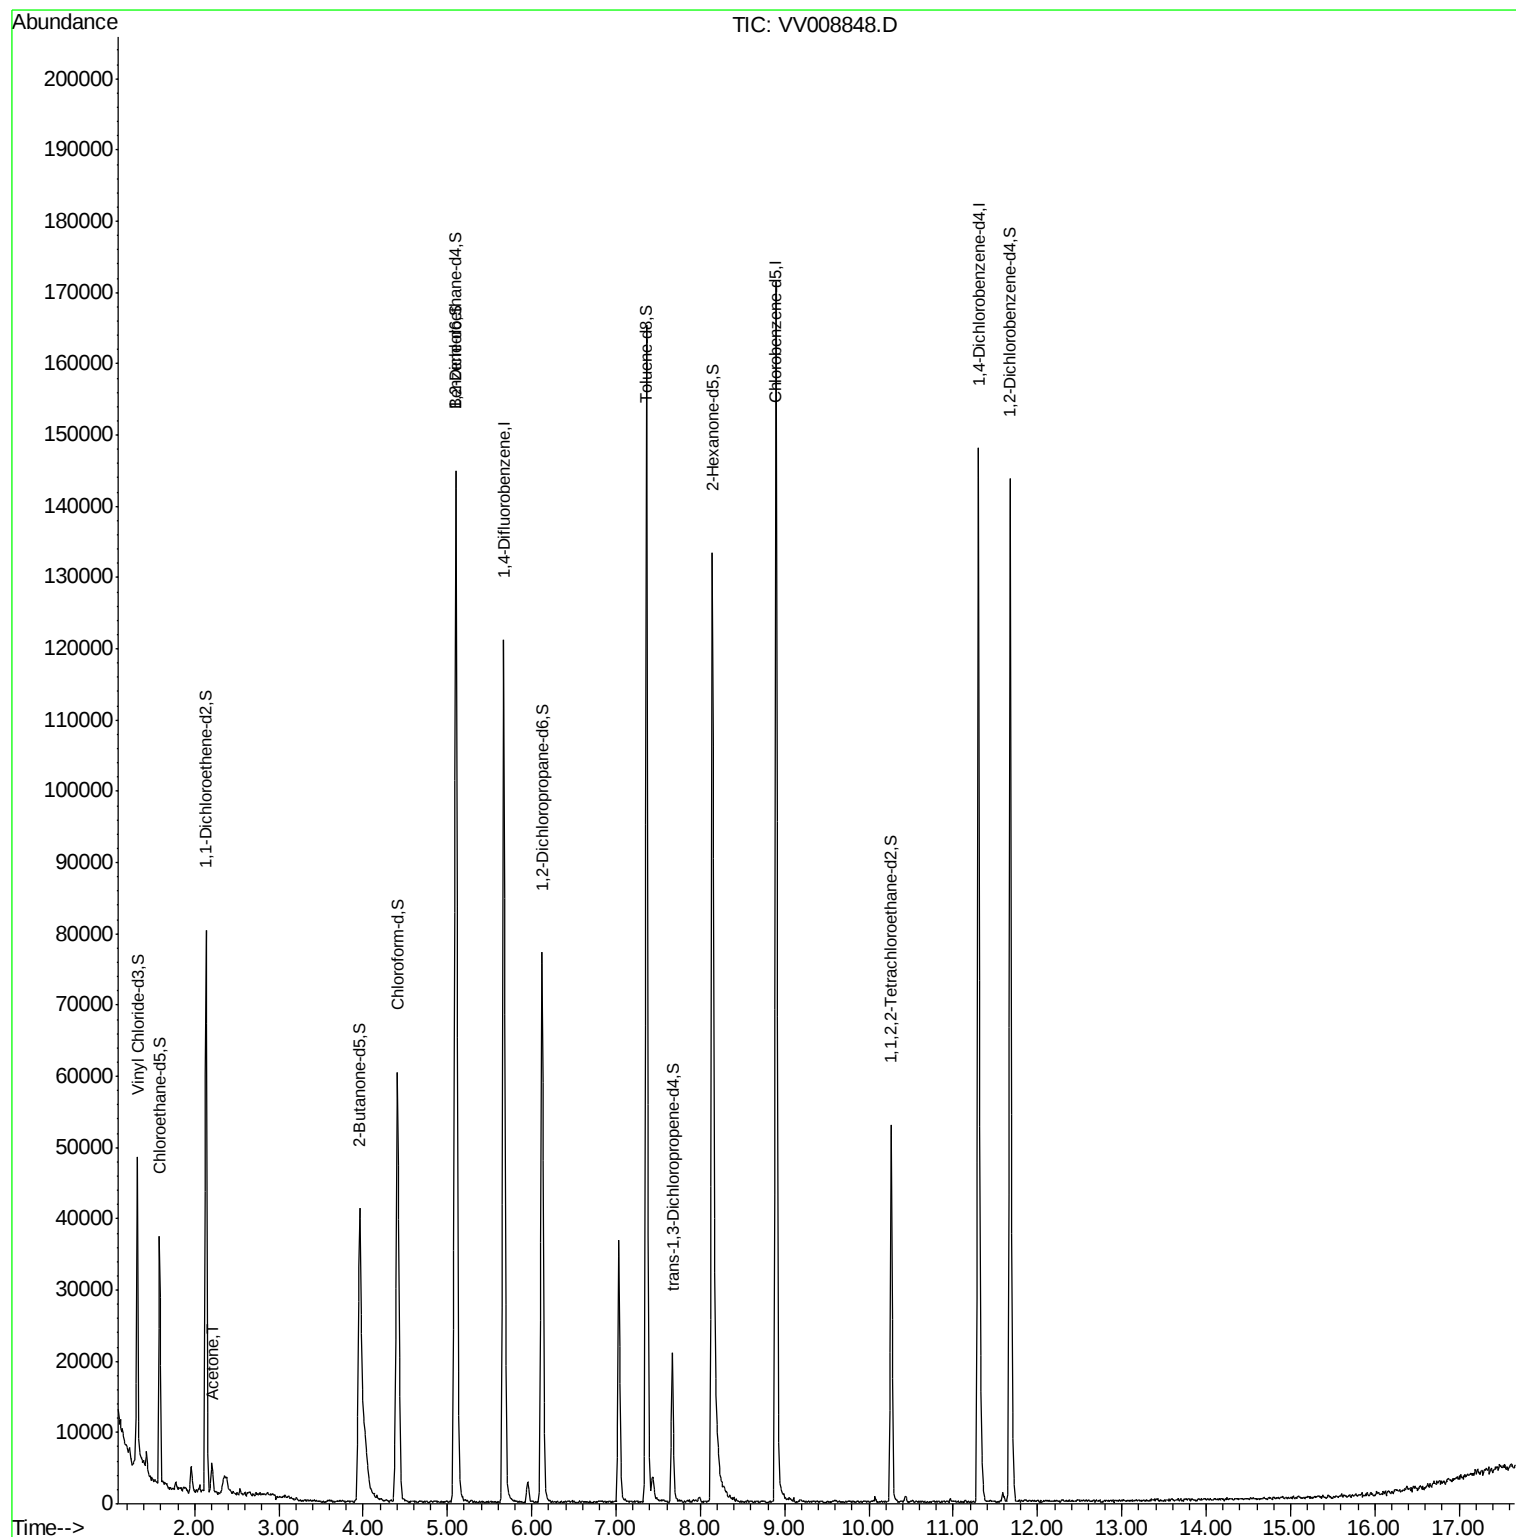

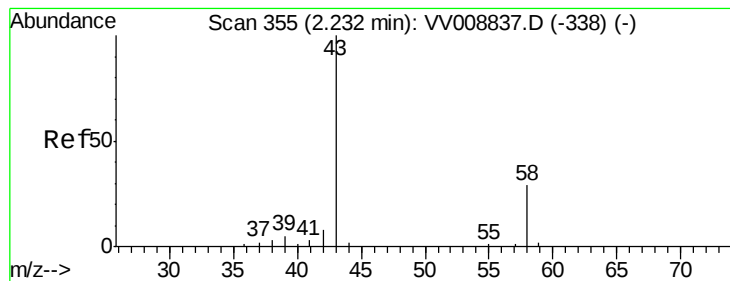

#13

Acetone

Concen: 6.092 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.02 min

Lab File: VV008848.D

Acq: 05 Dec 2018 18:42

Instrument :
MSVOA_V
ClientSampleId :
A4168

Tgt Ion: 43 Resp: 4700

Ion Ratio Lower Upper

43 100

58 27.8 0.0 52.4

