


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120518\
Data File : VV008834.D
Acq On : 05 Dec 2018 09:25
Operator : SY/MD
Sample : BFB55
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB55

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Dec 06 04:51:41 2018

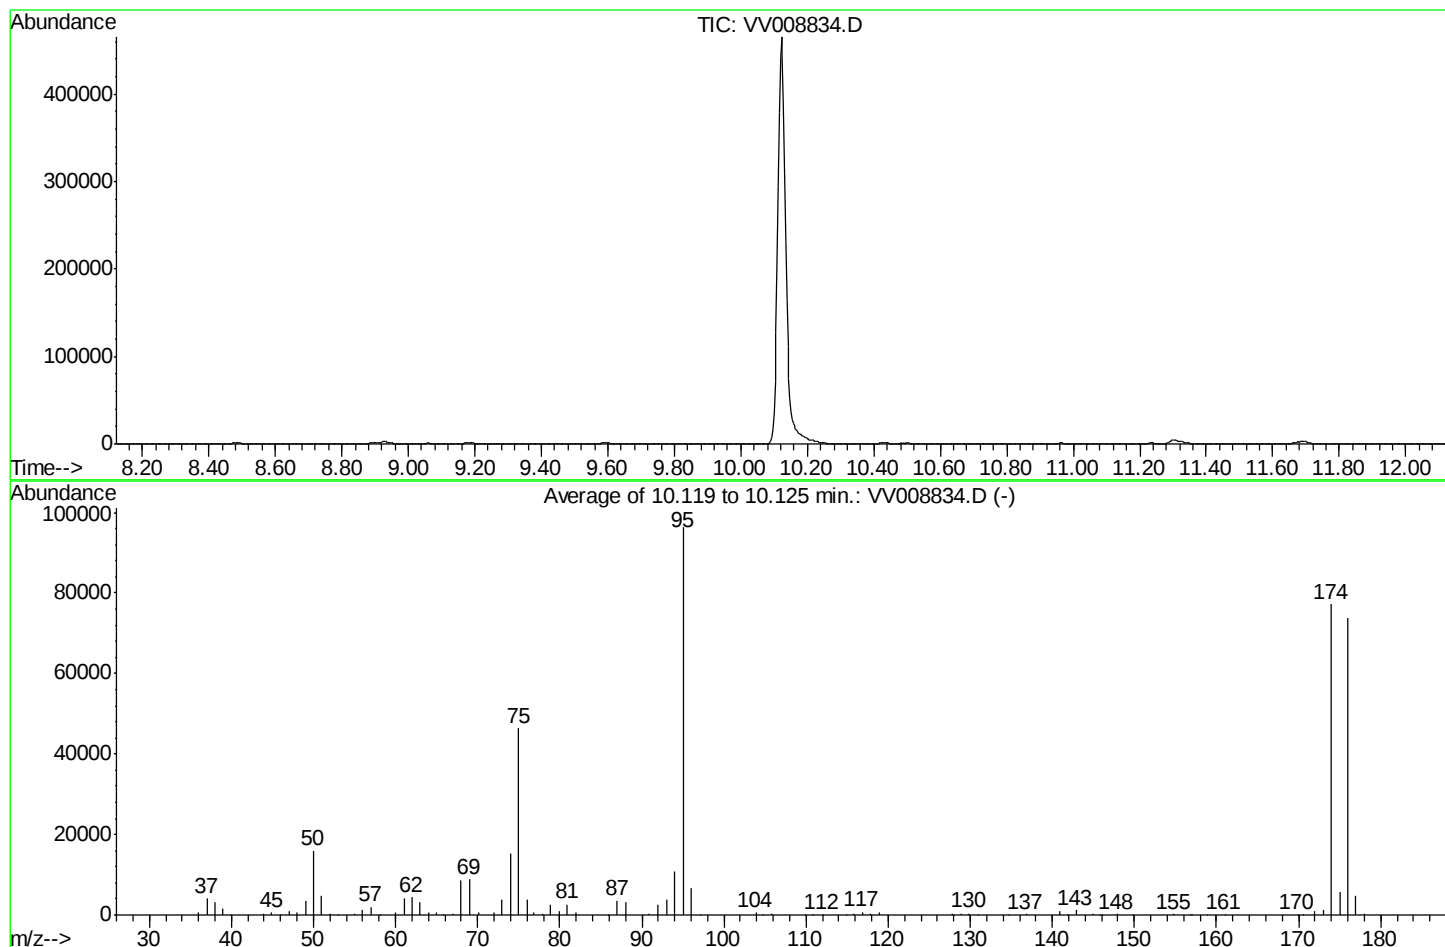

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	15988	PASS
75	95	30	80	48.1	46296	PASS
95	95	100	100	100.0	96306	PASS
96	95	5	9	6.8	6563	PASS
173	174	0.00	2	1.5	1163	PASS
174	95	50	120	80.1	77130	PASS
175	174	5	9	7.4	5733	PASS
176	174	95	101	95.8	73888	PASS
177	176	5	9	6.4	4762	PASS

m/z	Abundance
36.00	655.0
37.00	4063.0
38.00	3400.0
39.00	1431.0
39.90	222.0
43.90	705.0
44.90	590.0
45.90	169.0
47.00	963.0
48.00	703.0
49.00	3375.0
50.00	15886.0
51.00	4721.0
52.00	183.0
52.90	123.0
55.00	252.0
56.00	1415.0
57.00	1965.0
58.10	101.0
60.10	700.0
61.00	4111.0
62.00	4379.0
63.00	3195.0
64.00	483.0
64.90	566.0
67.10	204.0
68.00	8607.0
69.00	8998.0
70.00	659.0
72.00	418.0
73.00	3856.0
74.00	15203.0
75.00	45696.0
76.00	3940.0
76.90	535.0
77.90	329.0
78.90	2522.0
79.90	862.0
80.90	2627.0
82.00	607.0
85.90	120.0
87.00	3445.0
88.00	3174.0
90.80	301.0
92.00	2510.0
93.00	3936.0
94.00	10472.0
95.00	94856.0
96.00	6479.0
97.00	182.0
103.90	511.0
104.80	141.0
105.80	415.0
110.80	124.0
114.90	175.0
115.80	325.0
116.90	787.0
117.80	281.0
119.00	450.0
127.80	203.0
128.90	213.0
129.90	331.0
130.90	179.0
134.70	195.0
136.70	153.0
140.90	974.0
142.90	1158.0
144.90	211.0
145.80	106.0
147.80	172.0
149.80	135.0
154.80	229.0
156.80	103.0
158.80	118.0
161.00	123.0
171.90	963.0
173.10	1177.0
174.00	74584.0
175.00	5687.0
176.00	71360.0
177.00	4786.0
178.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	784.0
37.00	4183.0
38.00	3391.0
39.00	1597.0
39.90	227.0
44.00	674.0
44.90	621.0
45.90	163.0
47.00	1116.0
48.00	697.0
49.00	3591.0
50.00	16584.0
51.00	4983.0
52.00	194.0
55.00	276.0
56.00	1435.0
57.00	2074.0
60.00	748.0
61.00	4423.0
62.00	4632.0
63.00	3412.0
64.00	508.0
65.00	663.0
65.80	117.0
67.10	237.0
68.00	8897.0
69.00	9116.0
70.10	654.0
71.90	535.0
73.00	4081.0
74.00	15725.0
75.00	47864.0
76.00	3998.0
76.90	516.0
77.90	351.0
78.90	2614.0
80.00	913.0
80.90	2720.0
81.90	668.0
85.90	132.0
87.00	3617.0
88.00	3457.0
90.80	285.0
92.00	2506.0
93.00	3918.0
94.00	11066.0
95.00	99512.0
96.00	6811.0
97.10	169.0
103.90	537.0
104.80	135.0
105.90	425.0
110.80	109.0
112.00	109.0
114.90	160.0
115.90	345.0
116.90	779.0
117.80	300.0
118.90	503.0
127.80	227.0
128.80	224.0
129.90	346.0
130.90	185.0
134.70	166.0
136.80	214.0
140.90	1037.0
141.80	100.0
142.90	1214.0
144.90	205.0
146.00	138.0
147.80	181.0
149.70	166.0
154.80	273.0
158.80	157.0
161.00	144.0
171.90	1044.0
173.00	1212.0
174.00	79632.0
175.00	5996.0
176.00	76496.0
177.00	4933.0
178.00	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	793.0
37.00	3763.0
38.00	3196.0
39.00	1613.0
39.90	205.0
44.00	670.0
44.90	629.0
46.00	138.0
47.00	1170.0
48.00	575.0
49.00	3530.0
50.00	15495.0
51.00	4670.0
52.00	192.0
55.00	236.0
56.00	1356.0
57.00	2115.0
60.00	840.0
61.00	4319.0
62.00	4276.0
63.00	3172.0
64.00	492.0
65.00	757.0
67.00	273.0
68.00	8519.0
69.00	8580.0
70.10	566.0
71.90	617.0
73.00	3781.0
74.00	14852.0
75.00	45328.0
76.00	3706.0
76.90	476.0
78.00	314.0
78.90	2438.0
80.00	836.0
80.90	2485.0
81.90	630.0
85.80	128.0
87.00	3482.0
88.00	3244.0
90.80	275.0
92.00	2280.0
93.10	3761.0
94.00	10606.0
95.00	94552.0
96.00	6400.0
97.10	150.0
103.90	515.0
104.80	133.0
105.90	404.0
109.90	102.0
112.00	137.0
114.90	128.0
115.90	324.0
116.90	683.0
117.80	300.0
118.90	518.0
127.80	244.0
128.00	243.0
128.80	195.0
129.90	359.0
130.90	131.0
134.70	127.0
136.90	289.0
140.80	1069.0
141.80	139.0
142.90	1110.0
144.90	186.0
146.00	138.0
147.90	219.0
149.80	153.0
154.80	302.0
157.00	106.0
158.80	164.0
161.00	148.0
169.90	116.0
170.60	115.0
171.90	949.0
173.00	1101.0
174.00	77176.0
175.00	5517.0
176.00	73808.0
177.00	4568.0
178.00	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
39.90	177.0
43.90	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55