
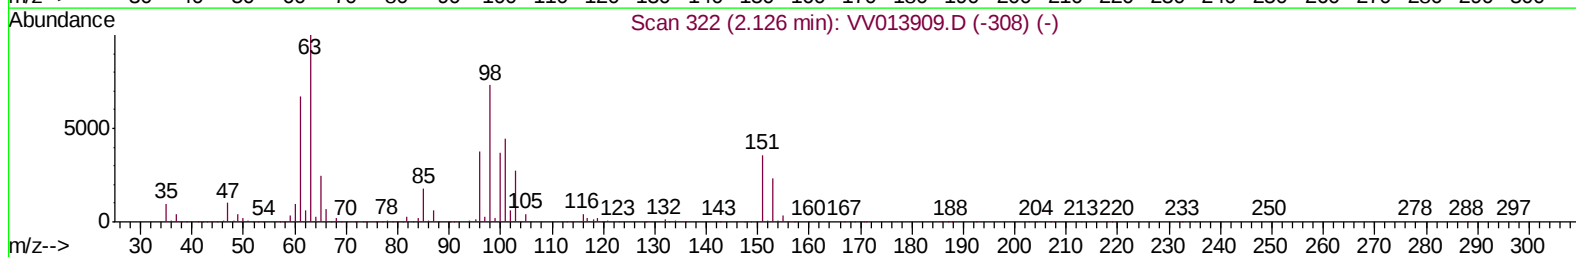
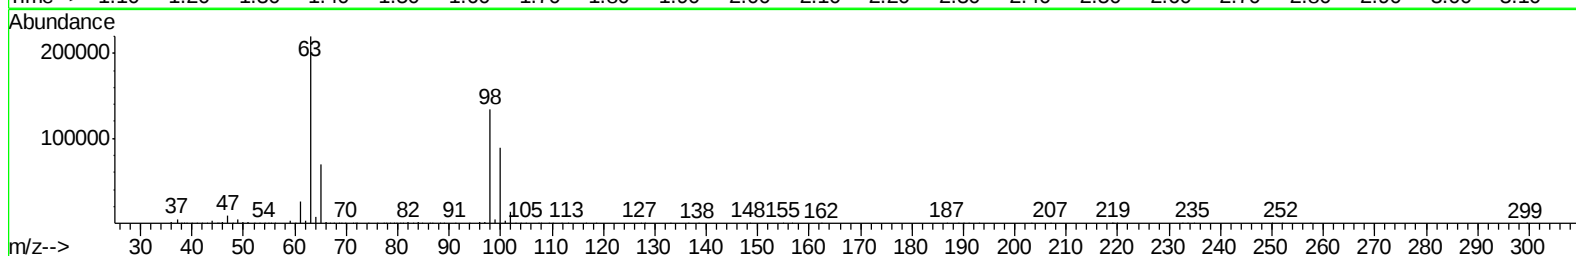


Data File : VV013927.D
Acq On : 05 Dec 2019 20:03
Operator : SY/MD
Sample : K6170-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 06 04:12:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 04:06:40 2019
Response via : Initial Calibration

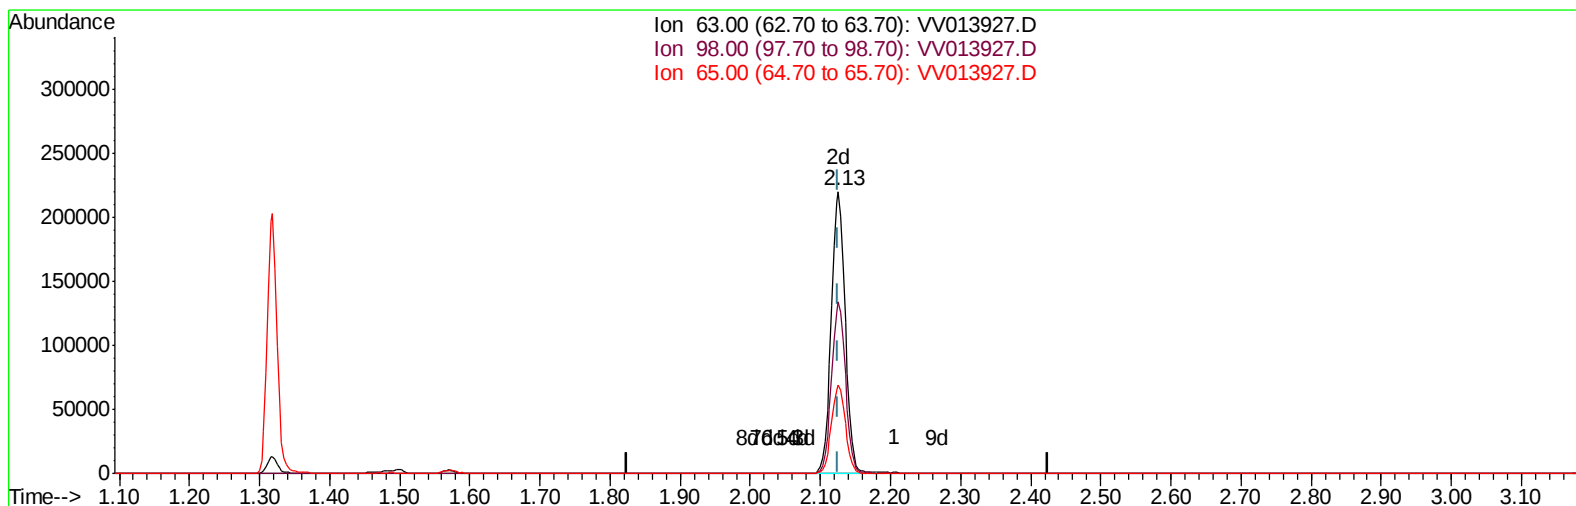

TIC: VV013927.D

(11) 1,1-Dichloroethene-d2 (S)

2.126min (+0.000) 39.93ug/L m

response 304890

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	0.04#
65.00	23.60	0.01#
0.00	0.00	0.00