
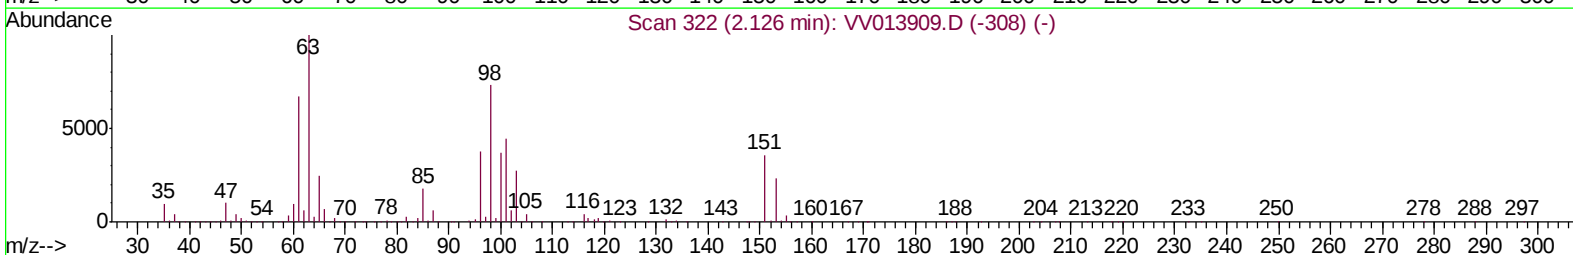
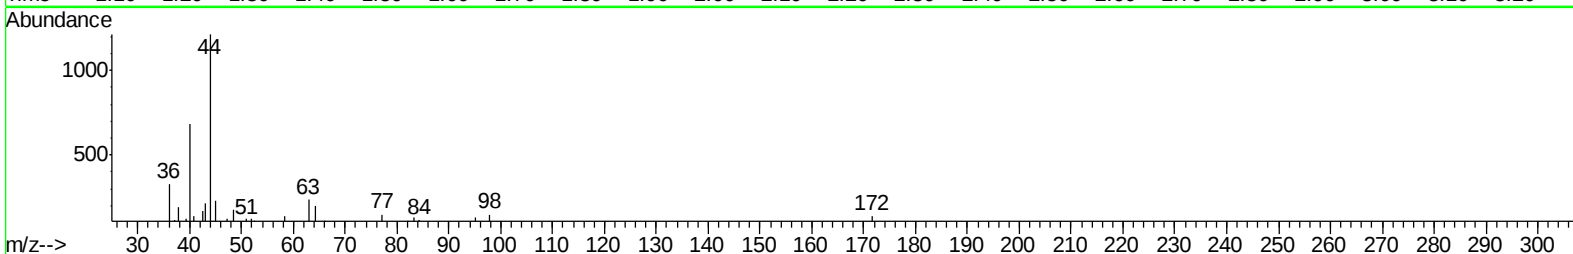


Data File : VV013928.D
Acq On : 05 Dec 2019 20:28
Operator : SY/MD
Sample : K6170-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 06 04:12:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 04:06:40 2019
Response via : Initial Calibration

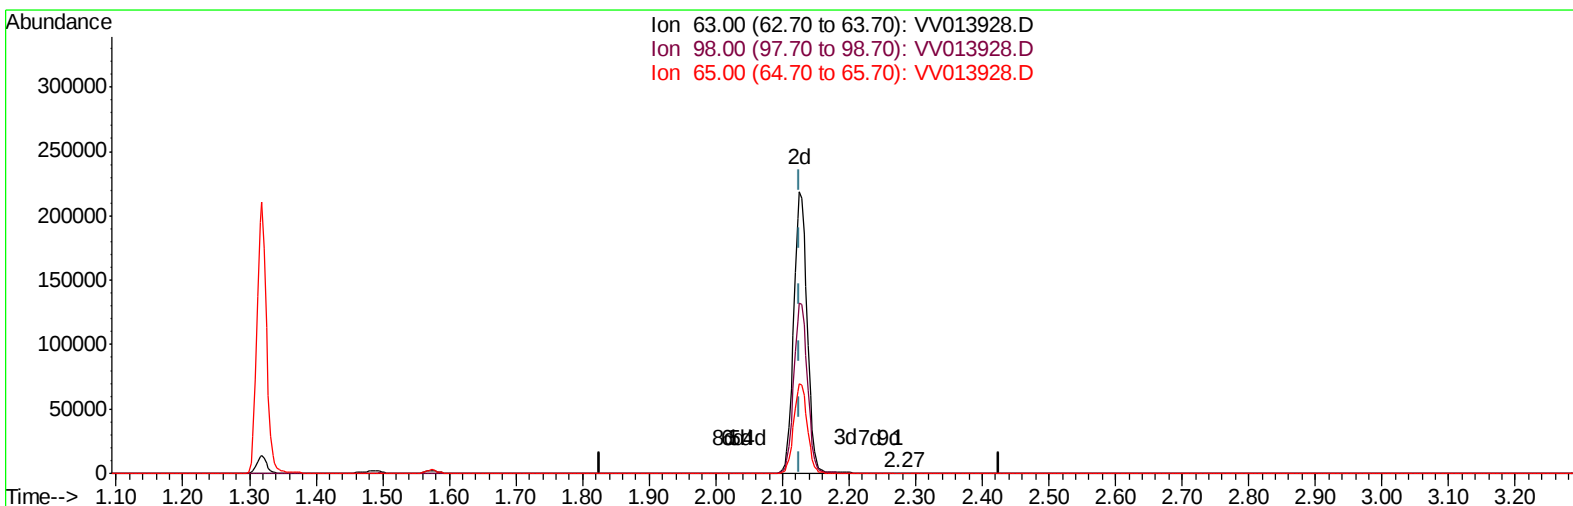

TIC: VV013928.D

(11) 1,1-Dichloroethene-d2 (S)

2.273min (+0.148) 0.03ug/L

response 228

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	69.74
65.00	23.60	30.26
0.00	0.00	0.00