

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013922.D
 Acq On : 05 Dec 2019 18:01
 Operator : SY/MD
 Sample : K6170-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BR7

Quant Time: Dec 06 05:36:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 06 04:06:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	679340	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	649041	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	242311	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	208469	53.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.12%
7) Chloroethane-d5	1.57	69	211827	51.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.30%
11) 1,1-Dichloroethene-d2	2.13	63	318079	36.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.22%
21) 2-Butanone-d5	3.92	46	286677	103.66	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.66%
24) Chloroform-d	4.39	84	432938	52.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.94%
26) 1,2-Dichloroethane-d4	5.08	65	279151	53.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.78%
32) Benzene-d6	5.09	84	906650	53.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.82%
36) 1,2-Dichloropropane-d6	6.11	67	280421	55.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	111.10%
41) Toluene-d8	7.36	98	774652	50.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.04%
43) trans-1,3-Dichloropropene-	7.66	79	116240	47.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.64%
47) 2-Hexanone-d5	8.13	63	157744	83.68	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.68%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	337787	46.21	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.42%
64) 1,2-Dichlorobenzene-d4	11.67	152	269076	56.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.08%


Target Compounds					Ovalue
13) Acetone	2.18	43	6041	1.491 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120519\
Data File : VV013922.D
Acq On : 05 Dec 2019 18:01
Operator : SY/MD
Sample : K6170-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR7

Quant Time: Dec 06 05:36:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 04:06:40 2019
Response via : Initial Calibration

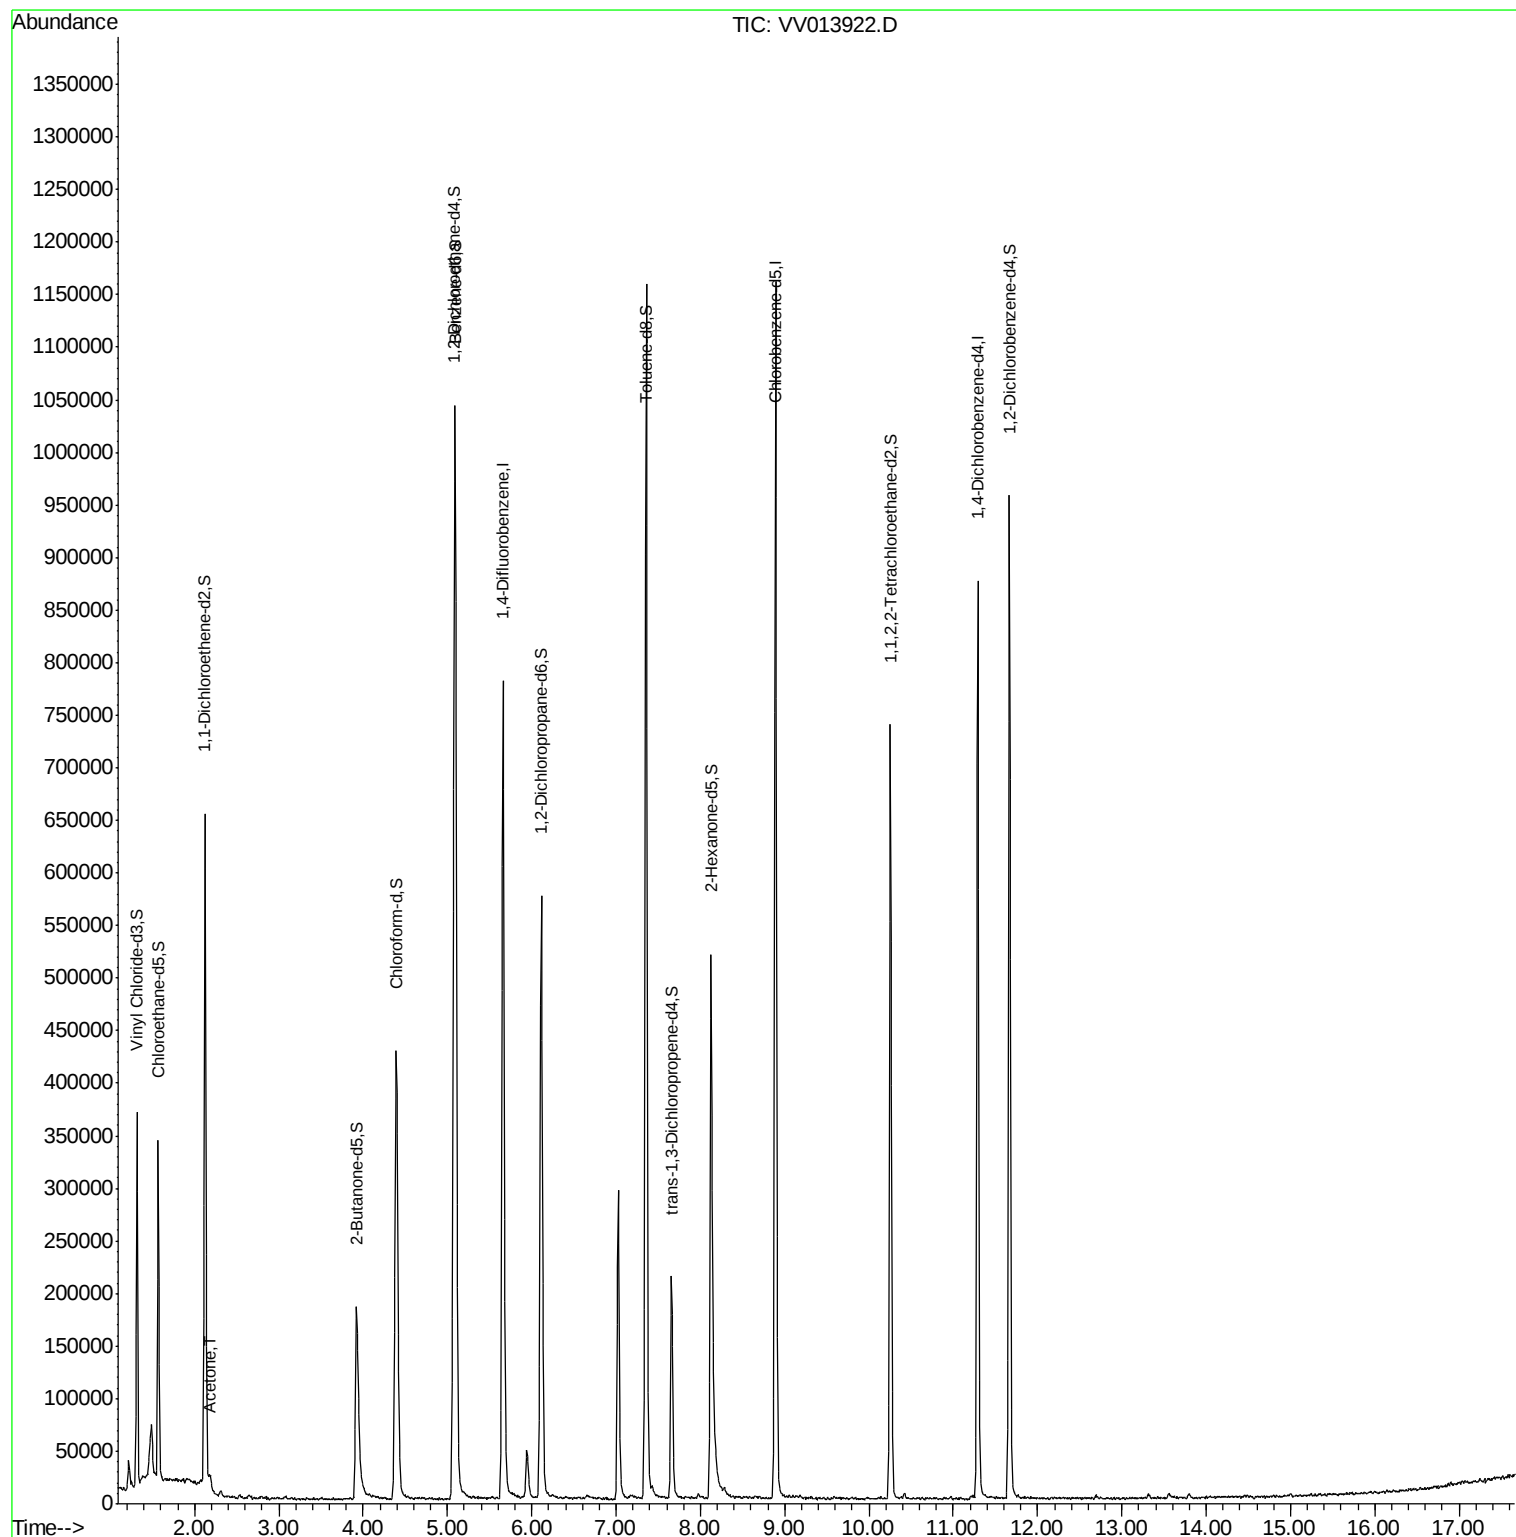

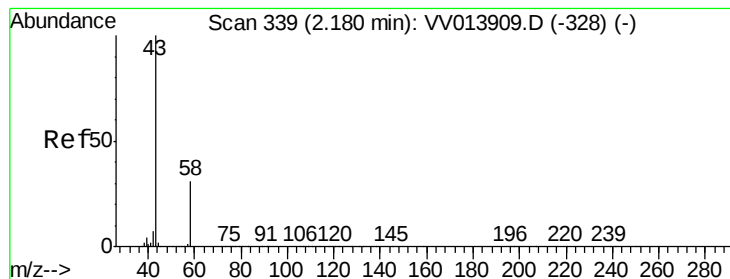

#13
 Acetone
 Concen: 1.491 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. 0.00 min
 Lab File: VV013922.D
 Acq: 05 Dec 2019 18:01

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BR7

Tot Ion: 43 Resp: 6041
 Ion Ratio Lower Upper
 43 100
 58 27.5 0.0 60.8

