

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013926.D
 Acq On : 05 Dec 2019 19:39
 Operator : SY/MD
 Sample : K6170-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BS5

Quant Time: Dec 06 05:48:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 06 04:06:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	550156	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	574408	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	212843	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	203786	64.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	128.10%
7) Chloroethane-d5	1.57	69	203683	61.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	122.66%
11) 1,1-Dichloroethene-d2	2.13	63	307962	43.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.54%
21) 2-Butanone-d5	3.92	46	238678	106.57	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.57%
24) Chloroform-d	4.40	84	361587	54.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.22%
26) 1,2-Dichloroethane-d4	5.08	65	232356	54.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.76%
32) Benzene-d6	5.09	84	748642	50.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.11	67	217744	48.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.48%
41) Toluene-d8	7.36	98	619825	45.68	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.36%
43) trans-1,3-Dichloropropene-	7.66	79	96810	44.53	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.06%
47) 2-Hexanone-d5	8.13	63	127459	76.40	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.40%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	273324	42.25	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.50%
64) 1,2-Dichlorobenzene-d4	11.67	152	230903	55.24	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.48%


Target Compounds					Ovalue
13) Acetone	2.18	43	5456	1.662 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120519\
Data File : VV013926.D
Acq On : 05 Dec 2019 19:39
Operator : SY/MD
Sample : K6170-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BS5

Quant Time: Dec 06 05:48:01 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 04:06:40 2019
Response via : Initial Calibration

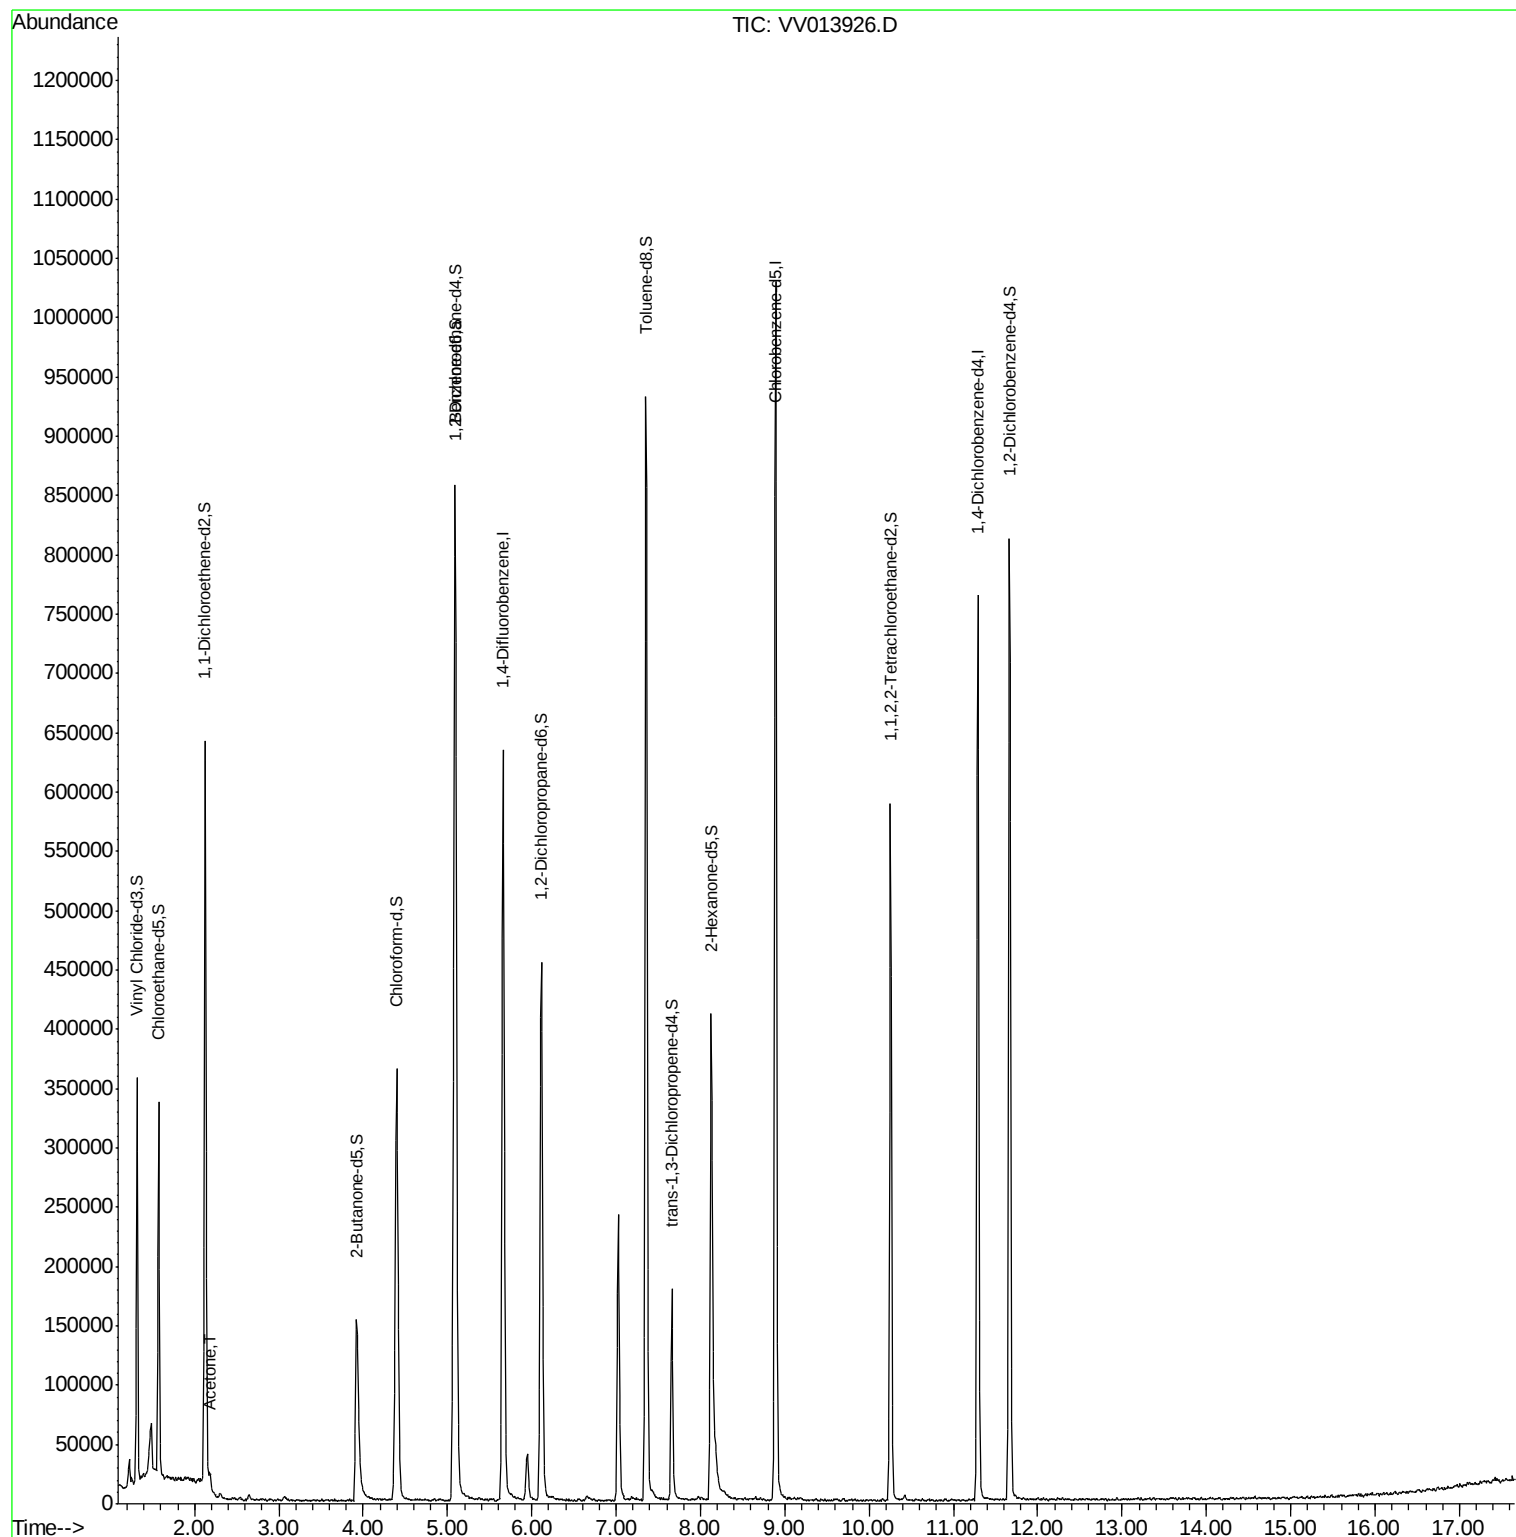

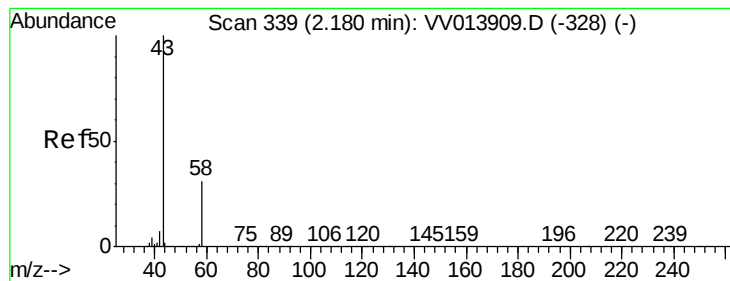

#13
 Acetone
 Concen: 1.662 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. 0.00 min
 Lab File: VV013926.D
 Acq: 05 Dec 2019 19:39

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BS5

Tot Ion: 43 Resp: 5456
 Ion Ratio Lower Upper
 43 100
 58 26.5 0.0 60.8

