

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013929.D
 Acq On : 05 Dec 2019 20:52
 Operator : SY/MD
 Sample : K6170-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT4

Quant Time: Dec 06 06:00:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 06 04:06:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	590154	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	579253	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	227384	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	205761	60.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	120.56%
7) Chloroethane-d5	1.57	69	201157	56.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	112.92%
11) 1,1-Dichloroethene-d2	2.13	63	304850	40.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.78%
21) 2-Butanone-d5	3.92	46	242349	100.88	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.88%
24) Chloroform-d	4.40	84	355985	49.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.32%
26) 1,2-Dichloroethane-d4	5.07	65	228742	50.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.72%
32) Benzene-d6	5.09	84	737133	49.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.22%
36) 1,2-Dichloropropane-d6	6.11	67	215119	47.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.50%
41) Toluene-d8	7.36	98	614038	44.87	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.74%
43) trans-1,3-Dichloropropene-	7.66	79	91357	41.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.34%
47) 2-Hexanone-d5	8.13	63	140872	83.73	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.73%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	307833	47.18	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.36%
64) 1,2-Dichlorobenzene-d4	11.67	152	243843	54.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.20%


Target Compounds					Ovalue
13) Acetone	2.18	43	5246	1.490 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
Data File : VV013929.D
Acq On : 05 Dec 2019 20:52
Operator : SY/MD
Sample : K6170-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT4

Quant Time: Dec 06 06:00:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 04:06:40 2019
Response via : Initial Calibration

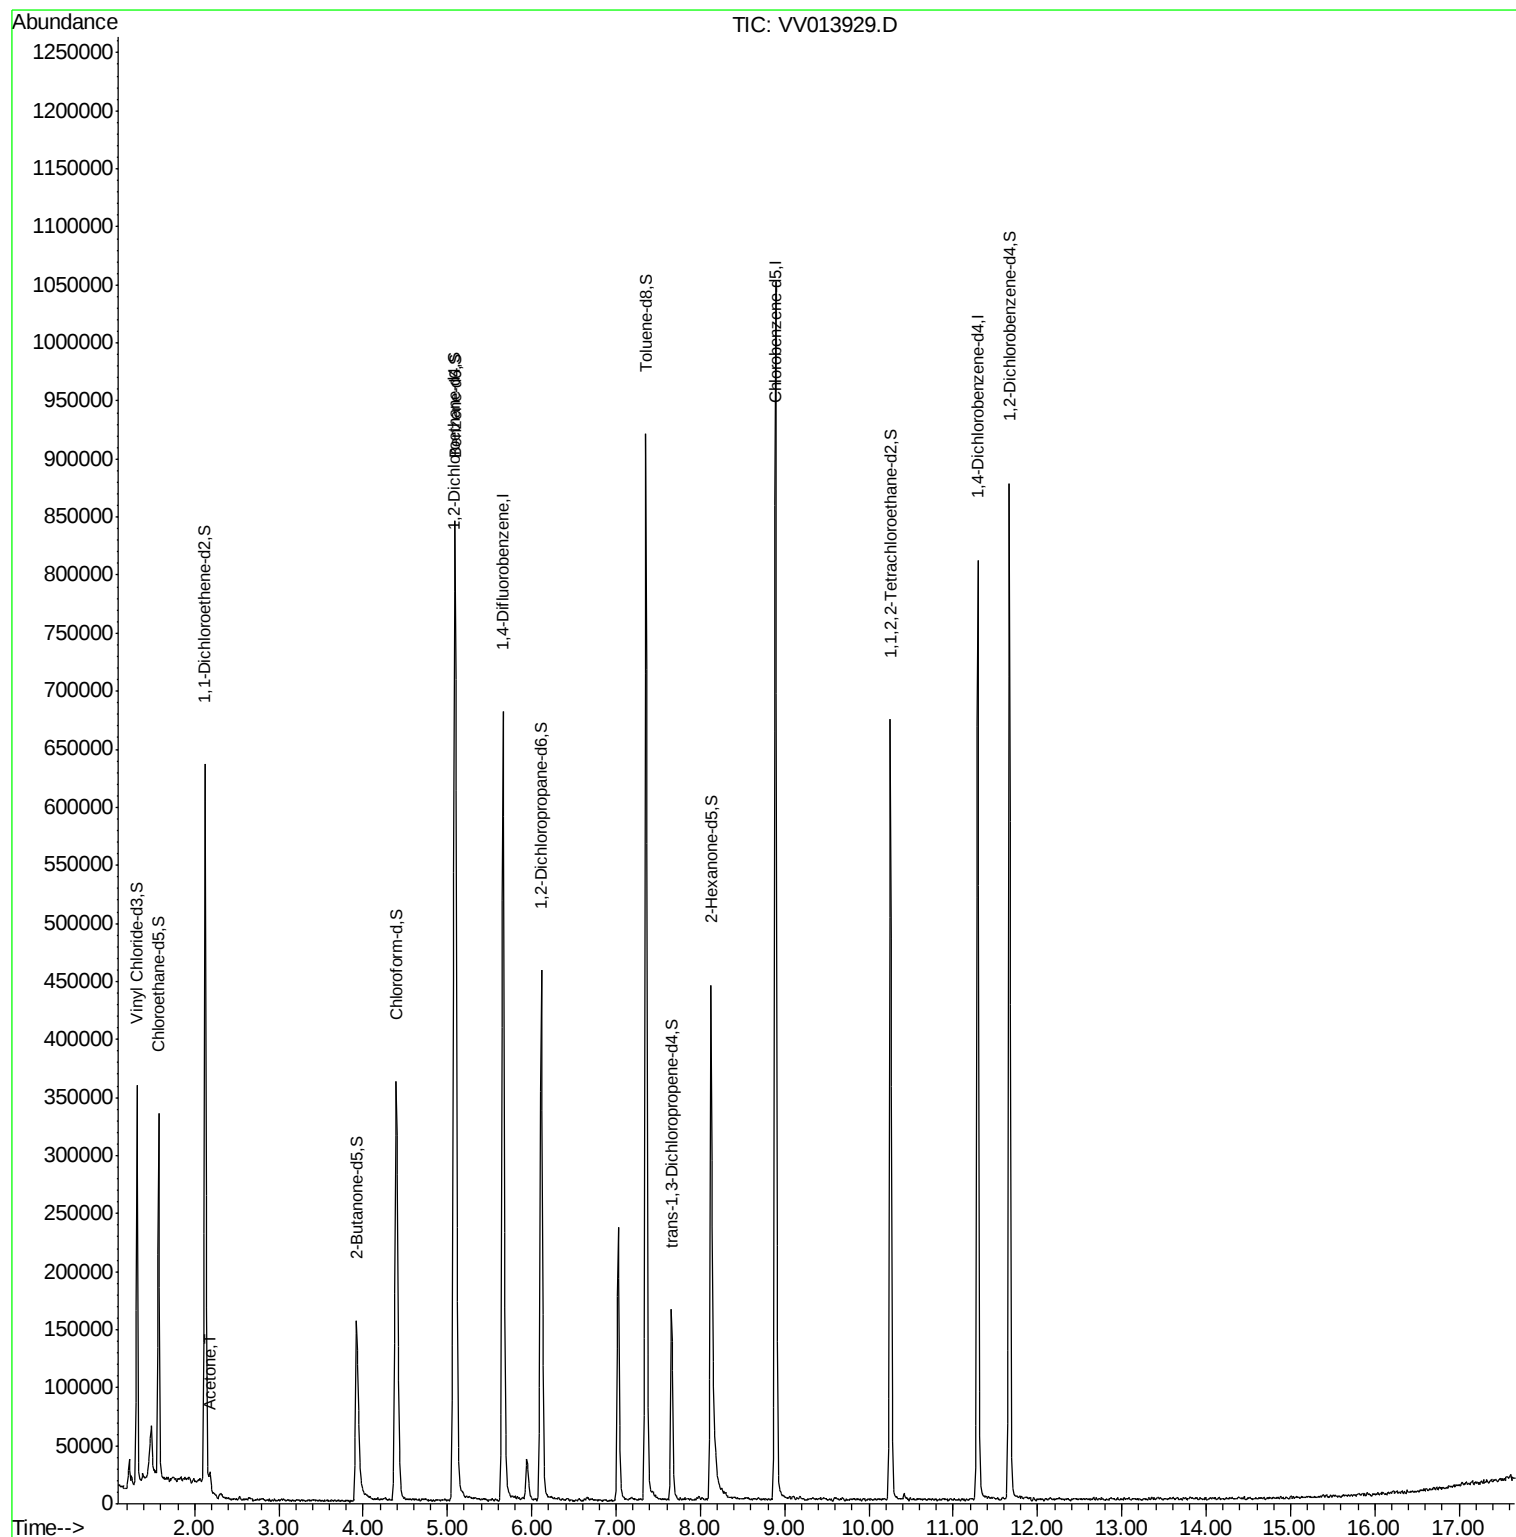

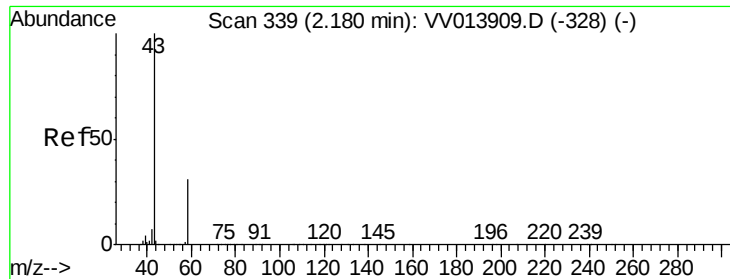

#13

Acetone

Concen: 1.490 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV013929.D

Acq: 05 Dec 2019 20:52

Instrument :
MSVOA_V
ClientSampleId :
C0BT4

Tot Ion: 43 Resp: 5246

Ion Ratio Lower Upper

43 100

58 37.2 0.0 60.8

