

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013910.D
 Acq On : 05 Dec 2019 11:41
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	267244	263139	12.21%	1.611%
2	1.557	140	145	161	rVB	271910	322831	14.98%	1.977%
3	2.119	312	320	334	rVB	529610	754234	34.99%	4.619%
4	2.380	399	401	404	rBV3	2438	1332	0.06%	0.008%
5	2.508	438	441	442	rBV2	2291	1503	0.07%	0.009%
6	2.582	460	464	467	rBV5	1568	1406	0.07%	0.009%
7	2.849	545	547	549	rBV2	932	457	0.02%	0.003%
8	2.920	567	569	573	rBV4	1410	1195	0.06%	0.007%
9	3.042	604	607	610	rBV4	1349	735	0.03%	0.005%
10	3.071	614	616	617	rBV	878	288	0.01%	0.002%
11	3.148	635	640	641	rBV3	913	631	0.03%	0.004%
12	3.155	641	642	644	rBV2	1367	640	0.03%	0.004%
13	3.206	656	658	660	rBV2	1584	928	0.04%	0.006%
14	3.290	683	684	685	rVB	798	154	0.01%	0.001%
15	3.299	685	687	689	rBV3	828	287	0.01%	0.002%
16	3.319	689	693	697	rBV6	1142	1025	0.05%	0.006%
17	3.380	709	712	715	rBV4	1749	1582	0.07%	0.010%
18	3.431	726	728	731	rBV4	1428	861	0.04%	0.005%
19	3.540	759	762	767	rBV6	1387	1596	0.07%	0.010%
20	3.605	779	782	784	rBV3	744	474	0.02%	0.003%
21	3.656	795	798	799	rBV2	1412	924	0.04%	0.006%
22	3.711	813	815	817	rBV2	925	433	0.02%	0.003%
23	3.733	820	822	823	rBV2	536	217	0.01%	0.001%
24	3.782	834	837	838	rBV3	1019	452	0.02%	0.003%
25	3.807	842	845	848	rBV4	776	608	0.03%	0.004%
26	3.852	856	859	860	rBV3	1072	566	0.03%	0.003%
27	3.920	869	880	913	rBV	173835	466386	21.64%	2.856%
28	4.306	998	1000	1005	rBV3	1286	683	0.03%	0.004%
29	4.392	1011	1027	1054	rBV	373656	892840	41.42%	5.467%
30	4.573	1079	1083	1086	rBV4	2088	1367	0.06%	0.008%
31	4.589	1086	1088	1089	rBV	1234	460	0.02%	0.003%
32	4.653	1104	1108	1110	rBV3	1811	1506	0.07%	0.009%
33	4.708	1123	1125	1127	rBV3	1910	894	0.04%	0.005%
34	4.833	1162	1164	1165	rVB2	729	187	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013910.D
 Acq On : 05 Dec 2019 11:41
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.087	1226	1243	1279	rBV2	853075	2155381	100.00%	13.199%
36	5.344	1321	1323	1325	rBV3	1444	785	0.04%	0.005%
37	5.396	1336	1339	1344	rBV5	1698	1431	0.07%	0.009%
38	5.601	1399	1403	1404	rBV3	2556	1541	0.07%	0.009%
39	5.656	1407	1420	1447	rVV	707425	1392970	64.63%	8.530%
40	6.109	1548	1561	1582	rBV	489804	993498	46.09%	6.084%
41	6.325	1626	1628	1629	rBV2	1560	626	0.03%	0.004%
42	6.386	1646	1647	1649	rBV2	1456	805	0.04%	0.005%
43	6.460	1668	1670	1672	rBV3	1099	646	0.03%	0.004%
44	6.585	1706	1709	1716	rVB5	1531	1442	0.07%	0.009%
45	6.614	1716	1718	1720	rBV3	1394	793	0.04%	0.005%
46	6.801	1773	1776	1778	rBV3	1339	876	0.04%	0.005%
47	6.839	1786	1788	1790	rBV3	1061	412	0.02%	0.003%
48	6.907	1807	1809	1812	rBV4	1291	629	0.03%	0.004%
49	6.939	1815	1819	1820	rBV4	991	509	0.02%	0.003%
50	7.023	1833	1845	1867	rBV	257215	464114	21.53%	2.842%
51	7.248	1912	1915	1916	rBV2	1628	882	0.04%	0.005%
52	7.354	1935	1948	1969	rBV	963362	1670870	77.52%	10.232%
53	7.656	2032	2042	2061	rBV	182039	310002	14.38%	1.898%
54	8.125	2178	2188	2222	rBV2	523994	1063882	49.36%	6.515%
55	8.521	2309	2311	2312	rBV3	1315	402	0.02%	0.002%
56	8.576	2325	2328	2330	rBV4	971	643	0.03%	0.004%
57	8.891	2414	2426	2447	rBV	1042160	1675946	77.76%	10.263%
58	9.235	2531	2533	2538	rVB5	1820	1224	0.06%	0.007%
59	9.254	2538	2539	2544	rBV4	994	789	0.04%	0.005%
60	9.576	2637	2639	2642	rBV3	1530	1164	0.05%	0.007%
61	9.756	2693	2695	2700	rBV4	1441	1208	0.06%	0.007%
62	9.797	2707	2708	2711	rBV3	779	378	0.02%	0.002%
63	9.849	2722	2724	2726	rBV3	1117	741	0.03%	0.005%
64	9.900	2738	2740	2745	rBV3	1148	853	0.04%	0.005%
65	10.003	2770	2772	2773	rBV2	956	312	0.01%	0.002%
66	10.084	2795	2797	2798	rBV2	1164	447	0.02%	0.003%
67	10.113	2802	2806	2808	rVV3	1085	677	0.03%	0.004%
68	10.196	2831	2832	2834	rBV2	1051	570	0.03%	0.003%
69	10.257	2839	2851	2863	rVV	657936	1040438	48.27%	6.371%
70	10.386	2889	2891	2892	rBV2	1873	633	0.03%	0.004%
71	10.476	2916	2919	2920	rBV3	1337	723	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013910.D
 Acq On : 05 Dec 2019 11:41
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.611	2959	2961	2965	rBV3	1059	654	0.03%	0.004%
73	10.685	2982	2984	2985	rBV2	616	143	0.01%	0.001%
74	10.727	2995	2997	3001	rVB3	1641	828	0.04%	0.005%
75	10.752	3001	3005	3006	rBV3	1526	807	0.04%	0.005%
76	10.794	3016	3018	3023	rVB5	1316	1213	0.06%	0.007%
77	10.823	3024	3027	3028	rBV3	1377	687	0.03%	0.004%
78	10.871	3038	3042	3045	rBV4	1303	1188	0.06%	0.007%
79	10.965	3064	3071	3076	rBV8	2556	3191	0.15%	0.020%
80	11.289	3160	3172	3198	rBV	842485	1322234	61.35%	8.097%
81	11.563	3255	3257	3262	rBV4	1220	1103	0.05%	0.007%
82	11.595	3265	3267	3268	rBV2	813	261	0.01%	0.002%
83	11.665	3277	3289	3308	rBV	937747	1472707	68.33%	9.018%
84	11.903	3361	3363	3364	rBV2	1863	930	0.04%	0.006%
85	11.984	3387	3388	3391	rBV3	1302	570	0.03%	0.003%
86	12.122	3425	3431	3434	rBV7	1940	2280	0.11%	0.014%
87	12.334	3494	3497	3500	rBV3	2305	1685	0.08%	0.010%
88	12.434	3526	3528	3531	rVB4	1832	745	0.03%	0.005%
89	12.736	3619	3622	3625	rBV3	1591	1329	0.06%	0.008%
90	13.421	3833	3835	3838	rBV2	2046	1322	0.06%	0.008%
91	13.646	3903	3905	3906	rBV2	1414	633	0.03%	0.004%
92	13.865	3971	3973	3974	rBV2	1289	577	0.03%	0.004%
93	13.923	3989	3991	3993	rBV	951	471	0.02%	0.003%
94	14.022	4020	4022	4027	rBV4	1578	1117	0.05%	0.007%
95	14.440	4150	4152	4156	rBV4	1759	1281	0.06%	0.008%


Sum of corrected areas: 16330019

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120519\
Data File : VV013910.D
Acq On : 05 Dec 2019 11:41
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

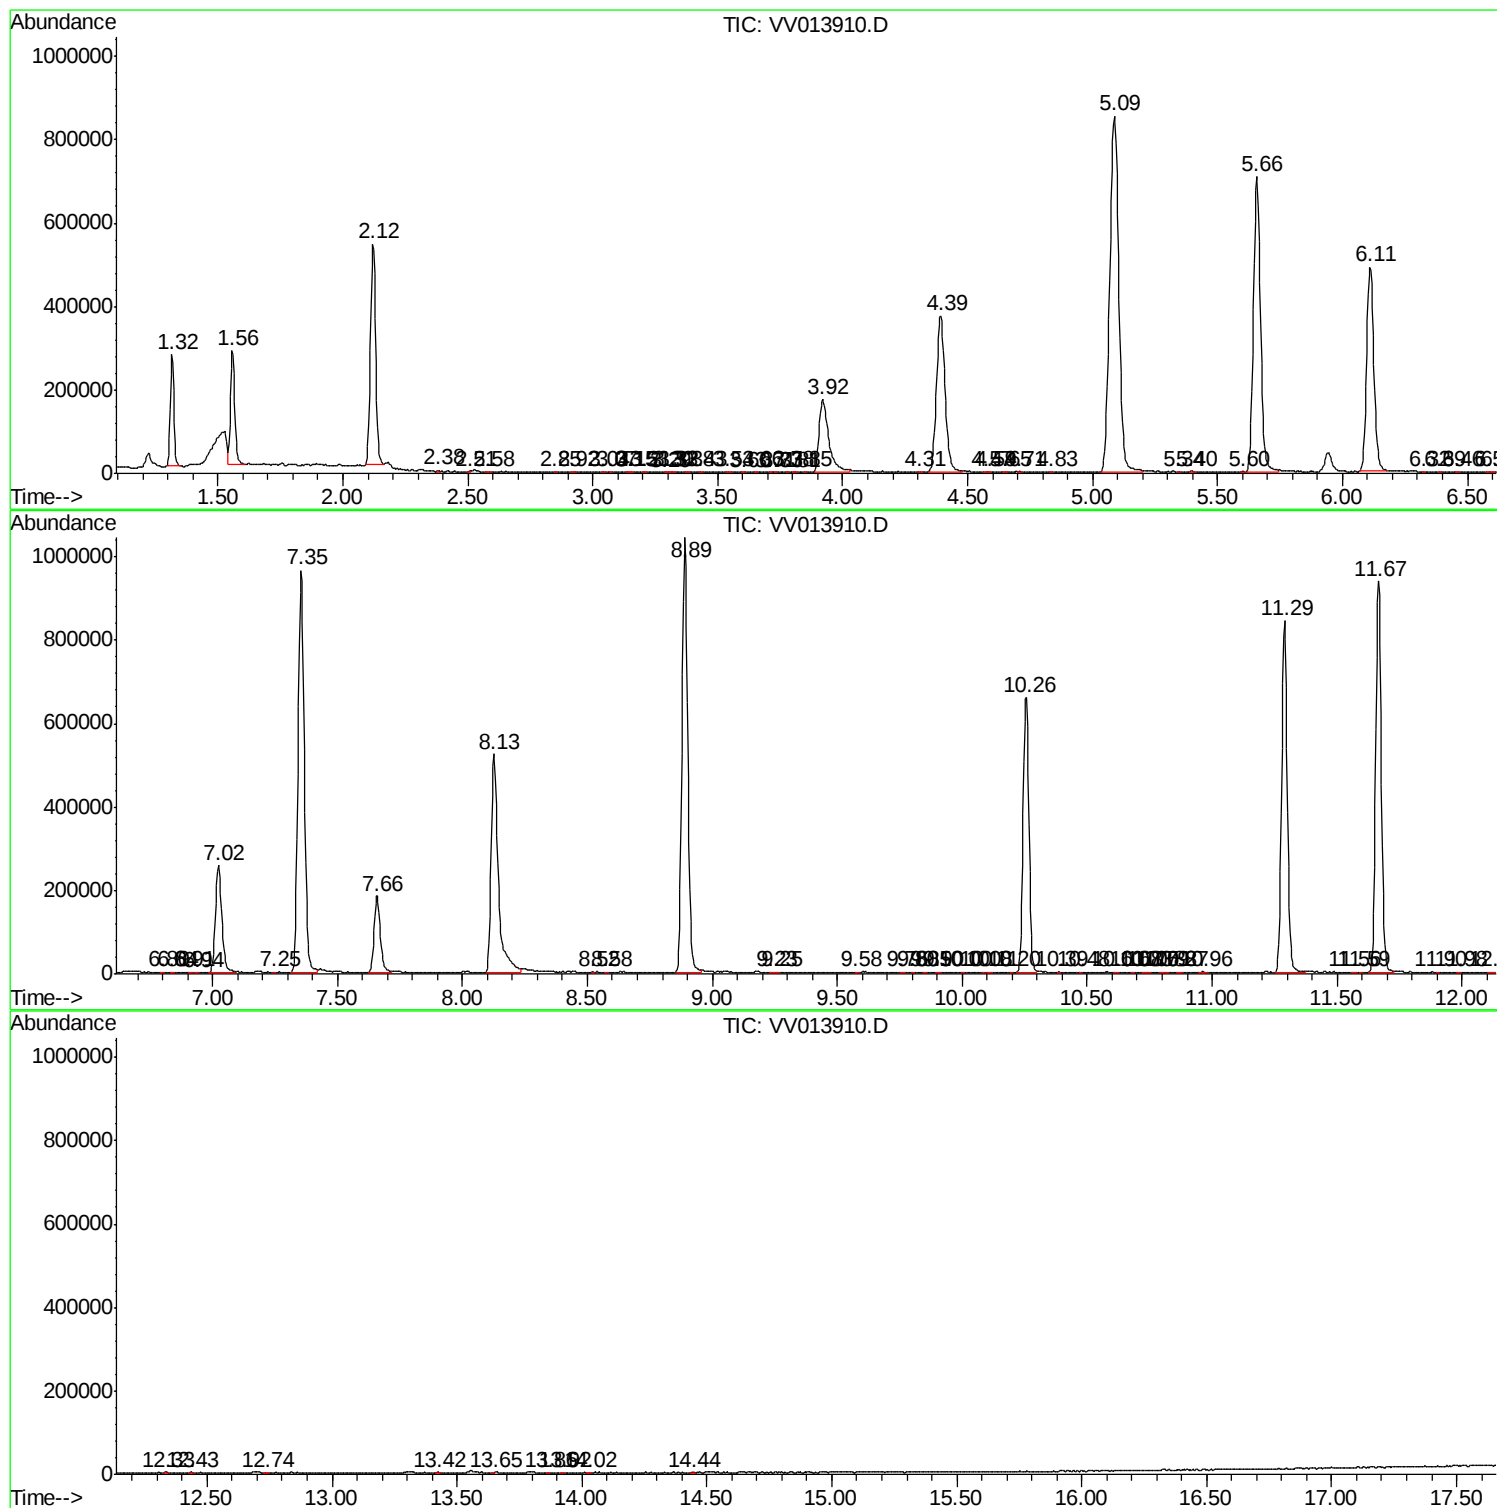

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120519\
Data File : VV013910.D
Acq On : 05 Dec 2019 11:41
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120519\
Data File : VV013910.D
Acq On : 05 Dec 2019 11:41
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc