

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013916.D
 Acq On : 05 Dec 2019 15:11
 Operator : SY/MD
 Sample : K6165-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBT4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	79	rVB	243720	233665	11.04%	1.418%
2	1.569	143	149	159	rVB	257641	291429	13.77%	1.769%
3	2.126	314	322	333	rVB	492737	697199	32.95%	4.232%
4	2.859	548	550	551	rBV	1347	678	0.03%	0.004%
5	2.904	562	564	567	rBV4	1012	715	0.03%	0.004%
6	2.997	586	593	594	rBV6	1546	1702	0.08%	0.010%
7	3.158	641	643	646	rBV4	1023	644	0.03%	0.004%
8	3.222	661	663	664	rBV2	937	313	0.01%	0.002%
9	3.261	673	675	679	rBV3	1239	859	0.04%	0.005%
10	3.280	679	681	685	rVB4	1341	686	0.03%	0.004%
11	3.303	685	688	692	rBV4	1604	1150	0.05%	0.007%
12	3.319	692	693	696	rBV4	735	497	0.02%	0.003%
13	3.505	750	751	752	rBV4	847	213	0.01%	0.001%
14	3.547	762	764	766	rBV2	1202	788	0.04%	0.005%
15	3.579	770	774	778	rBV7	1443	1368	0.06%	0.008%
16	3.634	789	791	794	rBV3	746	471	0.02%	0.003%
17	3.679	804	805	808	rBV3	705	446	0.02%	0.003%
18	3.711	812	815	817	rBV	1125	684	0.03%	0.004%
19	3.769	829	833	836	rBV5	1277	1293	0.06%	0.008%
20	3.852	856	859	862	rBV4	1350	1022	0.05%	0.006%
21	3.923	870	881	915	rBV	173784	498903	23.58%	3.028%
22	4.290	993	995	999	rVB5	1678	1030	0.05%	0.006%
23	4.399	1013	1029	1054	rBV4	399882	1178741	55.71%	7.155%
24	4.643	1102	1105	1109	rVB5	1732	1258	0.06%	0.008%
25	4.721	1127	1129	1130	rBV2	995	433	0.02%	0.003%
26	5.010	1217	1219	1221	rBV3	751	408	0.02%	0.002%
27	5.090	1226	1244	1271	rBV2	832540	2115989	100.00%	12.843%
28	5.450	1352	1356	1361	rBV5	1845	2098	0.10%	0.013%
29	5.659	1408	1421	1446	rBV	711267	1395693	65.96%	8.471%
30	5.859	1481	1483	1487	rBV5	2037	913	0.04%	0.006%
31	6.113	1549	1562	1586	rBV	482084	957945	45.27%	5.814%
32	6.553	1689	1699	1710	rBV	82373	147385	6.97%	0.895%
33	6.772	1765	1767	1771	rBV4	1408	899	0.04%	0.005%
34	7.026	1834	1846	1868	rBV2	252730	449549	21.25%	2.729%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013916.D
 Acq On : 05 Dec 2019 15:11
 Operator : SY/MD
 Sample : K6165-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBT4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	7.273	1915	1923	1927	rBV6	6048	9450	0.45%	0.057%
36	7.357	1936	1949	1969	rBV	949617	1635523	77.29%	9.927%
37	7.659	2032	2043	2067	rBV	184655	322712	15.25%	1.959%
38	8.016	2147	2154	2168	rVB	51305	86901	4.11%	0.527%
39	8.126	2177	2188	2221	rBV2	499035	1023981	48.39%	6.215%
40	8.749	2379	2382	2385	rVB6	1679	892	0.04%	0.005%
41	8.765	2385	2387	2389	rBV	894	449	0.02%	0.003%
42	8.891	2414	2426	2446	rBV	1036214	1660537	78.48%	10.079%
43	9.187	2516	2518	2526	rVB7	1810	1832	0.09%	0.011%
44	9.264	2539	2542	2543	rBV3	1582	789	0.04%	0.005%
45	9.588	2637	2643	2646	rBV6	1644	1875	0.09%	0.011%
46	9.688	2670	2674	2675	rBV3	1266	899	0.04%	0.005%
47	9.939	2749	2752	2755	rBV3	1680	1048	0.05%	0.006%
48	10.026	2777	2779	2780	rBV2	1216	501	0.02%	0.003%
49	10.103	2800	2803	2805	rBV4	1250	906	0.04%	0.005%
50	10.164	2818	2822	2823	rBV3	1315	822	0.04%	0.005%
51	10.254	2839	2850	2867	rBV	645440	1017735	48.10%	6.177%
52	10.379	2887	2889	2890	rBV2	1318	531	0.03%	0.003%
53	10.537	2936	2938	2941	rBV3	2041	1364	0.06%	0.008%
54	10.740	2999	3001	3003	rVB3	1019	380	0.02%	0.002%
55	10.772	3008	3011	3013	rBV4	1388	1046	0.05%	0.006%
56	10.846	3032	3034	3036	rBV2	1245	647	0.03%	0.004%
57	10.920	3055	3057	3061	rVB3	2062	1237	0.06%	0.008%
58	10.958	3061	3069	3072	rBV8	1935	2788	0.13%	0.017%
59	10.990	3077	3079	3080	rBV2	1274	553	0.03%	0.003%
60	11.051	3097	3098	3099	rBV	681	205	0.01%	0.001%
61	11.177	3134	3137	3141	rBV6	2291	1523	0.07%	0.009%
62	11.199	3141	3144	3145	rBV3	1720	1056	0.05%	0.006%
63	11.289	3161	3172	3189	rBV	847337	1300759	61.47%	7.895%
64	11.666	3277	3289	3312	rVB	884270	1407149	66.50%	8.541%
65	12.244	3464	3469	3471	rBV4	1397	1061	0.05%	0.006%
66	12.399	3515	3517	3521	rBV4	1291	966	0.05%	0.006%


Sum of corrected areas: 16475183

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120519\
Data File : VV013916.D
Acq On : 05 Dec 2019 15:11
Operator : SY/MD
Sample : K6165-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBT4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

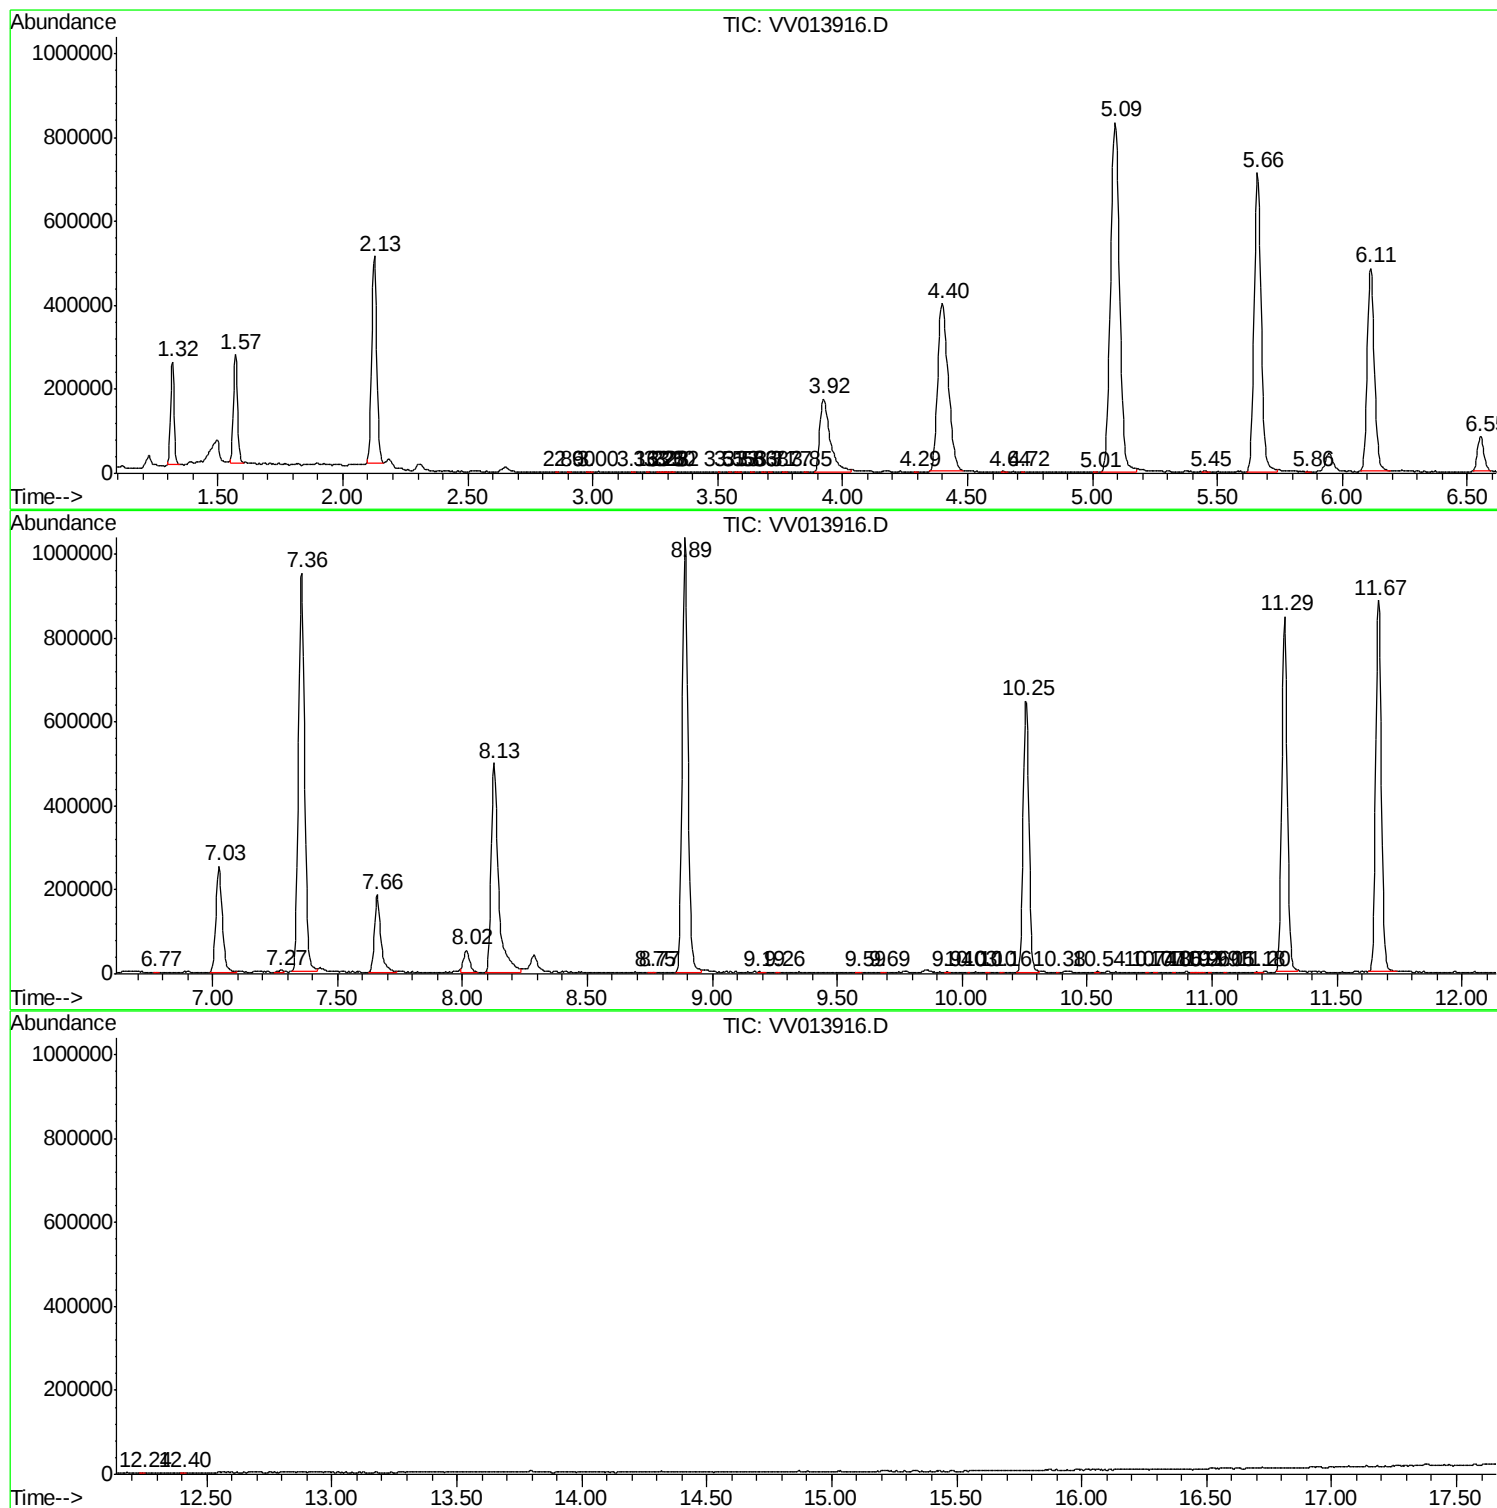

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120519\
Data File : VV013916.D
Acq On : 05 Dec 2019 15:11
Operator : SY/MD
Sample : K6165-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBT4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120519\
Data File : VV013916.D
Acq On : 05 Dec 2019 15:11
Operator : SY/MD
Sample : K6165-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBT4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc