

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013922.D
 Acq On : 05 Dec 2019 18:01
 Operator : SY/MD
 Sample : K6170-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BR7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	81	rVB	352317	337964	13.01%	1.823%
2	1.569	143	149	163	rVB	321706	376896	14.51%	2.033%
3	2.126	313	322	335	rVB	631166	871541	33.54%	4.700%
4	2.524	442	446	447	rBV4	2909	2082	0.08%	0.011%
5	2.634	477	480	482	rBV4	2108	1666	0.06%	0.009%
6	2.698	496	500	501	rBV4	2286	1608	0.06%	0.009%
7	2.872	552	554	558	rVB4	1702	952	0.04%	0.005%
8	2.894	558	561	564	rBV4	1415	1104	0.04%	0.006%
9	3.184	648	651	652	rBV3	1874	914	0.04%	0.005%
10	3.216	656	661	662	rBV3	1294	1096	0.04%	0.006%
11	3.299	682	687	689	rBV5	1229	919	0.04%	0.005%
12	3.325	692	695	696	rBV2	1152	620	0.02%	0.003%
13	3.364	705	707	709	rBV2	1136	455	0.02%	0.002%
14	3.383	709	713	715	rBV2	830	600	0.02%	0.003%
15	3.441	730	731	733	rBV2	1182	556	0.02%	0.003%
16	3.557	765	767	768	rVB2	965	227	0.01%	0.001%
17	3.589	774	777	779	rBV3	1108	530	0.02%	0.003%
18	3.676	799	804	805	rBV5	1134	842	0.03%	0.005%
19	3.708	812	814	816	rBV3	1524	778	0.03%	0.004%
20	3.762	829	831	833	rBV3	910	640	0.02%	0.003%
21	3.923	867	881	905	rBV	183514	500610	19.27%	2.700%
22	4.267	986	988	992	rVB3	1930	1056	0.04%	0.006%
23	4.286	992	994	996	rBV3	1132	605	0.02%	0.003%
24	4.312	1000	1002	1005	rBV3	1201	718	0.03%	0.004%
25	4.393	1011	1027	1053	rBV	425900	1056410	40.66%	5.697%
26	4.904	1183	1186	1190	rVB4	2348	1583	0.06%	0.009%
27	4.965	1201	1205	1208	rBV7	1044	1011	0.04%	0.005%
28	5.029	1222	1225	1226	rBV2	1313	765	0.03%	0.004%
29	5.090	1226	1244	1271	rVV2	1039270	2598237	100.00%	14.013%
30	5.274	1299	1301	1305	rVB4	1700	876	0.03%	0.005%
31	5.367	1328	1330	1336	rBV7	1846	1374	0.05%	0.007%
32	5.437	1349	1352	1355	rBV3	1647	1210	0.05%	0.007%
33	5.479	1361	1365	1367	rBV5	1971	1648	0.06%	0.009%
34	5.515	1373	1376	1378	rBV4	1358	962	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013922.D
 Acq On : 05 Dec 2019 18:01
 Operator : SY/MD
 Sample : K6170-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BR7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.659	1407	1421	1443	rBV	776673	1536939	59.15%	8.289%
36	5.942	1501	1509	1526	rVB3	44413	91049	3.50%	0.491%
37	6.113	1549	1562	1585	rBV	569764	1163994	44.80%	6.278%
38	6.852	1788	1792	1795	rBV3	2010	1786	0.07%	0.010%
39	6.868	1795	1797	1799	rBV3	1252	729	0.03%	0.004%
40	6.897	1804	1806	1810	rVB5	2426	1447	0.06%	0.008%
41	6.913	1810	1811	1814	rBV3	1285	825	0.03%	0.004%
42	6.936	1816	1818	1823	rVB4	1131	901	0.03%	0.005%
43	6.968	1825	1828	1830	rVB4	1267	751	0.03%	0.004%
44	7.026	1834	1846	1863	rBV	294254	532834	20.51%	2.874%
45	7.302	1931	1932	1933	rBV	1204	288	0.01%	0.002%
46	7.357	1933	1949	1967	rBV	1155997	2026280	77.99%	10.928%
47	7.659	2033	2043	2060	rBV	210180	352899	13.58%	1.903%
48	8.129	2177	2189	2223	rBV2	517359	1112986	42.84%	6.003%
49	8.830	2404	2407	2408	rBV3	1239	602	0.02%	0.003%
50	8.891	2414	2426	2448	rBV	1156308	1851055	71.24%	9.983%
51	9.232	2528	2532	2534	rBV4	2090	1906	0.07%	0.010%
52	9.267	2539	2543	2546	rBV6	2081	1351	0.05%	0.007%
53	9.386	2578	2580	2581	rBV2	867	265	0.01%	0.001%
54	9.402	2582	2585	2587	rBV4	1529	1015	0.04%	0.005%
55	9.498	2610	2615	2616	rBV4	1203	1012	0.04%	0.005%
56	9.540	2625	2628	2629	rBV3	1637	1110	0.04%	0.006%
57	9.576	2636	2639	2640	rBV2	1614	865	0.03%	0.005%
58	9.678	2668	2671	2673	rBV3	1491	870	0.03%	0.005%
59	9.768	2697	2699	2702	rBV4	1454	1092	0.04%	0.006%
60	9.865	2725	2729	2730	rBV4	1298	864	0.03%	0.005%
61	9.936	2749	2751	2754	rBV4	1425	991	0.04%	0.005%
62	9.952	2754	2756	2758	rBV2	649	298	0.01%	0.002%
63	9.968	2758	2761	2762	rBV4	1804	1094	0.04%	0.006%
64	10.138	2810	2814	2817	rBV6	2134	1688	0.06%	0.009%
65	10.254	2838	2850	2866	rBV	736779	1150656	44.29%	6.206%
66	10.373	2885	2887	2889	rBV3	1738	861	0.03%	0.005%
67	10.450	2909	2911	2914	rVB3	972	400	0.02%	0.002%
68	10.672	2978	2980	2981	rBV2	1624	633	0.02%	0.003%
69	10.871	3041	3042	3044	rBV2	1086	386	0.01%	0.002%
70	10.884	3044	3046	3047	rBV2	1537	645	0.02%	0.003%
71	11.064	3100	3102	3105	rBV3	1923	823	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013922.D
 Acq On : 05 Dec 2019 18:01
 Operator : SY/MD
 Sample : K6170-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BR7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.141	3122	3126	3129	rBV3	1243	943	0.04%	0.005%
73	11.289	3160	3172	3193	rBV	871569	1367092	52.62%	7.373%
74	11.666	3276	3289	3310	rBV	953811	1533522	59.02%	8.271%
75	12.199	3452	3455	3456	rBV3	1618	1040	0.04%	0.006%
76	12.228	3463	3464	3467	rBV3	1177	441	0.02%	0.002%
77	12.321	3491	3493	3496	rBV5	2395	1400	0.05%	0.008%
78	12.357	3501	3504	3505	rBV3	1418	702	0.03%	0.004%
79	12.405	3515	3519	3522	rBV4	1725	1574	0.06%	0.008%
80	12.534	3555	3559	3560	rBV2	1624	1062	0.04%	0.006%
81	12.691	3600	3608	3611	rBV7	4773	5998	0.23%	0.032%
82	12.817	3644	3647	3649	rBV3	1526	838	0.03%	0.005%
83	12.900	3670	3673	3674	rBV3	1549	861	0.03%	0.005%
84	13.006	3703	3706	3709	rBV5	1342	1128	0.04%	0.006%
85	13.055	3716	3721	3724	rBV6	2039	2102	0.08%	0.011%
86	13.090	3729	3732	3734	rBV3	2241	1574	0.06%	0.008%
87	13.164	3753	3755	3759	rBV5	1382	840	0.03%	0.005%
88	13.225	3773	3774	3777	rVB3	1643	543	0.02%	0.003%
89	13.399	3826	3828	3831	rBV3	1505	1050	0.04%	0.006%
90	13.518	3863	3865	3869	rBV4	1378	894	0.03%	0.005%
91	14.000	4012	4015	4018	rBV3	2348	1536	0.06%	0.008%
92	14.588	4193	4198	4200	rBV5	2578	2318	0.09%	0.013%
93	14.714	4234	4237	4239	rBV3	1931	1217	0.05%	0.007%


Sum of corrected areas: 18541920

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120519\
Data File : VV013922.D
Acq On : 05 Dec 2019 18:01
Operator : SY/MD
Sample : K6170-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

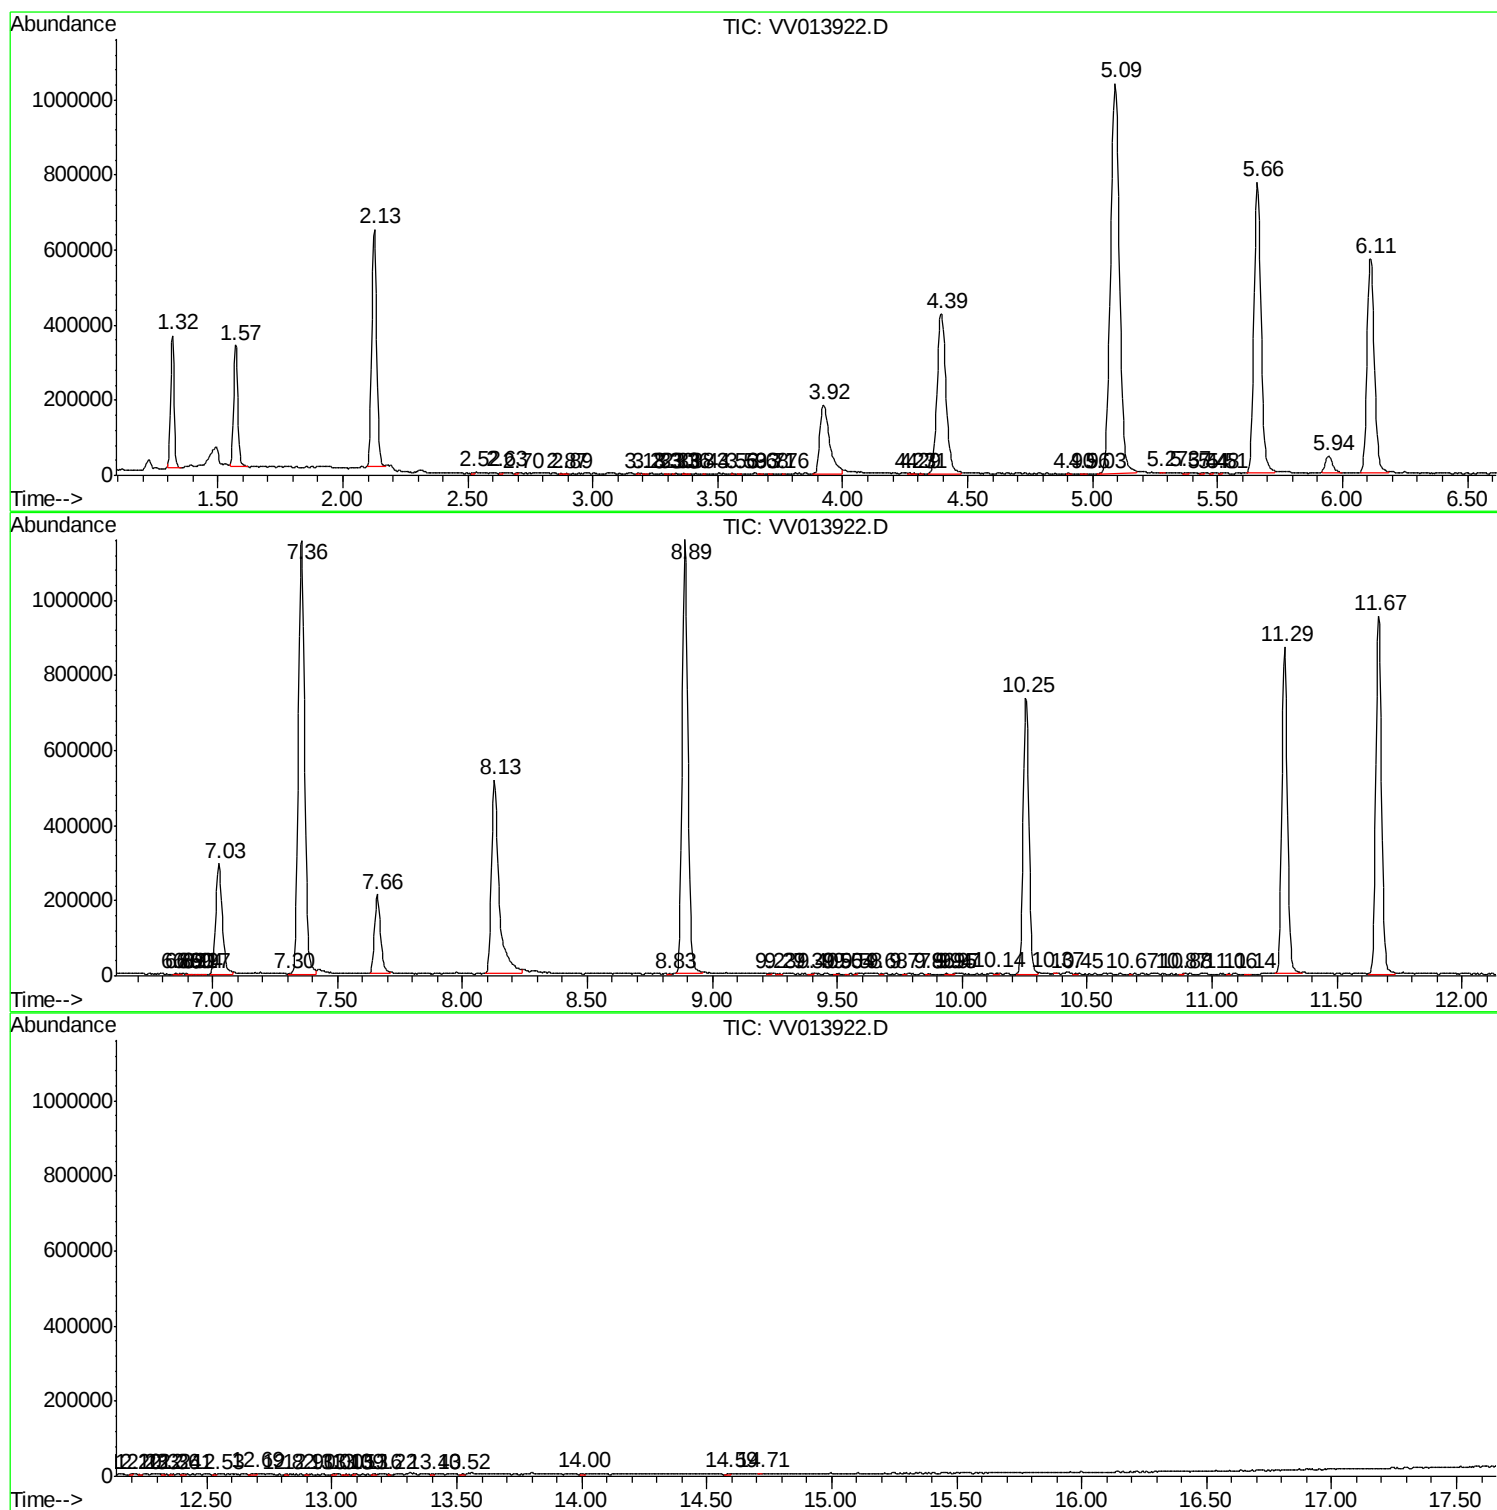

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120519\
Data File : VV013922.D
Acq On : 05 Dec 2019 18:01
Operator : SY/MD
Sample : K6170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120519\
Data File : VV013922.D
Acq On : 05 Dec 2019 18:01
Operator : SY/MD
Sample : K6170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc