

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013928.D
 Acq On : 05 Dec 2019 20:28
 Operator : SY/MD
 Sample : K6170-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	347047	337847	14.92%	2.103%
2	1.573	144	150	159	rVB	318789	359611	15.88%	2.239%
3	2.126	314	322	335	rVB	597573	849997	37.53%	5.291%
4	2.595	466	468	469	rBB2	1522	525	0.02%	0.003%
5	2.614	469	474	476	rBV5	1080	904	0.04%	0.006%
6	2.714	501	505	509	rVB5	1361	1169	0.05%	0.007%
7	2.833	539	542	547	rVB6	1795	1326	0.06%	0.008%
8	2.872	552	554	558	rVV3	1143	656	0.03%	0.004%
9	2.942	574	576	578	rBV3	1276	568	0.03%	0.004%
10	2.978	585	587	588	rBV2	949	337	0.01%	0.002%
11	3.045	604	608	609	rBV3	1756	1300	0.06%	0.008%
12	3.187	649	652	653	rBV3	721	370	0.02%	0.002%
13	3.232	664	666	669	rBV3	1134	875	0.04%	0.005%
14	3.309	688	690	692	rVB2	930	340	0.02%	0.002%
15	3.331	695	697	698	rBV2	594	215	0.01%	0.001%
16	3.399	716	718	723	rBV6	1738	1512	0.07%	0.009%
17	3.441	729	731	734	rVB3	812	450	0.02%	0.003%
18	3.463	736	738	741	rBV3	1092	697	0.03%	0.004%
19	3.499	747	749	753	rBV5	806	676	0.03%	0.004%
20	3.518	753	755	758	rVB3	1383	574	0.03%	0.004%
21	3.537	758	761	763	rBV3	966	602	0.03%	0.004%
22	3.556	765	767	769	rVB3	775	327	0.01%	0.002%
23	3.589	775	777	778	rVB2	959	345	0.02%	0.002%
24	3.598	778	780	786	rVB7	473	402	0.02%	0.003%
25	3.627	786	789	791	rBV3	1281	993	0.04%	0.006%
26	3.669	800	802	804	rBV2	813	317	0.01%	0.002%
27	3.704	810	813	816	rBV3	1389	964	0.04%	0.006%
28	3.746	823	826	828	rVB3	784	422	0.02%	0.003%
29	3.765	828	832	836	rBV4	1098	1133	0.05%	0.007%
30	3.794	839	841	844	rBV2	645	469	0.02%	0.003%
31	3.881	864	868	869	rBV3	1631	1043	0.05%	0.006%
32	3.920	870	880	907	rBV	155584	414544	18.30%	2.581%
33	4.228	973	976	979	rBV4	1320	971	0.04%	0.006%
34	4.261	985	986	988	rBV2	1097	390	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013928.D
 Acq On : 05 Dec 2019 20:28
 Operator : SY/MD
 Sample : K6170-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.396	1012	1028	1055	rBV	367178	897854	39.65%	5.589%
36	4.778	1143	1147	1151	rBV6	1459	1379	0.06%	0.009%
37	4.814	1156	1158	1160	rVB3	989	310	0.01%	0.002%
38	4.843	1164	1167	1172	rVB7	1538	1475	0.07%	0.009%
39	4.865	1172	1174	1175	rBV	1244	549	0.02%	0.003%
40	5.090	1226	1244	1276	rBV2	891446	2264698	100.00%	14.098%
41	5.659	1407	1421	1444	rBV	715358	1425680	62.95%	8.875%
42	6.113	1548	1562	1585	rBV	462012	938251	41.43%	5.841%
43	6.469	1671	1673	1675	rVB3	1676	633	0.03%	0.004%
44	6.486	1675	1678	1682	rBV4	1518	1277	0.06%	0.008%
45	6.531	1689	1692	1693	rBV3	771	418	0.02%	0.003%
46	6.556	1698	1700	1703	rVV4	1670	944	0.04%	0.006%
47	6.759	1760	1763	1764	rBV3	1169	543	0.02%	0.003%
48	6.833	1785	1786	1790	rVB4	1906	1047	0.05%	0.007%
49	6.855	1790	1793	1795	rBV2	1025	760	0.03%	0.005%
50	6.910	1808	1810	1811	rBV	1628	590	0.03%	0.004%
51	6.939	1816	1819	1821	rBV2	1186	772	0.03%	0.005%
52	6.961	1825	1826	1830	rVB3	1486	794	0.04%	0.005%
53	7.026	1834	1846	1872	rVV	237723	430855	19.02%	2.682%
54	7.354	1936	1948	1968	rBV	961824	1655039	73.08%	10.303%
55	7.659	2033	2043	2058	rBV	173744	290294	12.82%	1.807%
56	7.955	2132	2135	2136	rBV3	1801	1002	0.04%	0.006%
57	8.077	2171	2173	2176	rVB4	1600	914	0.04%	0.006%
58	8.125	2178	2188	2222	rBV2	436259	925732	40.88%	5.763%
59	8.891	2414	2426	2448	rBV	1043919	1704740	75.27%	10.612%
60	9.180	2512	2516	2517	rBV3	2481	1852	0.08%	0.012%
61	9.254	2537	2539	2542	rBV4	1824	1364	0.06%	0.008%
62	9.305	2551	2555	2557	rBV3	1368	852	0.04%	0.005%
63	9.431	2589	2594	2595	rBV3	1514	1150	0.05%	0.007%
64	9.524	2621	2623	2624	rBV2	990	392	0.02%	0.002%
65	9.836	2718	2720	2721	rBV2	1294	478	0.02%	0.003%
66	9.971	2757	2762	2764	rBV4	2791	2293	0.10%	0.014%
67	10.010	2772	2774	2775	rBV2	933	495	0.02%	0.003%
68	10.170	2821	2824	2829	rVB7	1407	1313	0.06%	0.008%
69	10.215	2836	2838	2839	rBV2	1115	486	0.02%	0.003%
70	10.254	2839	2850	2870	rVV	627358	992418	43.82%	6.178%
71	10.572	2947	2949	2952	rBV4	1214	746	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120519\
 Data File : VV013928.D
 Acq On : 05 Dec 2019 20:28
 Operator : SY/MD
 Sample : K6170-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.630	2963	2967	2969	rBV5	1226	977	0.04%	0.006%
73	10.675	2979	2981	2986	rBV3	917	665	0.03%	0.004%
74	10.710	2990	2992	2997	rBV5	1571	1542	0.07%	0.010%
75	10.810	3019	3023	3025	rBV4	1254	1104	0.05%	0.007%
76	10.842	3031	3033	3036	rBV3	751	490	0.02%	0.003%
77	10.865	3036	3040	3042	rBV2	2031	1388	0.06%	0.009%
78	10.955	3064	3068	3073	rBV7	2059	2164	0.10%	0.013%
79	10.977	3073	3075	3079	rVV4	1156	709	0.03%	0.004%
80	11.186	3133	3140	3141	rBV6	1578	1729	0.08%	0.011%
81	11.289	3160	3172	3191	rBV	768921	1215830	53.69%	7.569%
82	11.598	3265	3268	3274	rBV6	1594	1423	0.06%	0.009%
83	11.665	3278	3289	3304	rVV	816656	1287276	56.84%	8.013%
84	12.225	3460	3463	3465	rBV3	1446	1099	0.05%	0.007%
85	12.257	3471	3473	3477	rVB2	1329	778	0.03%	0.005%
86	12.308	3485	3489	3492	rBV5	1209	1006	0.04%	0.006%
87	12.453	3530	3534	3541	rBV9	1947	1969	0.09%	0.012%
88	12.482	3541	3543	3545	rVB4	1259	527	0.02%	0.003%
89	12.572	3569	3571	3576	rBV3	1019	586	0.03%	0.004%
90	12.604	3579	3581	3582	rBV2	877	413	0.02%	0.003%
91	12.659	3594	3598	3600	rBV4	1345	1175	0.05%	0.007%
92	12.739	3621	3623	3624	rBV2	1370	593	0.03%	0.004%
93	12.878	3664	3666	3668	rBV3	1180	734	0.03%	0.005%
94	12.948	3686	3688	3690	rBV3	891	543	0.02%	0.003%
95	13.032	3712	3714	3717	rBV3	1656	958	0.04%	0.006%
96	13.074	3722	3727	3730	rBV7	1380	1222	0.05%	0.008%
97	13.366	3815	3818	3819	rBV2	1634	1024	0.05%	0.006%
98	13.482	3851	3854	3856	rBV3	1323	841	0.04%	0.005%
99	13.897	3981	3983	3985	rBV3	1102	519	0.02%	0.003%
100	14.328	4114	4117	4119	rBV4	1787	1336	0.06%	0.008%


Sum of corrected areas: 16063880

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120519\
Data File : VV013928.D
Acq On : 05 Dec 2019 20:28
Operator : SY/MD
Sample : K6170-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

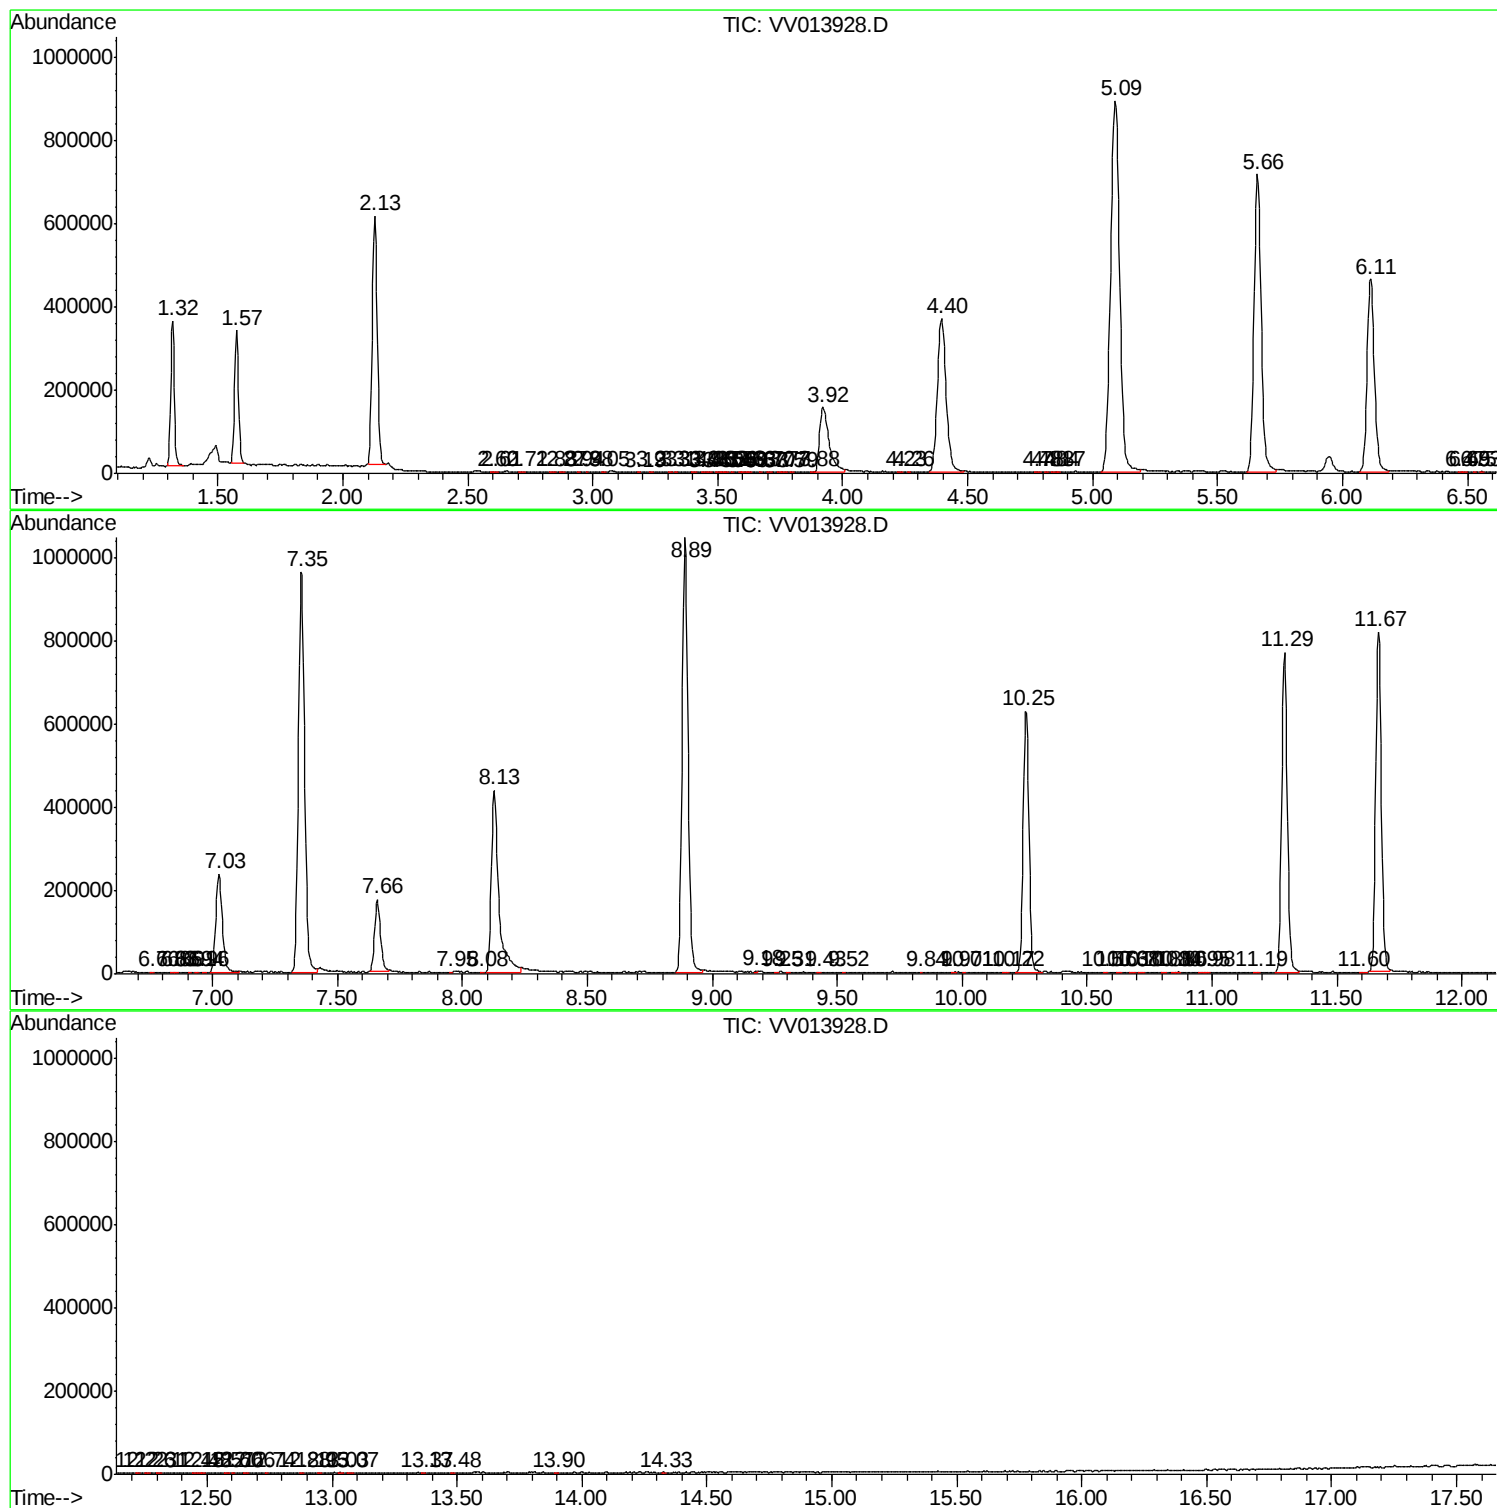

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120519\
Data File : VV013928.D
Acq On : 05 Dec 2019 20:28
Operator : SY/MD
Sample : K6170-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120519\
Data File : VV013928.D
Acq On : 05 Dec 2019 20:28
Operator : SY/MD
Sample : K6170-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc