


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120519\
 Data File : VV013908.D
 Acq On : 05 Dec 2019 09:40
 Operator : SY/MD
 Sample : BFB76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB76

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 06 10:04:43 2019

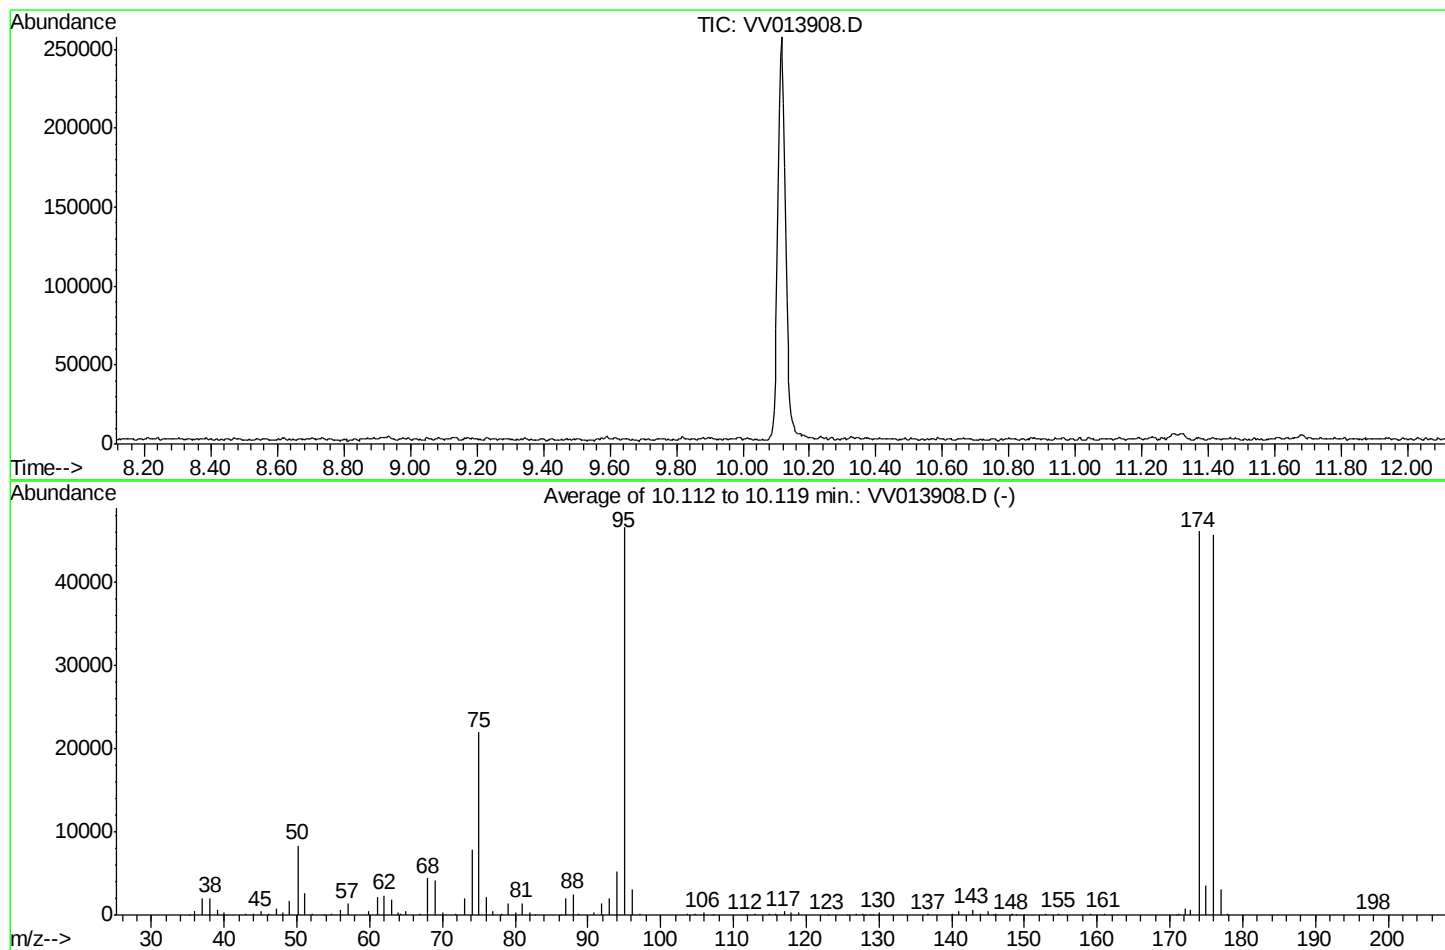

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	8351	PASS
75	95	30	80	47.2	21962	PASS
95	95	100	100	100.0	46517	PASS
96	95	5	9	6.7	3099	PASS
173	174	0.00	2	1.4	644	PASS
174	95	50	120	99.1	46112	PASS
175	174	5	9	7.7	3528	PASS
176	174	95	101	99.1	45698	PASS
177	176	5	9	6.8	3101	PASS

m/z	Abundance
36.00	734.0
37.00	2219.0
38.00	1970.0
39.10	742.0
39.90	968.0
42.90	151.0
44.10	916.0
45.00	483.0
46.20	127.0
47.10	671.0
48.00	355.0
49.00	1824.0
50.10	8510.0
51.00	2498.0
52.20	215.0
53.10	154.0
53.80	113.0
54.70	112.0
55.90	717.0
57.00	1501.0
59.90	531.0
61.00	2152.0
62.00	2386.0
63.10	1614.0
63.90	226.0
64.20	270.0
65.00	504.0
66.80	143.0
68.00	4407.0
69.00	4411.0
70.10	421.0
71.90	227.0
73.00	1993.0
74.10	7563.0
75.00	21912.0
76.10	2071.0
76.90	337.0
78.10	349.0
79.00	1375.0
80.10	293.0
81.00	1375.0
81.90	269.0
82.70	143.0
83.70	113.0
87.00	2404.0
88.00	2416.0
90.80	261.0
91.90	1169.0
93.00	1905.0
94.10	5112.0
95.00	45216.0
96.10	3150.0
97.20	129.0
103.80	152.0
104.80	117.0
105.80	266.0
111.70	112.0
112.90	157.0
114.90	172.0
115.80	241.0
117.00	431.0
117.90	259.0
118.90	361.0
123.00	139.0
126.90	129.0
128.10	192.0
128.90	144.0
130.00	207.0
140.00	215.0
140.90	578.0
142.80	570.0
143.90	147.0
145.00	480.0
148.10	141.0
149.90	107.0
153.00	109.0
154.70	231.0
159.10	111.0
161.00	159.0
171.30	305.0
172.00	547.0
172.80	577.0
174.00	44584.0
175.00	3385.0
176.00	45280.0
177.00	2905.0
177.90	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.00	678.0
37.00	2130.0
38.00	2096.0
39.10	736.0
39.90	895.0
42.90	158.0
44.10	841.0
45.00	441.0
46.00	135.0
47.10	797.0
48.10	368.0
49.00	1766.0
50.10	8899.0
51.00	2616.0
52.20	245.0
53.00	102.0
53.70	107.0
54.80	149.0
56.00	636.0
57.00	1470.0
59.90	473.0
61.00	2187.0
62.00	2445.0
63.10	1836.0
63.80	244.0
64.20	230.0
65.00	543.0
66.90	126.0
68.00	4596.0
69.00	4351.0
70.10	331.0
71.90	237.0
73.00	2125.0
74.10	8113.0
75.00	22496.0
76.10	2335.0
76.90	411.0
78.10	281.0
79.00	1499.0
80.10	344.0
80.90	1469.0
81.90	268.0
83.70	114.0
86.90	2098.0
88.00	2697.0
88.70	161.0
90.80	306.0
92.00	1355.0
93.00	2176.0
94.00	5397.0
95.00	47688.0
96.00	3174.0
97.20	173.0
103.70	189.0
104.80	136.0
105.90	269.0
107.10	118.0
112.90	104.0
114.90	118.0
115.80	230.0
117.00	412.0
117.90	260.0
118.90	413.0
125.70	104.0
126.90	144.0
127.80	263.0
130.00	238.0
136.70	122.0
140.00	102.0
140.90	555.0
142.90	650.0
143.90	199.0
145.00	507.0
145.70	107.0
146.10	109.0
148.30	154.0
148.80	117.0
152.90	151.0
154.70	205.0
159.00	118.0
161.00	192.0
171.30	344.0
172.10	743.0
172.80	670.0
174.00	47664.0
175.00	3673.0
176.00	47272.0
177.00	3181.0
177.90	187.0
198.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.20	133.0
36.00	533.0
37.10	1825.0
38.10	2123.0
39.00	717.0
39.90	833.0
42.90	118.0
44.00	737.0
45.00	372.0
46.00	184.0
47.10	721.0
48.10	332.0
49.00	1574.0
50.10	8054.0
51.00	2616.0
52.20	219.0
54.80	183.0
56.00	560.0
57.00	1152.0
59.90	403.0
61.00	2135.0
62.00	2167.0
63.00	1935.0
63.90	298.0
65.00	544.0
68.00	4169.0
69.10	3860.0
70.00	269.0
71.90	240.0
73.00	2075.0
74.10	7723.0
75.00	21480.0
76.10	2517.0
77.00	490.0
78.90	1381.0
79.90	413.0
80.90	1344.0
82.00	308.0
86.20	213.0
87.00	1718.0
87.90	2429.0
88.80	180.0
90.90	294.0
92.00	1547.0
93.00	2068.0
94.00	5225.0
95.00	46648.0
96.00	2975.0
97.10	212.0
103.70	196.0
106.00	280.0
107.20	112.0
115.90	178.0
117.00	332.0
117.90	221.0
118.90	345.0
127.80	306.0
129.20	101.0
130.00	264.0
136.80	150.0
140.90	490.0
143.00	680.0
144.00	163.0
145.00	495.0
145.80	132.0
146.20	143.0
148.30	155.0
148.90	111.0
152.90	156.0
154.80	145.0
158.90	157.0
160.90	191.0
170.90	224.0
172.10	844.0
172.80	687.0
174.00	46088.0
175.00	3526.0
176.00	44544.0
177.00	3219.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
36.20	145.0
39.20	154.0
39.90	659.0
41.70	186.0
42.30	108.0
44.00	653.0
47.70	112.0
50.10	136.0
51.70	107.0
52.90	107.0
68.80	123.0
70.90	154.0
71.90	105.0
73.20	114.0
75.90	101.0
83.50	115.0
157.30	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76