

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
 Data File : VV029396.D
 Acq On : 05 Dec 2022 11:07
 Operator : SY/MD
 Sample : VV1205WBL04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK283

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	117256	119823	18.46%	2.148%
2	1.564	156	163	175	rVB	88007	98011	15.10%	1.757%
3	2.105	316	331	350	rBV	165588	240148	36.99%	4.304%
4	2.507	446	456	464	rVB	5744	9180	1.41%	0.165%
5	3.905	879	891	928	rBV2	38649	144960	22.33%	2.598%
6	4.342	1010	1027	1053	rBV	106298	269229	41.47%	4.825%
7	5.040	1227	1244	1275	rBV2	256611	648200	99.85%	11.618%
8	5.609	1409	1421	1460	rBV	253593	525967	81.02%	9.427%
9	6.063	1548	1562	1583	rBV	144805	299385	46.12%	5.366%
10	6.982	1837	1848	1867	rBV	74946	142738	21.99%	2.558%
11	7.310	1936	1950	1979	rBV	331128	593680	91.46%	10.640%
12	7.616	2033	2045	2065	rBV	42773	78368	12.07%	1.405%
13	8.085	2180	2191	2222	rBV	235997	465739	71.75%	8.347%
14	8.844	2414	2427	2452	rBV	366849	610252	94.01%	10.937%
15	10.207	2838	2851	2865	rBV	101490	157195	24.22%	2.817%
16	11.239	3161	3172	3196	rBV	419635	649148	100.00%	11.635%
17	11.615	3276	3289	3310	rBV	304201	491781	75.76%	8.814%
18	12.242	3475	3484	3494	rVB2	7961	12415	1.91%	0.223%
19	13.493	3863	3873	3886	rVB2	5456	8794	1.35%	0.158%
20	14.033	4033	4041	4050	rVB2	4999	7610	1.17%	0.136%
21	15.760	4574	4578	4589	rVB8	4949	6869	1.06%	0.123%




Sum of corrected areas: 5579492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
Data File : VV029396.D
Acq On : 05 Dec 2022 11:07
Operator : SY/MD
Sample : VV1205WBL04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK283

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

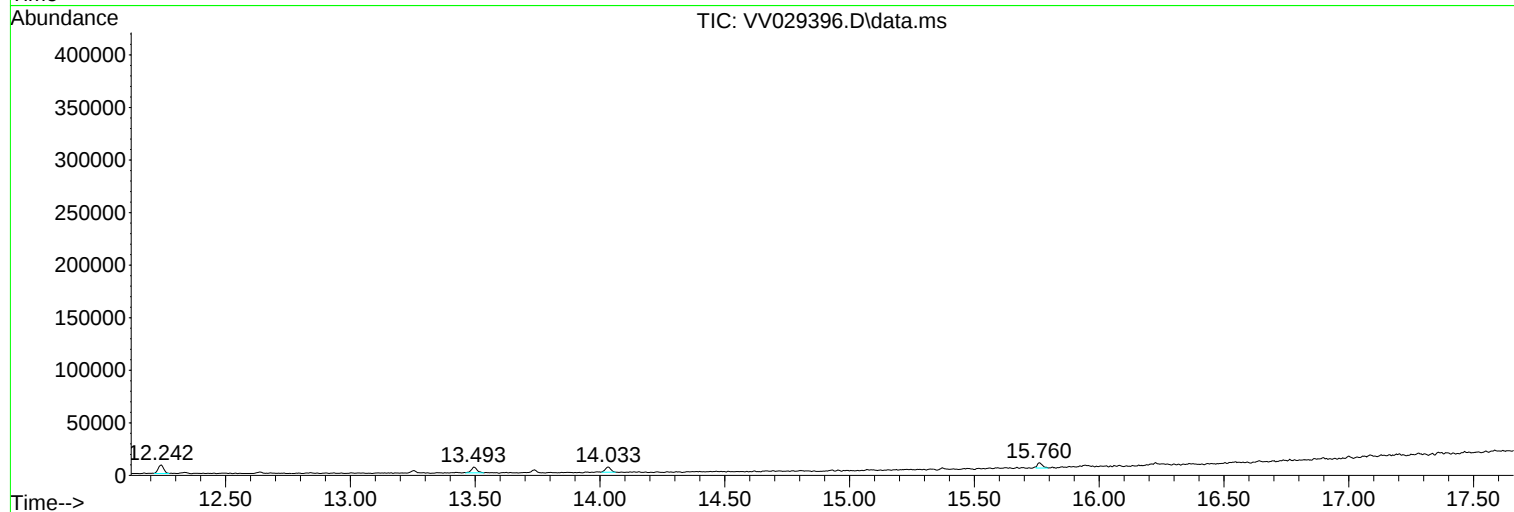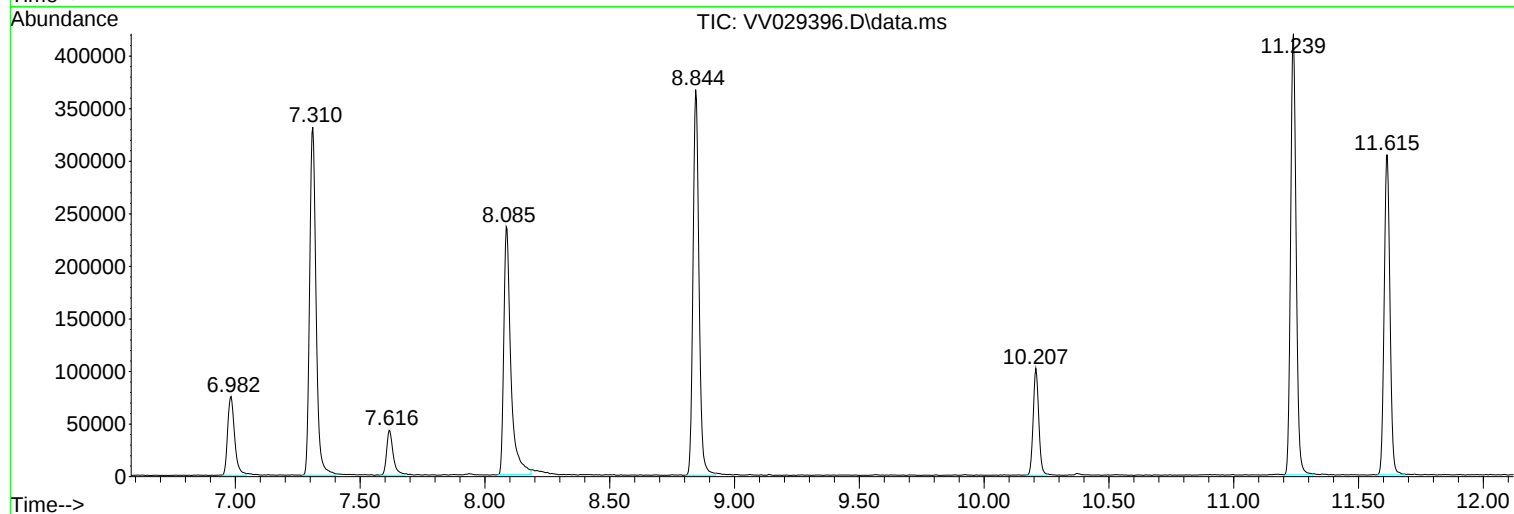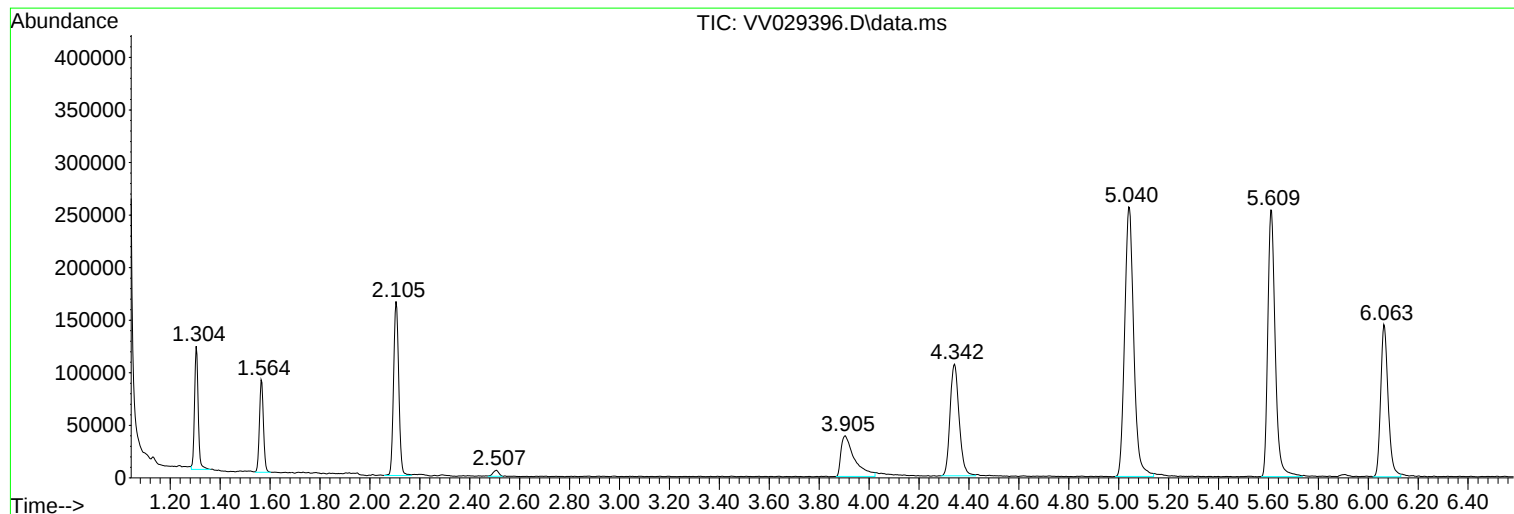

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
Data File : VV029396.D
Acq On : 05 Dec 2022 11:07
Operator : SY/MD
Sample : VV1205WBL04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK283

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
Data File : VV029396.D
Acq On : 05 Dec 2022 11:07
Operator : SY/MD
Sample : VV1205WBL04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK283

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc