

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
 Data File : VV029397.D
 Acq On : 05 Dec 2022 11:31
 Operator : SY/MD
 Sample : VV1205WBL05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK284

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	118126	119785	18.70%	2.185%
2	1.565	156	163	175	rVB	86779	95880	14.97%	1.749%
3	2.105	320	331	347	rBV	165191	234143	36.55%	4.270%
4	2.503	446	455	467	rVB2	5732	10261	1.60%	0.187%
5	3.905	875	891	924	rBV2	34495	137610	21.48%	2.510%
6	4.343	1010	1027	1057	rBV	107973	268770	41.95%	4.902%
7	5.043	1228	1245	1275	rBV2	254713	640683	100.00%	11.684%
8	5.609	1409	1421	1449	rBV	248770	513025	80.07%	9.356%
9	6.063	1549	1562	1599	rBV	141886	295832	46.17%	5.395%
10	6.982	1837	1848	1873	rBV	73669	139746	21.81%	2.549%
11	7.310	1937	1950	1978	rBV	322009	584220	91.19%	10.654%
12	7.616	2034	2045	2066	rBV	41942	76448	11.93%	1.394%
13	8.088	2181	2192	2223	rBV	228737	466052	72.74%	8.499%
14	8.844	2412	2427	2458	rBV	362350	605557	94.52%	11.043%
15	10.207	2840	2851	2870	rBV	95923	153542	23.97%	2.800%
16	11.239	3160	3172	3202	rBV	407058	639617	99.83%	11.665%
17	11.616	3275	3289	3304	rBV	305235	482861	75.37%	8.806%
18	12.243	3473	3484	3494	rVB2	6990	11539	1.80%	0.210%
19	14.030	4030	4040	4049	rBV	5330	7826	1.22%	0.143%




Sum of corrected areas: 5483397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
Data File : VV029397.D
Acq On : 05 Dec 2022 11:31
Operator : SY/MD
Sample : VV1205WBL05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK284

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

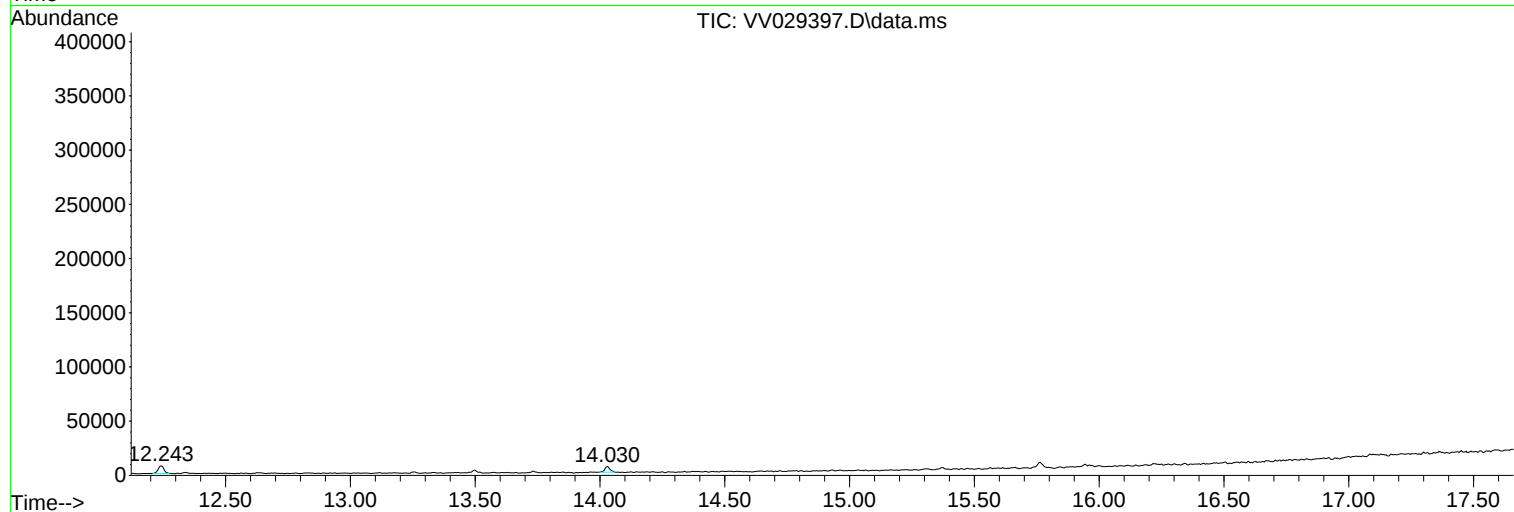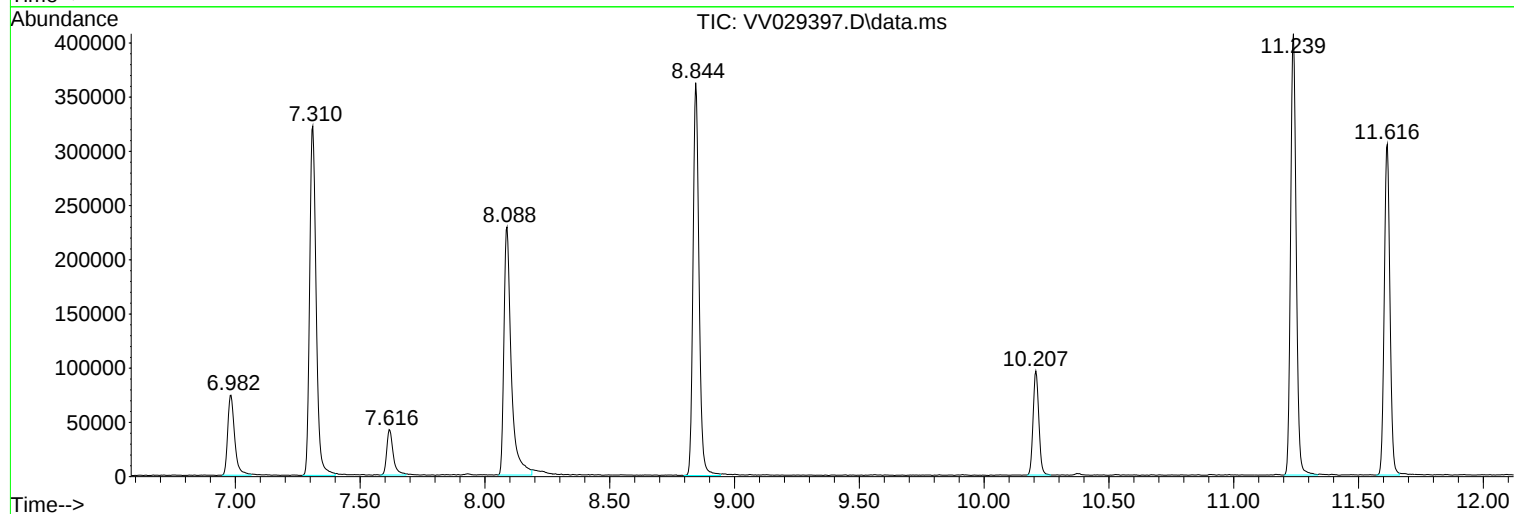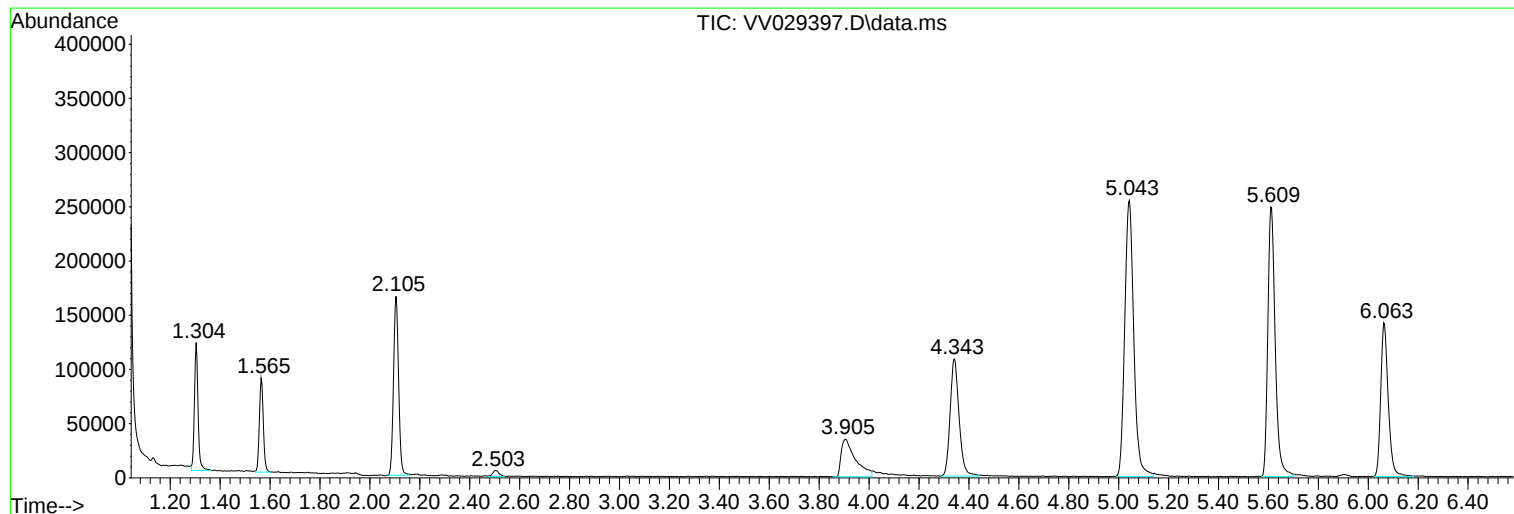

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
Data File : VV029397.D
Acq On : 05 Dec 2022 11:31
Operator : SY/MD
Sample : VV1205WBL05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK284

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120522\
Data File : VV029397.D
Acq On : 05 Dec 2022 11:31
Operator : SY/MD
Sample : VV1205WBL05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK284

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc