

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
 Data File : VV033102.D
 Acq On : 05 Dec 2023 11:44
 Operator : SY/MD
 Sample : VV1205MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	138133	149890	14.24%	1.702%
2	1.420	110	118	130	rBV4	5439	9312	0.88%	0.106%
3	1.532	145	153	164	rBV	102972	119029	11.31%	1.351%
4	1.645	186	188	192	rVV	789	653	0.06%	0.007%
5	1.664	192	194	197	rVV	1520	822	0.08%	0.009%
6	1.706	202	207	215	rVB4	1563	2087	0.20%	0.024%
7	1.777	225	229	232	rVB3	1580	1017	0.10%	0.012%
8	1.822	240	243	246	rVB	1461	945	0.09%	0.011%
9	1.873	253	259	260	rBV2	1159	1126	0.11%	0.013%
10	1.883	260	262	265	rVV	1317	1093	0.10%	0.012%
11	1.921	269	274	279	rVB2	1532	1587	0.15%	0.018%
12	1.998	294	298	300	rBV	1399	760	0.07%	0.009%
13	2.060	306	317	333	rBV	211084	312811	29.72%	3.551%
14	2.162	341	349	352	rBV	3741	5578	0.53%	0.063%
15	2.182	352	355	357	rBV	1581	1119	0.11%	0.013%
16	2.201	358	361	366	rBV	1382	1420	0.13%	0.016%
17	2.227	367	369	371	rBV	1593	1038	0.10%	0.012%
18	2.709	517	519	522	rBV2	1260	689	0.07%	0.008%
19	2.822	551	554	556	rBV	1422	1125	0.11%	0.013%
20	2.986	603	605	609	rBV2	1305	900	0.09%	0.010%
21	3.082	631	635	639	rBV	2442	2512	0.24%	0.029%
22	3.365	718	723	728	rBV	2031	2859	0.27%	0.032%
23	3.458	747	752	756	rBV	1973	2145	0.20%	0.024%
24	3.777	843	851	879	rBV	62763	162416	15.43%	1.844%
25	4.121	955	958	963	rBV2	1947	1824	0.17%	0.021%
26	4.246	982	997	1019	rBV	178452	450524	42.81%	5.114%
27	4.375	1034	1037	1039	rBV2	1842	1288	0.12%	0.015%
28	4.455	1059	1062	1066	rBV3	2006	1706	0.16%	0.019%
29	4.629	1113	1116	1122	rVB	2471	1755	0.17%	0.020%
30	4.683	1130	1133	1134	rBV2	1577	985	0.09%	0.011%
31	4.953	1201	1217	1250	rBV2	394233	1052396	100.00%	11.947%
32	5.445	1367	1370	1371	rBV	1130	710	0.07%	0.008%
33	5.532	1385	1397	1417	rBV	377354	766339	72.82%	8.700%
34	5.757	1464	1467	1471	rVB	1769	1257	0.12%	0.014%
35	5.783	1472	1475	1478	rBV	1997	1618	0.15%	0.018%
36	5.828	1483	1489	1502	rVB5	9294	18648	1.77%	0.212%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
 Data File : VV033102.D
 Acq On : 05 Dec 2023 11:44
 Operator : SY/MD
 Sample : VV1205MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.985	1527	1538	1560	rBV	221359	453093	43.05%	5.144%
38	6.268	1624	1626	1629	rVB2	1654	816	0.08%	0.009%
39	6.329	1643	1645	1650	rBV	1106	1008	0.10%	0.011%
40	6.455	1681	1684	1687	rBV	1781	1135	0.11%	0.013%
41	6.792	1787	1789	1792	rBV	1119	692	0.07%	0.008%
42	6.911	1816	1826	1850	rBV	130706	247242	23.49%	2.807%
43	7.172	1901	1907	1911	rBV2	2210	2743	0.26%	0.031%
44	7.243	1918	1929	1953	rBV	491998	859998	81.72%	9.763%
45	7.551	2016	2025	2039	rBV2	97829	171535	16.30%	1.947%
46	8.021	2162	2171	2193	rBV	223127	406322	38.61%	4.613%
47	8.355	2272	2275	2277	rBV	1990	1424	0.14%	0.016%
48	8.384	2281	2284	2286	rBV	2014	1417	0.13%	0.016%
49	8.529	2326	2329	2333	rBV2	2594	2365	0.22%	0.027%
50	8.587	2344	2347	2352	rBV	1706	1373	0.13%	0.016%
51	8.783	2397	2408	2429	rBV	592773	966859	91.87%	10.976%
52	8.956	2460	2462	2465	rBV	1547	802	0.08%	0.009%
53	9.191	2529	2535	2538	rBV	1748	2315	0.22%	0.026%
54	9.487	2622	2627	2630	rBV2	1573	1795	0.17%	0.020%
55	9.619	2665	2668	2672	rVB	1799	1196	0.11%	0.014%
56	9.699	2691	2693	2698	rVB	1851	1293	0.12%	0.015%
57	9.728	2698	2702	2704	rBV	1902	1706	0.16%	0.019%
58	9.866	2743	2745	2749	rBV2	1201	979	0.09%	0.011%
59	9.908	2755	2758	2761	rBV	1379	1049	0.10%	0.012%
60	9.998	2782	2786	2789	rBV	2160	1922	0.18%	0.022%
61	10.152	2823	2834	2849	rBV	320100	505042	47.99%	5.733%
62	10.435	2919	2922	2927	rVB3	1143	1129	0.11%	0.013%
63	10.767	3023	3025	3028	rVB	2056	1136	0.11%	0.013%
64	10.789	3029	3032	3033	rBV	1124	697	0.07%	0.008%
65	10.863	3053	3055	3057	rBV2	1293	709	0.07%	0.008%
66	10.940	3076	3079	3082	rBV	1355	1136	0.11%	0.013%
67	11.005	3096	3099	3102	rBV	1112	788	0.07%	0.009%
68	11.185	3144	3155	3173	rBV	679797	1026456	97.54%	11.653%
69	11.561	3259	3272	3288	rBV	592699	930111	88.38%	10.559%
70	11.969	3397	3399	3402	rVB	1576	791	0.08%	0.009%
71	12.059	3424	3427	3431	rVB	1588	1198	0.11%	0.014%
72	12.088	3432	3436	3439	rBV2	1567	1518	0.14%	0.017%
73	12.323	3507	3509	3514	rVB	2404	1753	0.17%	0.020%
74	12.583	3585	3590	3593	rBV3	3308	3835	0.36%	0.044%
75	12.882	3680	3683	3684	rBV2	1874	1006	0.10%	0.011%
76	12.985	3713	3715	3718	rVB	1287	688	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
 Data File : VV033102.D
 Acq On : 05 Dec 2023 11:44
 Operator : SY/MD
 Sample : VV1205MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.204	3776	3783	3797	rBV3	9311	16039	1.52%	0.182%
78	13.300	3811	3813	3816	rBV	1379	754	0.07%	0.009%
79	13.394	3839	3842	3846	rVB	1830	1394	0.13%	0.016%
80	13.445	3849	3858	3872	rVB	31005	51016	4.85%	0.579%
81	13.503	3872	3876	3879	rBV	1660	1352	0.13%	0.015%
82	13.580	3897	3900	3904	rVB2	1673	1242	0.12%	0.014%
83	13.603	3904	3907	3915	rBV2	1718	2708	0.26%	0.031%
84	13.683	3927	3932	3943	rVB	12305	18615	1.77%	0.211%
85	13.747	3948	3952	3959	rBV	1420	2103	0.20%	0.024%
86	13.786	3961	3964	3967	rVV	1605	1329	0.13%	0.015%
87	13.805	3967	3970	3973	rVB	1482	901	0.09%	0.010%
88	13.889	3993	3996	3999	rBV	1213	741	0.07%	0.008%
89	14.149	4074	4077	4082	rBV	1591	1792	0.17%	0.020%
90	14.345	4135	4138	4141	rVB	2015	1363	0.13%	0.015%
91	14.516	4188	4191	4194	rBV	2189	1645	0.16%	0.019%
92	14.554	4200	4203	4205	rBV3	1306	929	0.09%	0.011%
93	14.686	4241	4244	4248	rVB	2238	1550	0.15%	0.018%
94	14.709	4249	4251	4253	rBV	1301	725	0.07%	0.008%
95	14.966	4327	4331	4335	rBV3	1513	1691	0.16%	0.019%
96	15.094	4368	4371	4373	rBV2	1599	1062	0.10%	0.012%
97	15.155	4387	4390	4396	rVB2	1295	1202	0.11%	0.014%
98	16.490	4802	4805	4807	rBV3	2106	1576	0.15%	0.018%
99	16.625	4844	4847	4850	rBV	2862	2255	0.21%	0.026%
100	17.091	4989	4992	5000	rBV	2725	3735	0.35%	0.042%




Sum of corrected areas: 8808774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033102.D
Acq On : 05 Dec 2023 11:44
Operator : SY/MD
Sample : VV1205MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

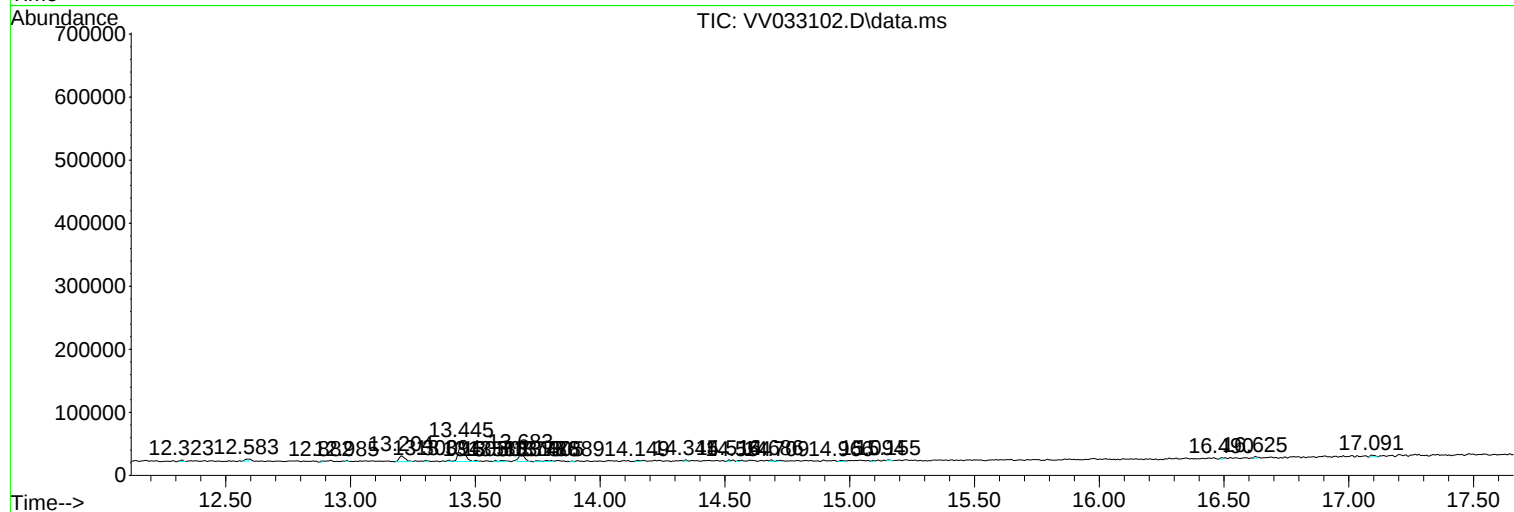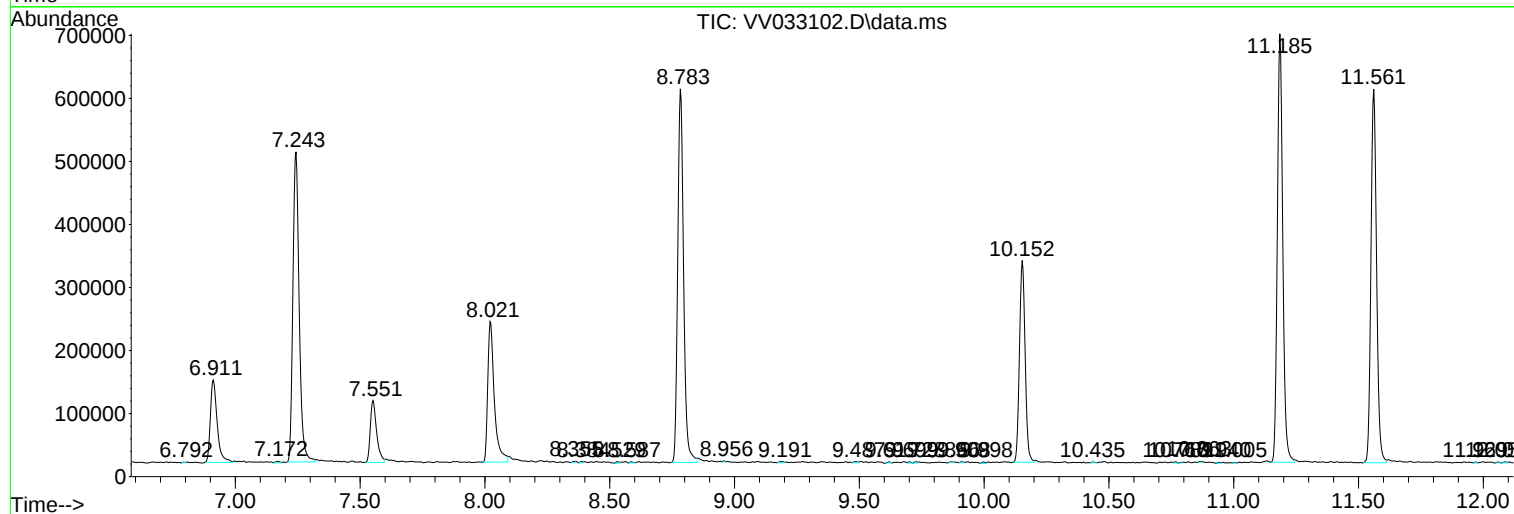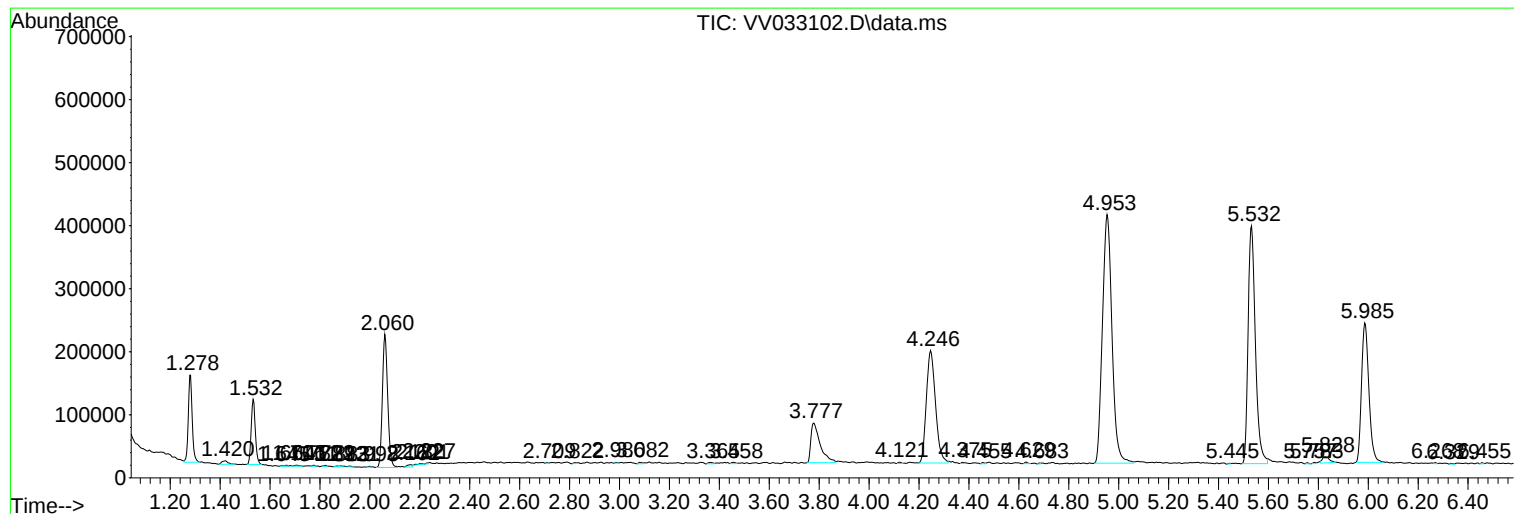

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033102.D
Acq On : 05 Dec 2023 11:44
Operator : SY/MD
Sample : VV1205MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033102.D
Acq On : 05 Dec 2023 11:44
Operator : SY/MD
Sample : VV1205MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc