

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
 Data File : VV033103.D
 Acq On : 05 Dec 2023 12:08
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rVB	131508	139691	13.71%	1.651%
2	1.423	112	119	126	rVB2	5955	8248	0.81%	0.097%
3	1.491	138	140	144	rVB2	2049	1185	0.12%	0.014%
4	1.536	145	154	168	rVB	97848	118940	11.68%	1.406%
5	1.590	168	171	175	rBV3	1184	1116	0.11%	0.013%
6	1.606	175	176	180	rVB	1018	528	0.05%	0.006%
7	1.639	180	186	188	rBV3	944	757	0.07%	0.009%
8	1.651	188	190	193	rVB	1369	666	0.07%	0.008%
9	1.671	193	196	200	rVB	755	544	0.05%	0.006%
10	1.696	200	204	206	rBV3	781	633	0.06%	0.007%
11	1.709	206	208	210	rBV	651	274	0.03%	0.003%
12	1.722	210	212	214	rBV2	1328	789	0.08%	0.009%
13	1.770	224	227	233	rBV2	1541	1524	0.15%	0.018%
14	1.803	233	237	241	rVB3	848	803	0.08%	0.009%
15	1.822	241	243	247	rVB	1063	583	0.06%	0.007%
16	1.841	247	249	252	rBV2	1235	806	0.08%	0.010%
17	1.867	252	257	259	rBV2	1000	849	0.08%	0.010%
18	1.893	264	265	269	rVB3	586	356	0.03%	0.004%
19	1.925	273	275	279	rVB	1086	758	0.07%	0.009%
20	1.957	283	285	287	rBV	292	114	0.01%	0.001%
21	1.989	291	295	301	rBV	1547	1480	0.15%	0.017%
22	2.063	301	318	332	rBV	194440	290678	28.54%	3.436%
23	2.140	337	342	344	rBV	2100	2082	0.20%	0.025%
24	2.156	344	347	349	rBV	1047	768	0.08%	0.009%
25	2.188	350	357	358	rBV	2139	2552	0.25%	0.030%
26	2.304	388	393	396	rBV	2043	2182	0.21%	0.026%
27	2.417	423	428	432	rBV2	1725	2055	0.20%	0.024%
28	2.870	566	569	572	rBV	1745	1129	0.11%	0.013%
29	3.365	720	723	725	rBV	1604	1188	0.12%	0.014%
30	3.783	844	853	877	rBV	62109	165137	16.21%	1.952%
31	4.121	955	958	961	rBV	2734	2187	0.21%	0.026%
32	4.249	983	998	1030	rVB2	170329	437408	42.94%	5.170%
33	4.690	1133	1135	1138	rBV	1255	957	0.09%	0.011%
34	4.799	1166	1169	1173	rBV2	1695	1277	0.13%	0.015%
35	4.957	1202	1218	1247	rBV2	377936	1018644	100.00%	12.039%
36	5.072	1252	1254	1257	rBV2	1655	1298	0.13%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
 Data File : VV033103.D
 Acq On : 05 Dec 2023 12:08
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.391	1350	1353	1358	rBV2	1507	1799	0.18%	0.021%
38	5.471	1375	1378	1381	rBV	1494	932	0.09%	0.011%
39	5.532	1387	1397	1419	rBV	358631	734861	72.14%	8.685%
40	5.777	1471	1473	1476	rVB	1624	885	0.09%	0.010%
41	5.828	1482	1489	1505	rVB6	9999	20404	2.00%	0.241%
42	5.989	1527	1539	1559	rBV	215518	446346	43.82%	5.275%
43	6.912	1817	1826	1841	rBV	127012	231974	22.77%	2.742%
44	7.079	1874	1878	1881	rBV	2194	1767	0.17%	0.021%
45	7.243	1919	1929	1954	rBV	473846	831889	81.67%	9.832%
46	7.551	2017	2025	2043	rBV	92512	162262	15.93%	1.918%
47	8.024	2163	2172	2197	rBV	217048	402061	39.47%	4.752%
48	8.140	2206	2208	2213	rVB2	2918	1881	0.18%	0.022%
49	8.442	2299	2302	2303	rBV2	1275	738	0.07%	0.009%
50	8.783	2398	2408	2431	rBV	571144	936554	91.94%	11.069%
51	9.153	2520	2523	2526	rBV	1438	895	0.09%	0.011%
52	9.529	2637	2640	2641	rBV	1525	875	0.09%	0.010%
53	10.082	2808	2812	2816	rBV	2082	2094	0.21%	0.025%
54	10.153	2823	2834	2854	rBV	308790	495640	48.66%	5.858%
55	10.899	3062	3066	3069	rBV	1873	1814	0.18%	0.021%
56	10.998	3094	3097	3104	rVB	1607	1626	0.16%	0.019%
57	11.085	3121	3124	3127	rBV	1884	1210	0.12%	0.014%
58	11.117	3132	3134	3138	rBV2	1474	1064	0.10%	0.013%
59	11.185	3144	3155	3179	rBV	652981	1003936	98.56%	11.865%
60	11.477	3243	3246	3248	rBV	1334	904	0.09%	0.011%
61	11.561	3261	3272	3291	rBV	599249	917978	90.12%	10.850%
62	12.120	3442	3446	3450	rBV	1979	1921	0.19%	0.023%
63	12.169	3459	3461	3465	rBV	1690	1276	0.13%	0.015%
64	12.255	3485	3488	3493	rBV	2013	1997	0.20%	0.024%
65	12.419	3535	3539	3542	rBV	1497	1445	0.14%	0.017%
66	12.506	3563	3566	3572	rVB	2141	1693	0.17%	0.020%
67	12.577	3583	3588	3590	rBV	1908	2034	0.20%	0.024%
68	12.699	3622	3626	3633	rVB	1731	1905	0.19%	0.023%
69	13.207	3780	3784	3793	rVB2	4214	5440	0.53%	0.064%
70	13.448	3852	3859	3868	rBV2	7278	11118	1.09%	0.131%
71	13.625	3911	3914	3916	rBV	2187	1610	0.16%	0.019%
72	13.654	3920	3923	3927	rVV2	1658	1546	0.15%	0.018%
73	13.757	3953	3955	3957	rBV	1412	832	0.08%	0.010%
74	14.043	4042	4044	4051	rVB	1849	1535	0.15%	0.018%
75	14.072	4051	4053	4055	rBV	1458	803	0.08%	0.009%
76	14.484	4179	4181	4184	rBV	1199	803	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033103.D
Acq On : 05 Dec 2023 12:08
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis

77	14.934	4317	4321	4324	rBV2	2058	1601	0.16%	0.019%
78	15.288	4427	4431	4435	rBV	2359	2719	0.27%	0.032%
79	15.796	4584	4589	4591	rBV	2862	2771	0.27%	0.033%
80	15.882	4610	4616	4619	rBV3	1989	2718	0.27%	0.032%
81	15.934	4629	4632	4636	rBV	1627	1621	0.16%	0.019%
82	16.053	4667	4669	4672	rBV	1895	1015	0.10%	0.012%




Sum of corrected areas: 8460978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033103.D
Acq On : 05 Dec 2023 12:08
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

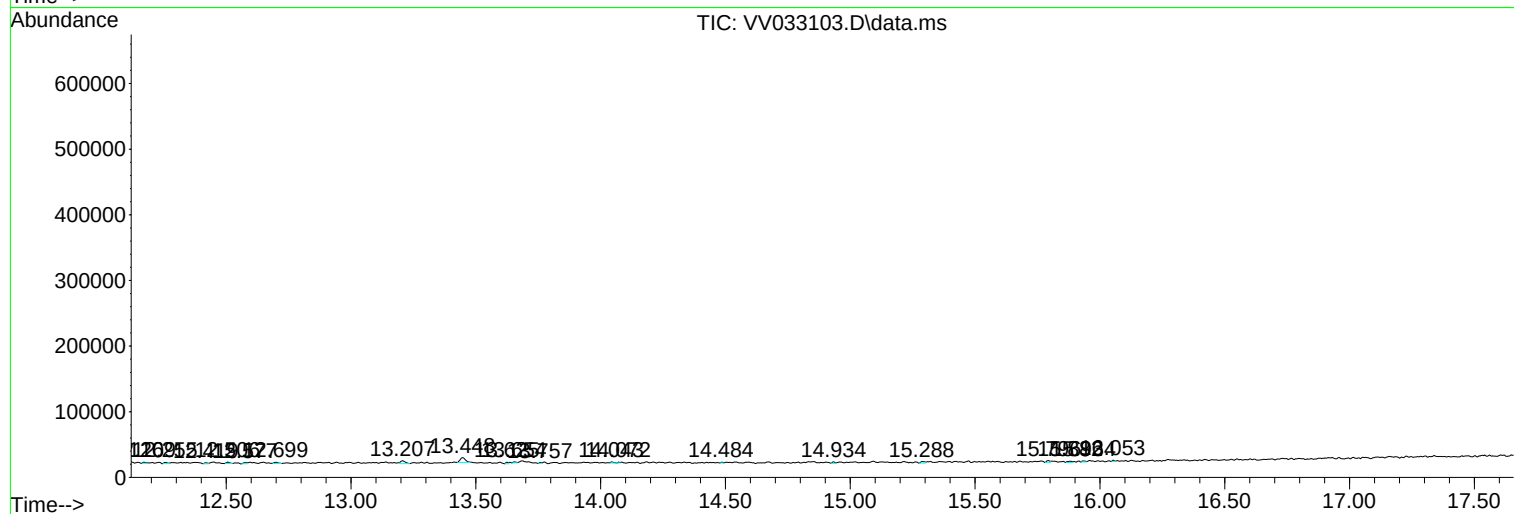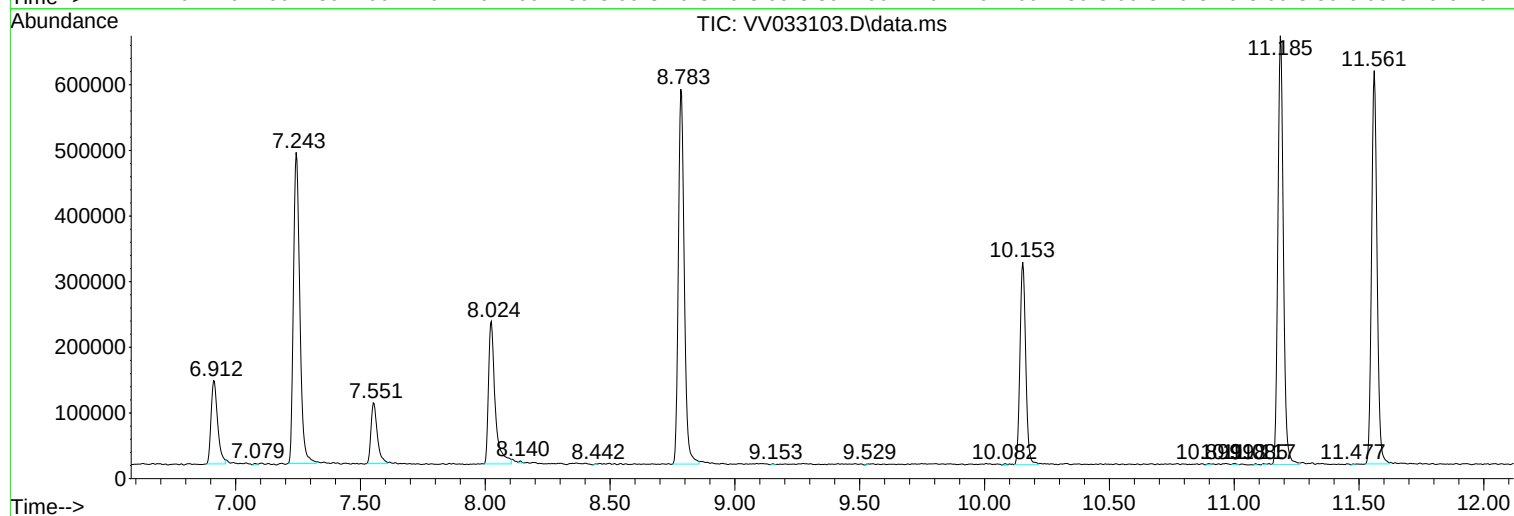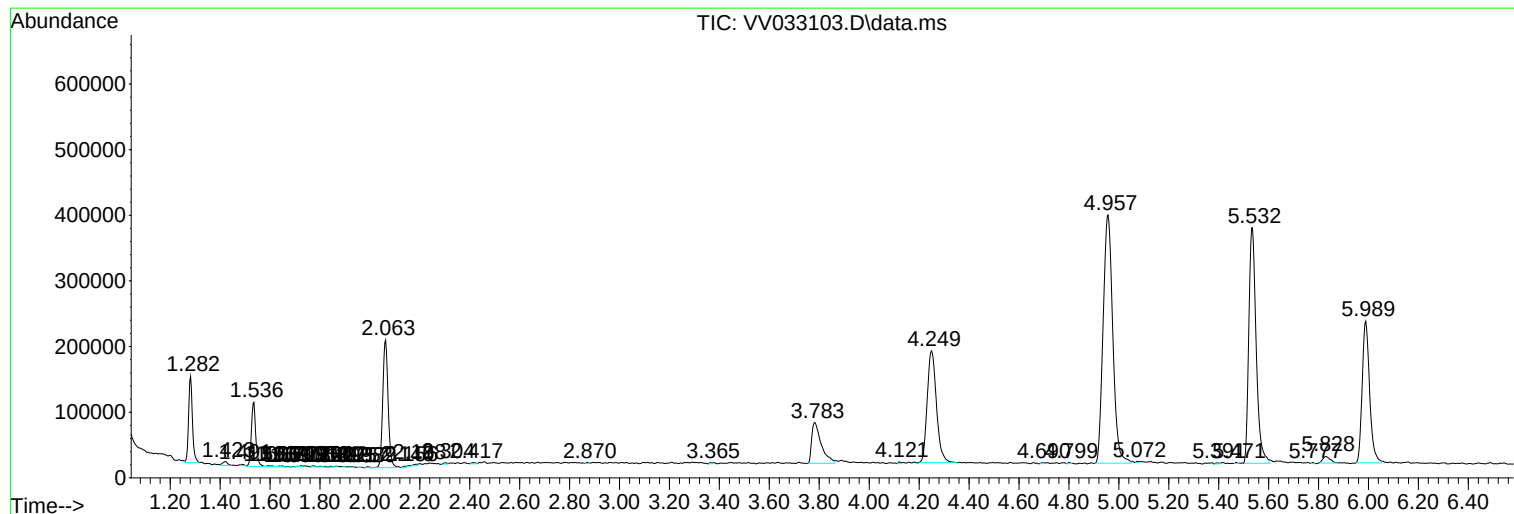

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033103.D
Acq On : 05 Dec 2023 12:08
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033103.D
Acq On : 05 Dec 2023 12:08
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------