
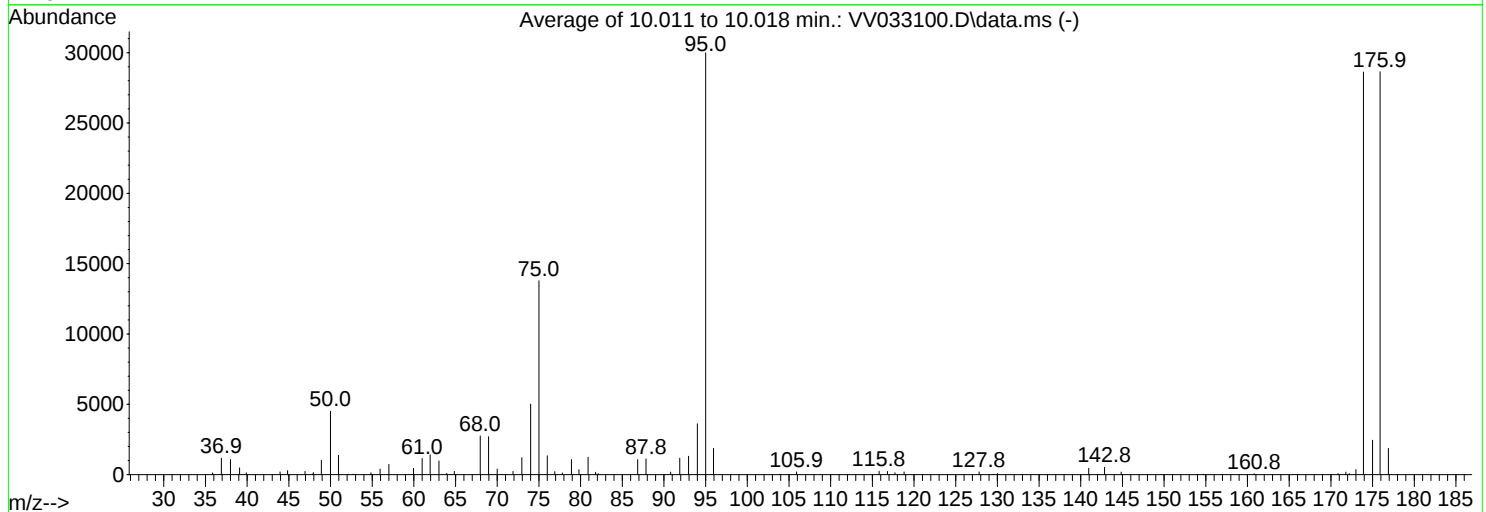


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120523\
Data File : VV033100.D
Acq On : 05 Dec 2023 10:39
Operator : SY/MD
Sample : BFB240
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB240

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis
Last Update : Wed Dec 06 01:18:11 2023

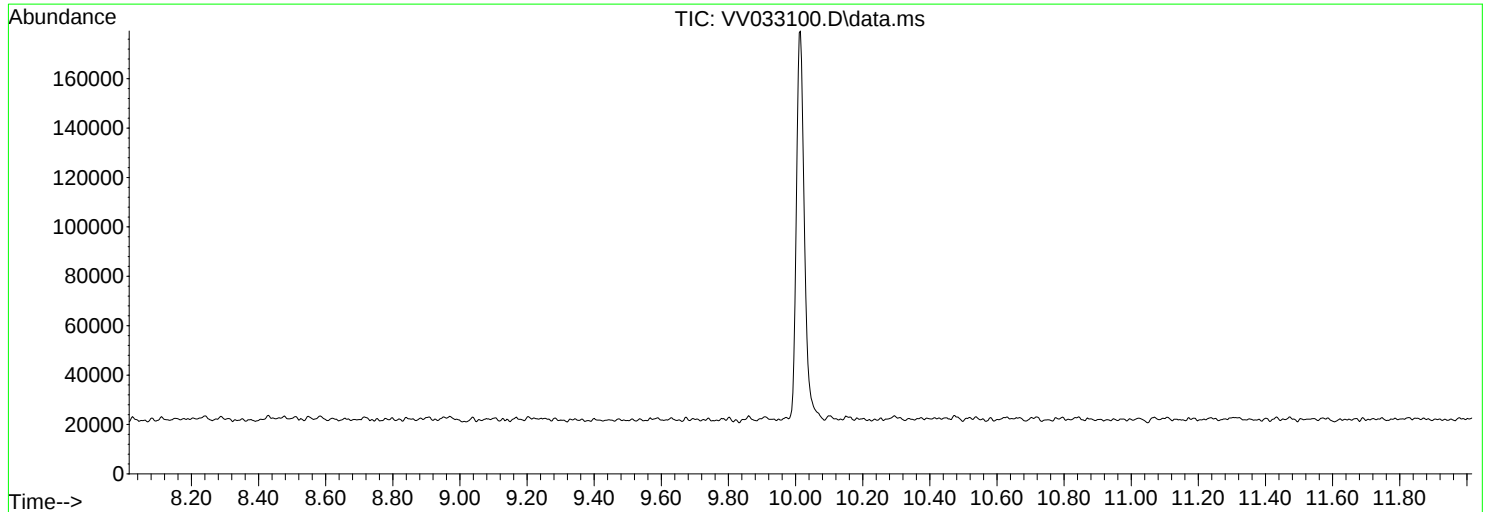

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	4502	PASS
75	95	30	80	46.0	13792	PASS
95	95	100	100	100.0	29987	PASS
96	95	5	9	6.2	1869	PASS
173	174	0.00	2	1.3	365	PASS
174	95	50	120	95.5	28624	PASS
175	174	5	9	8.6	2448	PASS
176	174	95	105	100.1	28645	PASS
177	176	5	10	6.5	1866	PASS

m/z	Abundance
35.80	123.0
39.10	118.0
39.90	22216.0
44.00	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.90	254.0
36.90	1170.0
38.00	1109.0
39.10	697.0
39.90	22552.0
44.00	407.0
44.90	276.0
47.00	237.0
47.80	138.0
48.00	140.0
48.90	1023.0
50.00	4708.0
51.00	1425.0
52.70	111.0
54.80	128.0
56.00	422.0
57.00	791.0
59.90	389.0
61.00	1200.0
62.00	1454.0
63.00	1070.0
64.80	284.0
67.90	2769.0
69.00	2925.0
70.00	419.0
71.90	193.0
73.00	1252.0
74.00	5039.0
75.00	14381.0
76.00	1381.0
77.00	227.0
77.80	104.0
78.90	1098.0
79.80	385.0
80.90	1352.0
81.80	262.0
86.90	1122.0
87.80	1128.0
90.80	171.0
91.90	1196.0
92.90	1361.0
94.00	3779.0
95.00	30536.0
96.00	1876.0
103.90	103.0
106.00	140.0
115.80	218.0
116.80	223.0
117.70	161.0
118.70	174.0
127.80	199.0
129.50	119.0
140.90	500.0
142.90	600.0
144.90	194.0
154.70	113.0
170.90	119.0
171.80	283.0
173.00	330.0
173.90	28568.0
175.00	2501.0
175.90	29240.0
176.90	1865.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.90	241.0
36.90	1241.0
38.00	1121.0
39.10	604.0
39.90	22400.0
43.90	375.0
44.90	299.0
46.90	224.0
47.90	159.0
48.90	1060.0
50.00	4601.0
50.90	1359.0
54.90	141.0
55.90	410.0
57.00	750.0
59.90	475.0
61.00	1158.0
61.90	1472.0
63.00	984.0
64.00	121.0
64.80	225.0
67.90	2775.0
69.00	2749.0
70.00	429.0
71.90	230.0
73.00	1252.0
74.00	5111.0
75.00	14135.0
76.00	1393.0
76.90	220.0
77.80	128.0
78.90	1139.0
79.80	357.0
80.90	1256.0
81.80	242.0
86.90	1072.0
87.90	1159.0
90.80	197.0
91.90	1222.0
93.00	1345.0
94.00	3665.0
95.00	30904.0
96.00	1936.0
105.80	138.0
106.10	135.0
115.80	266.0
116.80	249.0
117.70	142.0
118.80	194.0
127.80	203.0
130.00	121.0
141.00	464.0
142.90	532.0
144.90	199.0
160.80	104.0
170.80	110.0
171.80	275.0
173.00	382.0
173.90	29456.0
175.00	2503.0
175.90	29520.0
176.90	1954.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.90	253.0
36.90	1111.0
38.00	1002.0
39.10	488.0
39.90	22096.0
43.90	356.0
44.80	274.0
46.90	213.0
47.90	152.0
48.90	973.0
50.00	4198.0
50.90	1338.0
52.10	107.0
54.80	144.0
55.90	365.0
57.00	654.0
60.00	469.0
61.00	1085.0
61.90	1307.0
63.00	895.0
63.90	161.0
64.90	180.0
68.00	2729.0
68.90	2405.0
70.00	344.0
71.90	255.0
72.90	1114.0
74.00	4916.0
75.00	12861.0
76.00	1243.0
76.80	185.0
77.80	137.0
78.90	1017.0
79.80	305.0
80.90	1103.0
82.10	239.0
86.80	1030.0
87.90	1086.0
90.80	188.0
91.90	1093.0
92.90	1212.0
94.00	3404.0
95.00	28520.0
95.90	1796.0
105.80	158.0
115.80	248.0
116.80	228.0
117.70	124.0
118.90	225.0
127.80	190.0
130.00	127.0
141.00	418.0
142.80	436.0
144.80	159.0
160.80	111.0
172.20	234.0
173.00	384.0
173.90	27848.0
175.00	2341.0
175.90	27176.0
176.90	1780.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240