

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120525\
 Data File : VV039483.D
 Acq On : 05 Dec 2025 16:29
 Operator : SY/MD
 Sample : Q3756-12
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Dec 05 22:49:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	5671	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	5736	0.500	ug/L	0.02
12) 1,4-Dichlorobenzene-d4	11.197	152	2936	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.294	65	3377	0.592	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	118.000%
4) 1,2-Dichloroethane-d4	4.993	65	1821	0.482	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	96.000%
7) 1,2-Dichloropropane-d6	5.995	67	2072	0.428	ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	86.000%
8) Toluene-d8	7.253	98	3812	0.467	ug/L	0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	94.000%
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1445	0.530	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%
Target Compounds						
					Qvalue	
11) 1,1,2,2-Tetrachloroethane	9.556	83	682	0.119	ug/L #	1
14) 1,2-Dibromo-3-chloropr...	12.528	75	15	0.024	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120525\
Data File : VV039483.D
Acq On : 05 Dec 2025 16:29
Operator : SY/MD
Sample : Q3756-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Dec 05 22:49:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration




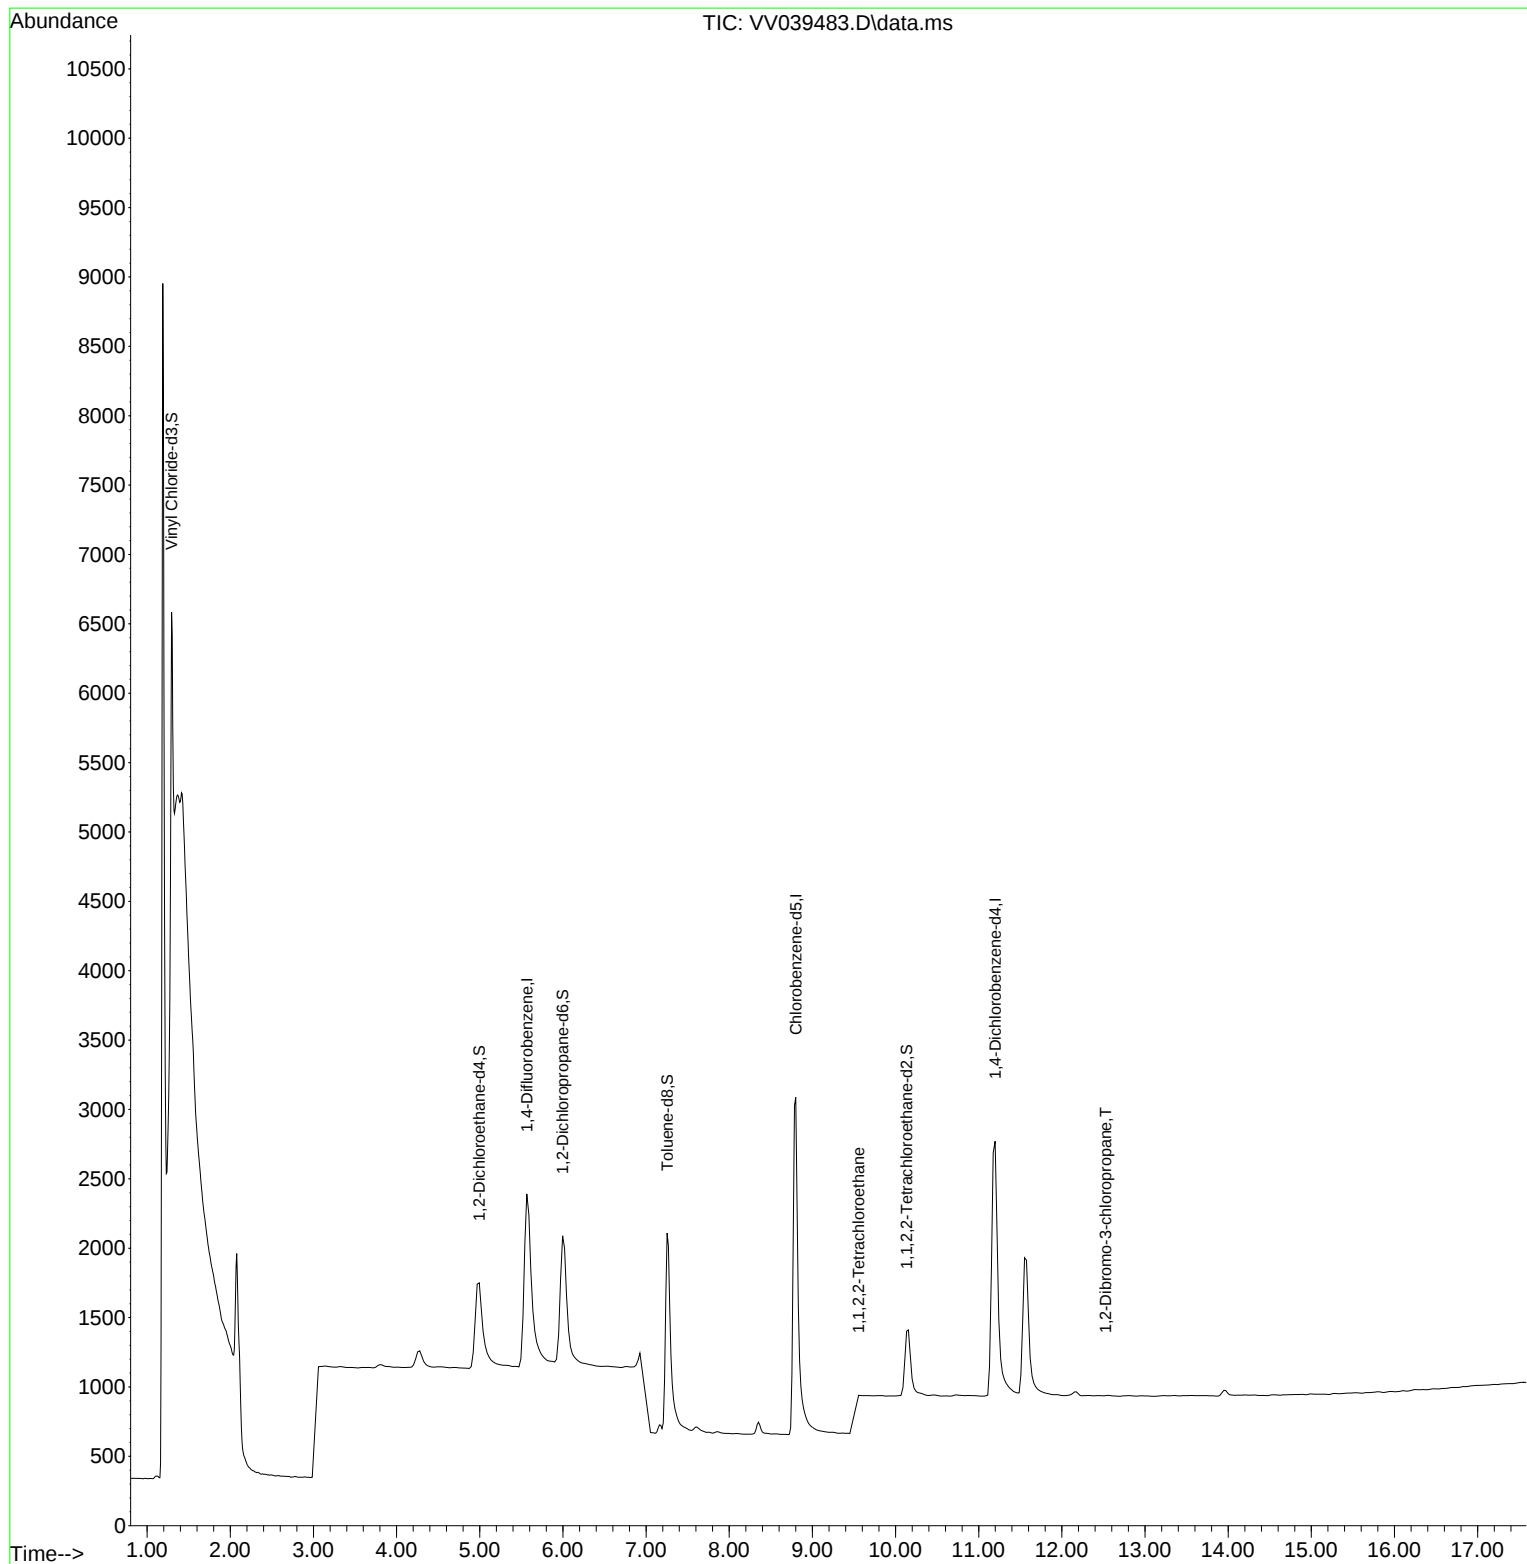


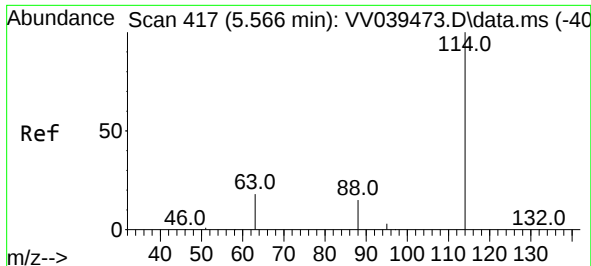

#1
 1,4-Difluorobenzene
 Concen: 0.500 ug/L
 RT: 5.566 min Scan# 417
 Delta R.T. -0.000 min
 Lab File: VV039483.D
 Acq: 05 Dec 2025 16:29




Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001


Tgt Ion:	114	Resp:	5671
Ion	Ratio	Lower	Upper
114	100		
63	20.3	15.0	22.4
88	15.4	12.0	18.0

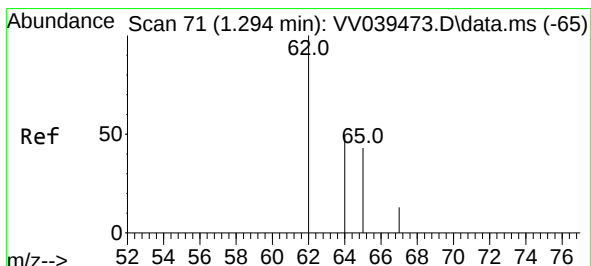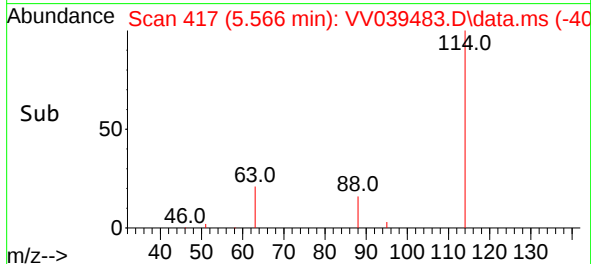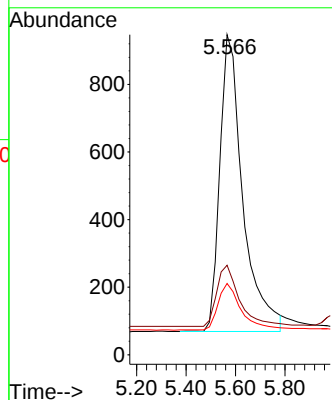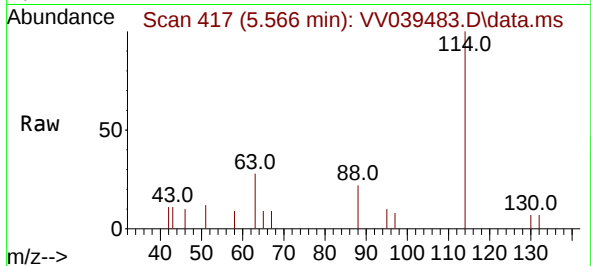

#2
 Vinyl Chloride-d3
 Concen: 0.592 ug/L
 RT: 1.294 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: VV039483.D
 Acq: 05 Dec 2025 16:29

Tgt Ion:	65	Resp:	3377
Ion	Ratio	Lower	Upper
65	100		
67	31.3	22.3	41.5


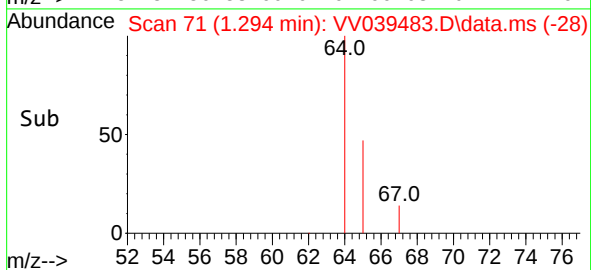
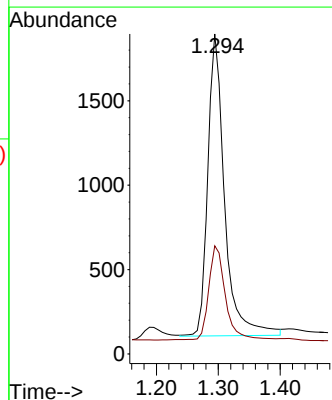
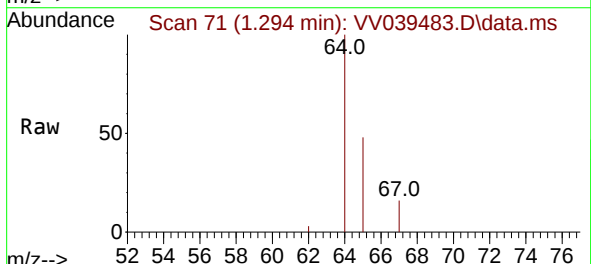


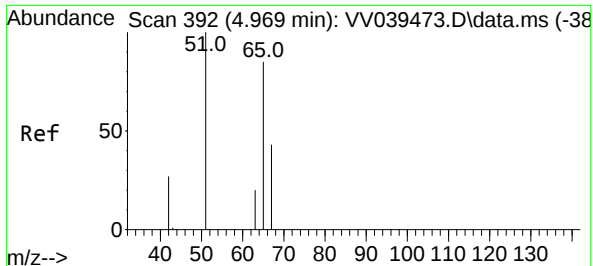

#4
1,2-Dichloroethane-d4
Concen: 0.482 ug/L
RT: 4.993 min Scan# 392
Delta R.T. 0.024 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29




Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Tgt Ion: 65 Resp: 1821
Ion Ratio Lower Upper
65 100
67 53.0 32.5 60.3
51 39.3 121.4 225.6#

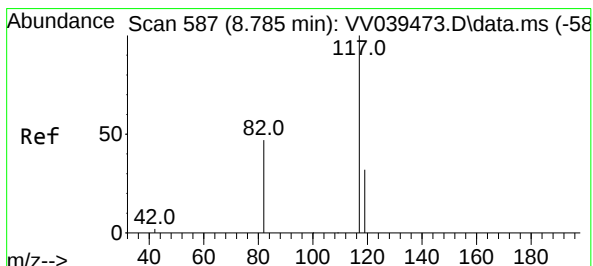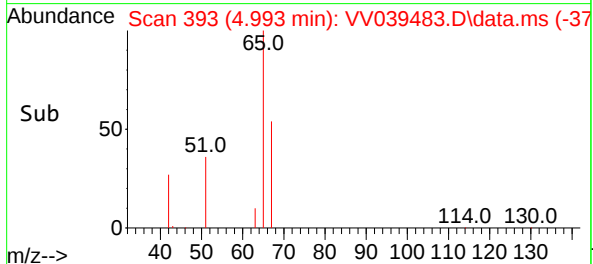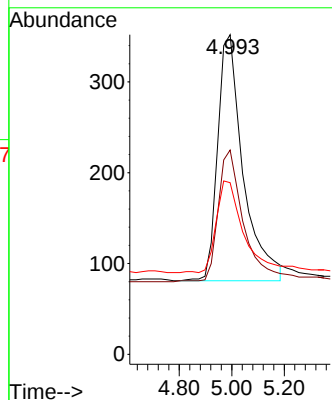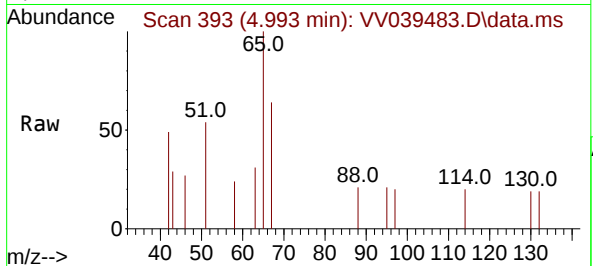

#5
Chlorobenzene-d5
Concen: 0.500 ug/L
RT: 8.800 min Scan# 588
Delta R.T. 0.015 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29

Tgt Ion:117 Resp: 5736
Ion Ratio Lower Upper
117 100
82 47.9 39.4 59.2
119 32.7 26.2 39.2


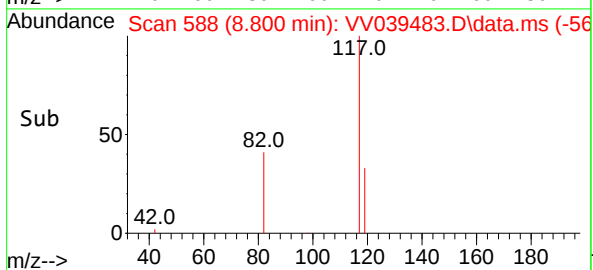
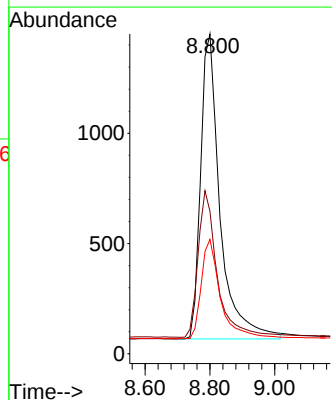
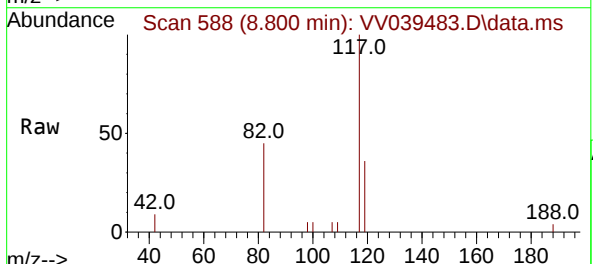


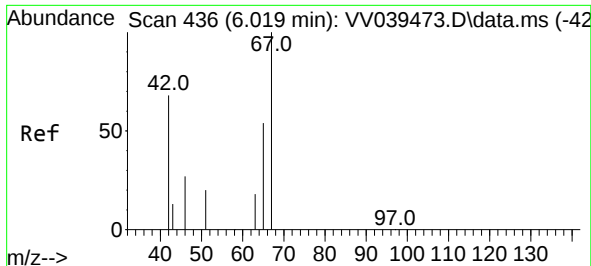

#7
1,2-Dichloropropane-d6
Concen: 0.428 ug/L
RT: 5.995 min Scan# 41
Delta R.T. -0.024 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29




Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Tgt Ion:	67	Resp:	2072
Ion	Ratio	Lower	Upper
67	100		
65	64.7	37.9	56.9#
46	45.7	27.4	41.0#
42	29.3	51.2	76.8#

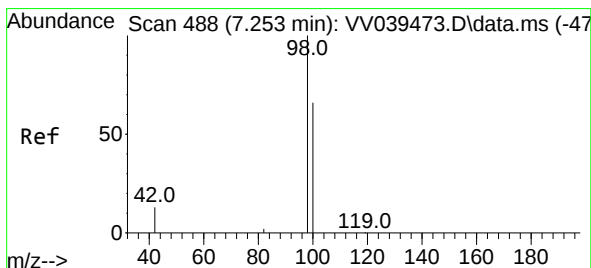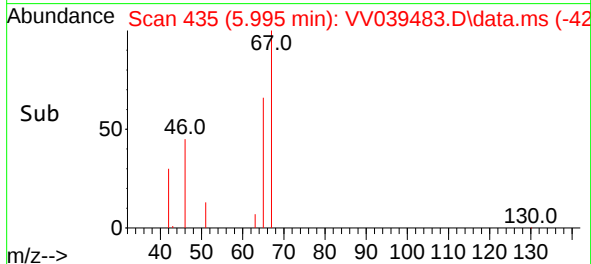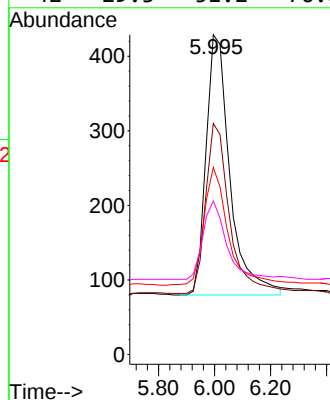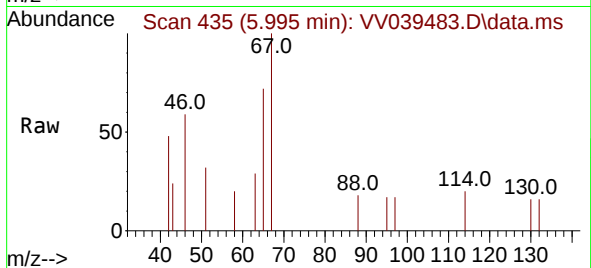

#8
Toluene-d8
Concen: 0.467 ug/L
RT: 7.253 min Scan# 488
Delta R.T. 0.015 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29

Tgt Ion:	98	Resp:	3812
Ion	Ratio	Lower	Upper
98	100		
100	61.1	44.5	82.7
42	10.5	10.1	18.7


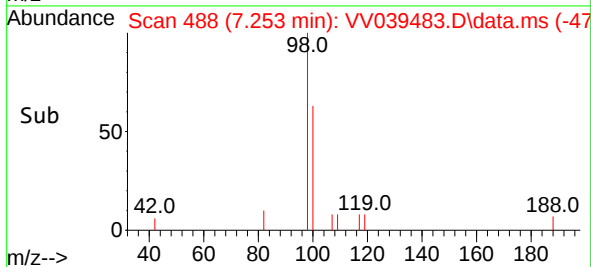
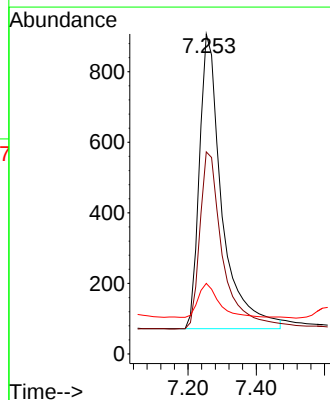
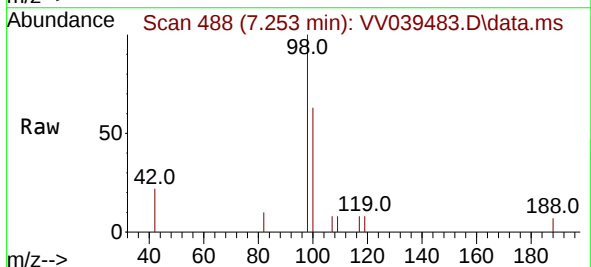


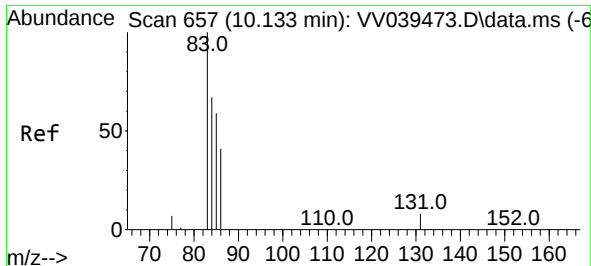

#10
1,1,2,2-Tetrachloroethane-d2
Concen: 0.530 ug/L
RT: 10.133 min Scan# 610
Delta R.T. -0.000 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29




Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Tgt Ion: 84 Resp: 1445
Ion Ratio Lower Upper
84 100
86 62.1 44.4 82.5

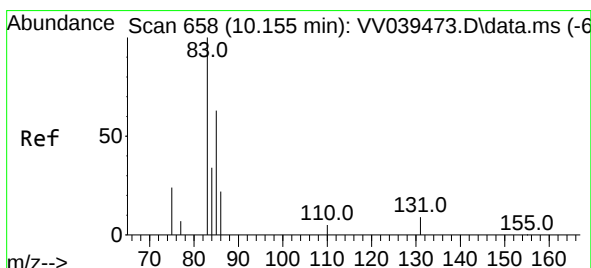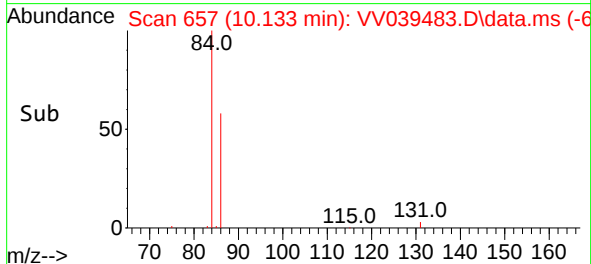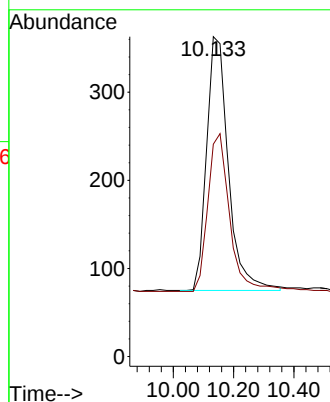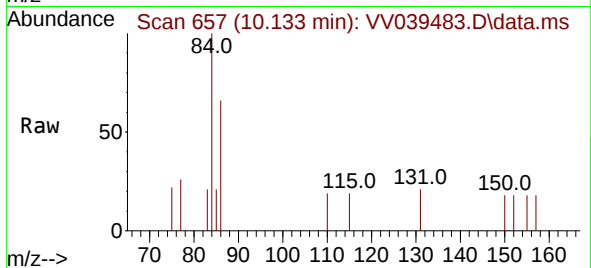

#11
1,1,2,2-Tetrachloroethane
Concen: 0.119 ug/L
RT: 9.556 min Scan# 631
Delta R.T. -0.599 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29

Tgt Ion: 83 Resp: 682
Ion Ratio Lower Upper
83 100
85 130.6 51.0 76.6#
131 171.8 8.6 12.8#


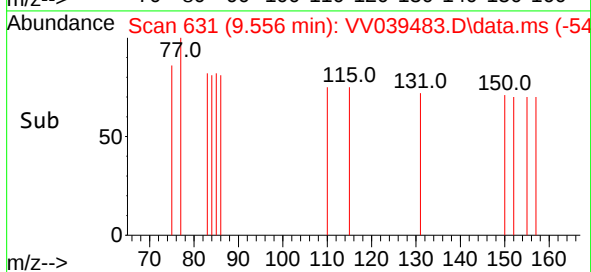
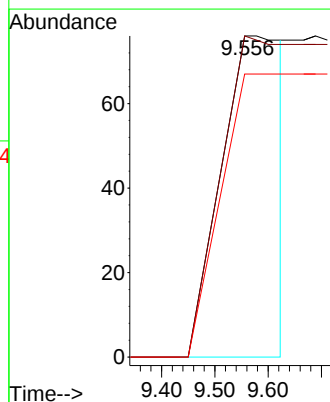
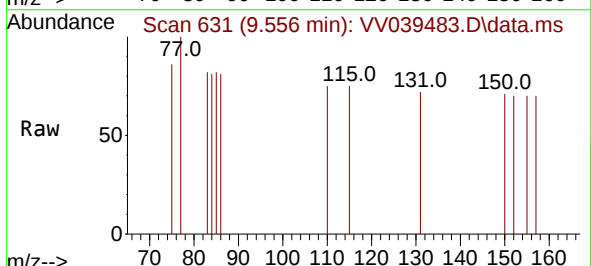


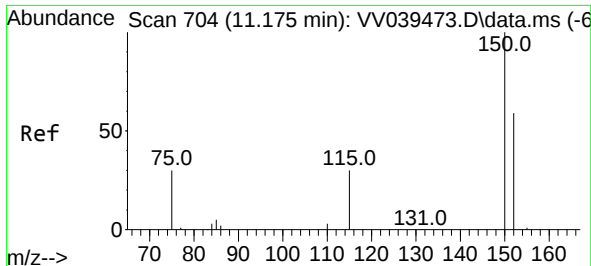

#12
1,4-Dichlorobenzene-d4
Concen: 0.500 ug/L
RT: 11.197 min Scan# 704
Delta R.T. 0.022 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:152 Resp: 2936
Ion Ratio Lower Upper
152 100
115 55.2 0.0 101.6
150 158.1 0.0 396.2

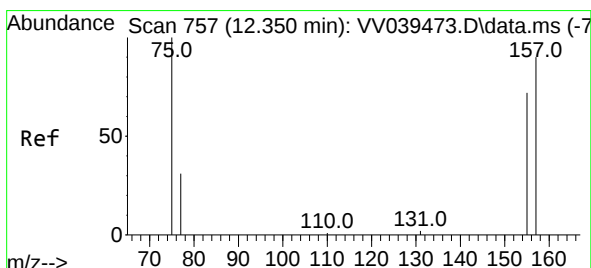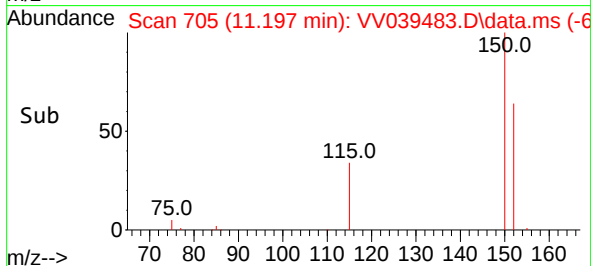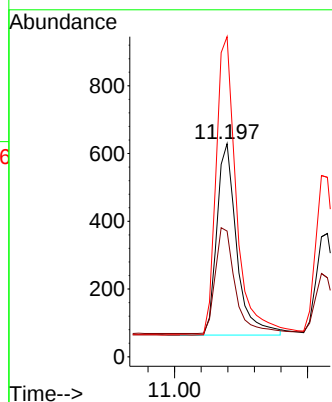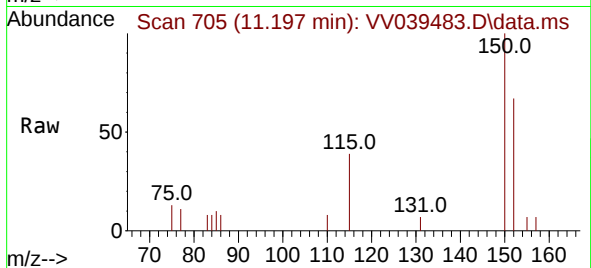

#14
1,2-Dibromo-3-chloropropane
Concen: 0.024 ug/L
RT: 12.528 min Scan# 765
Delta R.T. 0.177 min
Lab File: VV039483.D
Acq: 05 Dec 2025 16:29

Tgt Ion: 75 Resp: 15
Ion Ratio Lower Upper
75 100
157 77.1 67.8 101.6
155 75.9 61.9 92.9

